

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018025.D
 Acq On : 10 Nov 2023 13:16
 Operator : MA/JU
 Sample : 05091-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCK17

Quant Time: Nov 10 22:17:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 09 22:34:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	76683	20.000	ng/ul	0.00
20) Naphthalene-d8	10.686	136	310664	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	201751	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.321	188	457809	20.000	ng/ul	0.00
79) Chrysene-d12	21.451	240	438473	20.000	ng/ul	0.00
88) Perylene-d12	23.968	264	468624	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	7004	3.127	ng/uL	0.00
4) Pyridine-d5	3.687	84	36191	6.216	ng/ul	0.00
7) Phenol-d5	7.028	99	134841	18.711	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.210	67	83376	19.100	ng/ul	0.00
11) 2-Chlorophenol-d4	7.381	132	110167	19.107	ng/ul	0.00
15) 4-Methylphenol-d8	8.587	113	89612	15.504	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128	55644	20.001	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	62146	20.071	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.310	165	103649	18.687	ng/ul	0.00
31) 4-Chloroaniline-d4	10.869	131	132952	17.491	ng/ul	0.00
46) Dimethylphthalate-d6	13.963	166	371964	20.056	ng/ul	0.00
49) Acenaphthylene-d8	14.239	160	397962	20.015	ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143	39312	14.472	ng/ul	0.00
60) Fluorene-d10	15.539	176	312908	20.355	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.839	200	103	0.032	ng/ul	0.14
73) Anthracene-d10	17.421	188	505822	20.620	ng/ul	0.00
81) Pyrene-d10	19.674	212	662730	23.485	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.797	264	602098	22.105	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.063	94	11974	1.687	ng/ul	93
16) Acetophenone	8.722	105	61052	6.606	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018025.D
Acq On : 10 Nov 2023 13:16
Operator : MA/JU
Sample : 05091-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKI7

Quant Time: Nov 10 22:17:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 09 22:34:38 2023
Response via : Initial Calibration




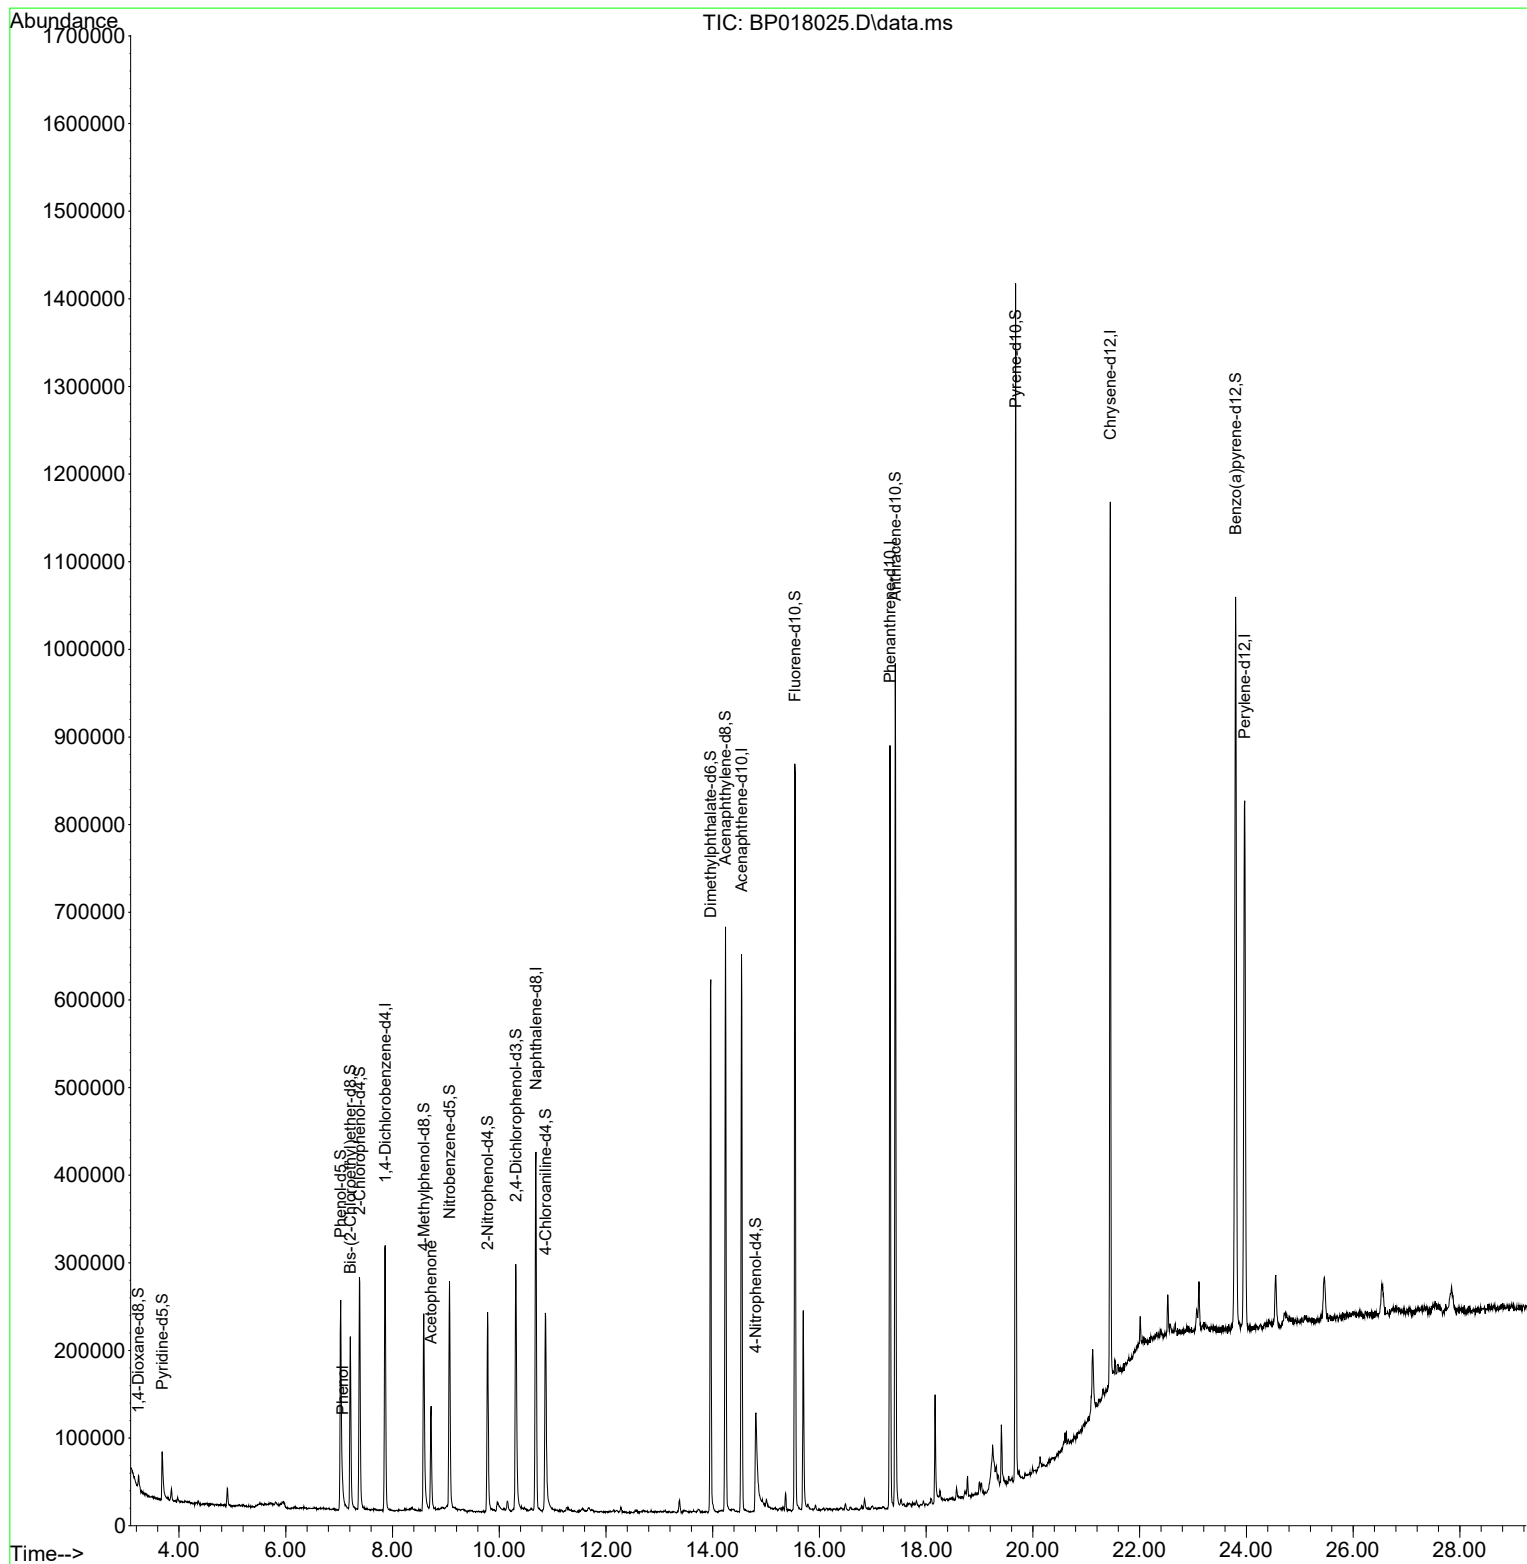


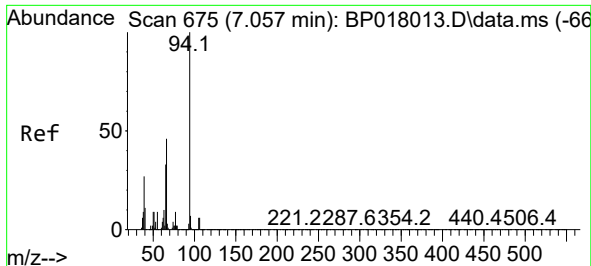

#8
Phenol
Concen: 1.687 ng/ul
RT: 7.063 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP018025.D
Acq: 10 Nov 2023 13:16

Instrument :
BNA_P
ClientSampleId :
DCKI7

Tgt Ion: 94 Resp: 11974
Ion Ratio Lower Upper
94 100
65 33.3 26.5 39.7
66 54.2 37.0 55.6

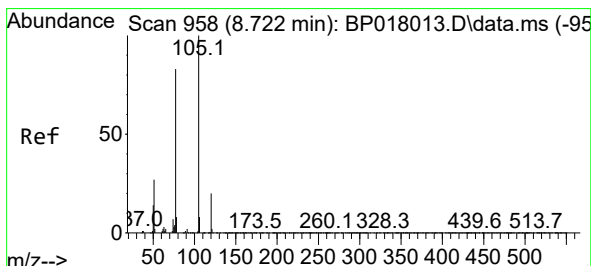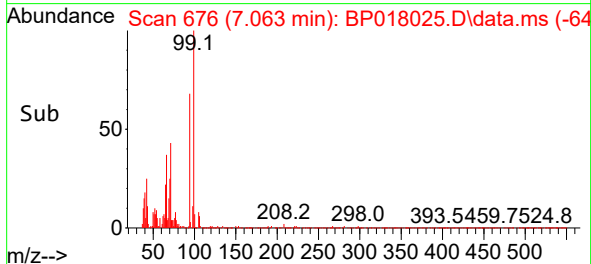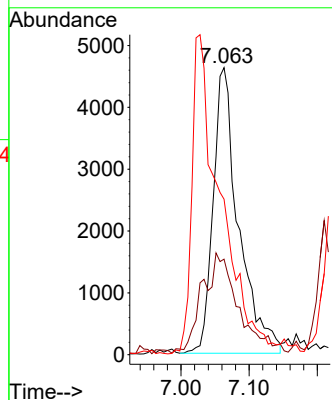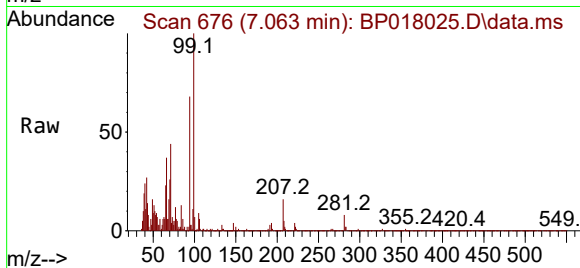

#16
Acetophenone
Concen: 6.606 ng/ul
RT: 8.722 min Scan# 958
Delta R.T. -0.000 min
Lab File: BP018025.D
Acq: 10 Nov 2023 13:16

Tgt Ion: 105 Resp: 61052
Ion Ratio Lower Upper
105 100
77 84.0 68.2 102.4
51 28.0 24.1 36.1

