




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018005.D
Acq On : 10 Nov 2023 00:38
Operator : MA/JU
Sample : 05082-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH325

Manual IntegrationsAPPROVED

Quant Time: Nov 10 01:11:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 09 22:34:38 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2023
Supervised By :mohammad ahmed 11/15/2023

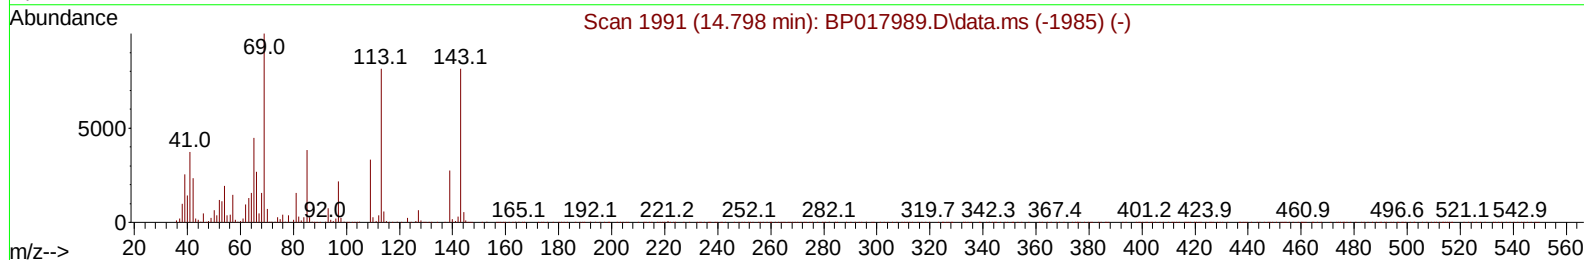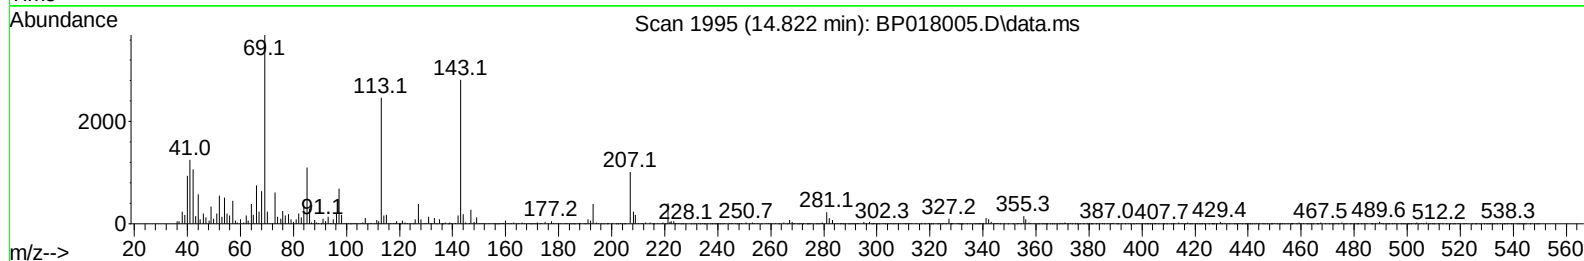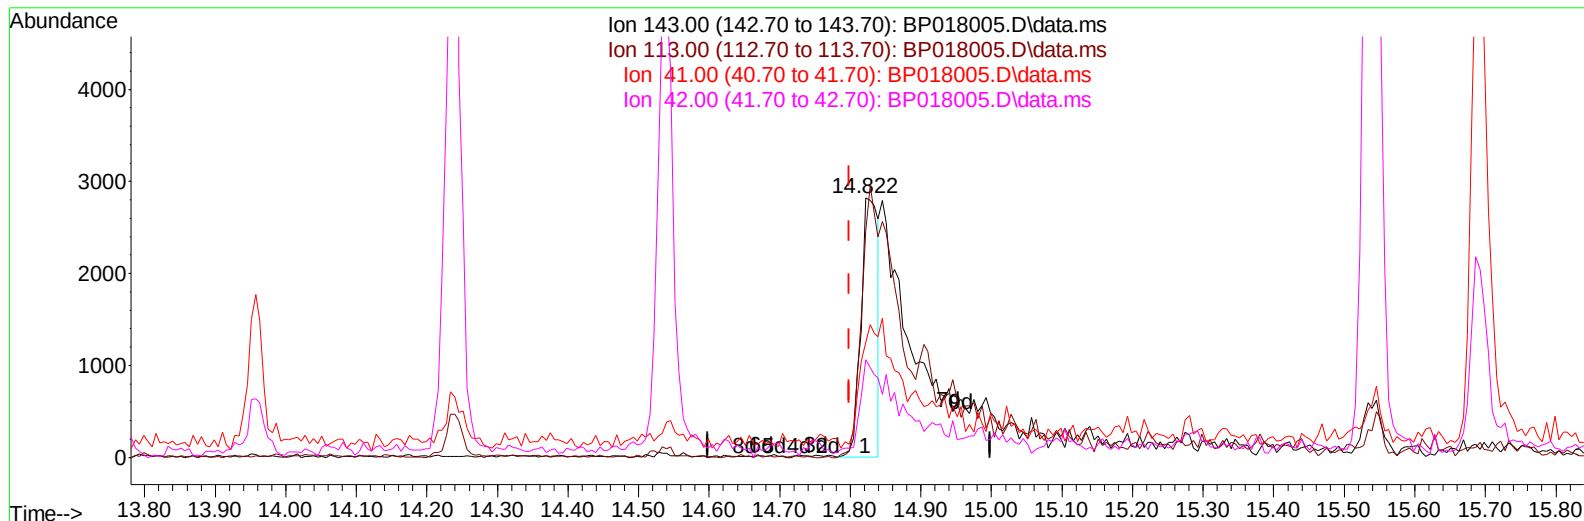

TIC: BP018005.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.822min (+ 0.024) 1.99 ng/ul

response 4788

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	100.40	87.59
41.00	46.90	44.33
42.00	29.70	37.77#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018005.D
Acq On : 10 Nov 2023 00:38
Operator : MA/JU
Sample : 05082-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH325

Manual IntegrationsAPPROVED

Quant Time: Nov 10 01:11:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 09 22:34:38 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2023
Supervised By :mohammad ahmed 11/15/2023

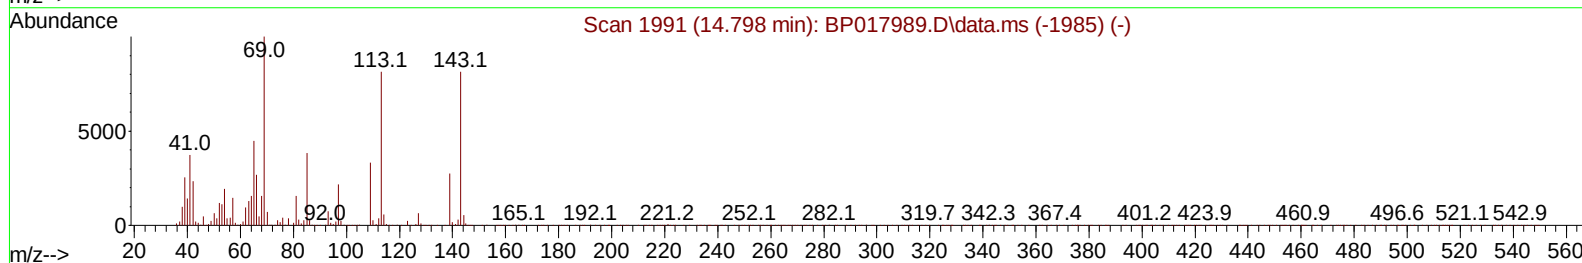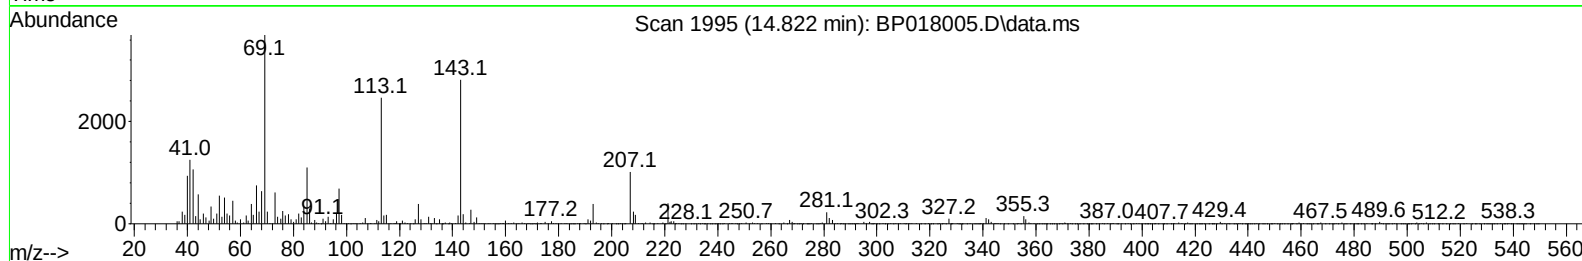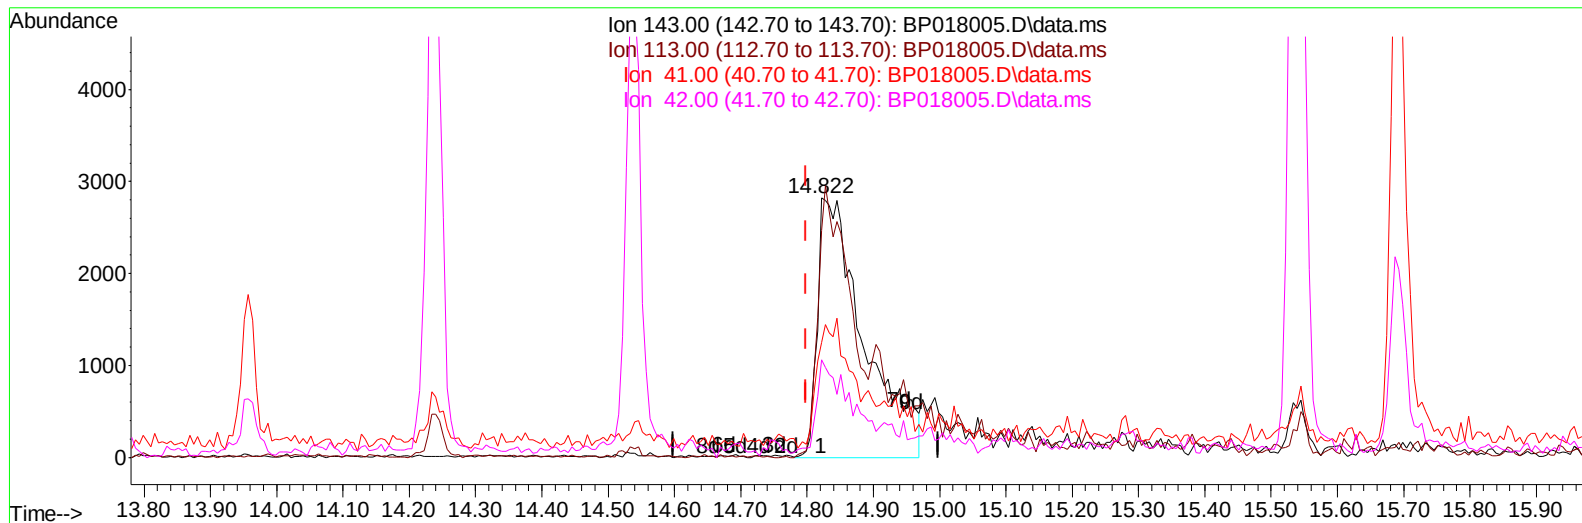

TIC: BP018005.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.822min (+ 0.024) 5.73 ng/ul m

response 13795

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	100.40	87.59
41.00	46.90	44.33
42.00	29.70	37.77#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018005.D
 Acq On : 10 Nov 2023 00:38
 Operator : MA/JU
 Sample : 05082-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH325

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2023
 Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 10 01:12:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 09 22:34:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	67736	20.000	ng/ul	0.00
20) Naphthalene-d8	10.687	136	278511	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	178759	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.316	188	414683	20.000	ng/ul	0.00
79) Chrysene-d12	21.445	240	401141	20.000	ng/ul	0.00
88) Perylene-d12	23.957	264	449839	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	8028	4.057	ng/uL	0.00
4) Pyridine-d5	3.687	84	36589	7.115	ng/ul	0.00
7) Phenol-d5	7.034	99	46372	7.285	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.210	67	130473	33.837	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	131642	25.847	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	84848	16.619	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128	83024	33.288	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	88962	32.049	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.310	165	142605	28.678	ng/ul	0.00
31) 4-Chloroaniline-d4	10.863	131	172101	25.256	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	598403	36.415	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	605875	34.391	ng/ul	0.00
54) 4-Nitrophenol-d4	14.822	143	13795m	5.732	ng/ul	0.02
60) Fluorene-d10	15.539	176	498342	36.588	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	100771	34.802	ng/ul	0.00
73) Anthracene-d10	17.422	188	868745	39.099	ng/ul	0.00
81) Pyrene-d10	19.669	212	1094185	42.382	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.786	264	1047090	40.047	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018005.D
Acq On : 10 Nov 2023 00:38
Operator : MA/JU
Sample : 05082-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH325

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2023
Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 10 01:12:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 09 22:34:38 2023
Response via : Initial Calibration

