

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP017994.D
 Acq On : 09 Nov 2023 18:24
 Operator : MA/JU
 Sample : PB156741BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK741

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	33	rVB2	23292	33063	1.76%	0.176%
2	3.681	97	101	114	rBV	225381	366892	19.50%	1.953%
3	3.981	149	152	156	rVB4	6220	6606	0.35%	0.035%
4	4.516	242	243	246	rBV3	2396	2039	0.11%	0.011%
5	4.758	282	284	286	rBV3	1851	1889	0.10%	0.010%
6	6.152	519	521	524	rVB4	2486	2350	0.12%	0.013%
7	6.546	586	588	594	rVB7	1009	1916	0.10%	0.010%
8	7.034	664	671	690	rBV	235098	460453	24.48%	2.451%
9	7.216	696	702	721	rVB	211801	345186	18.35%	1.838%
10	7.387	725	731	749	rBV	301184	506350	26.92%	2.696%
11	7.863	805	812	825	rBV	250902	426582	22.68%	2.271%
12	8.057	842	845	848	rBV5	1447	1960	0.10%	0.010%
13	8.587	929	935	954	rBV	290769	570437	30.32%	3.037%
14	9.075	1006	1018	1028	rBV	268173	473807	25.19%	2.523%
15	9.510	1089	1092	1095	rBV5	2287	2581	0.14%	0.014%
16	9.787	1130	1139	1149	rBV	236541	417822	22.21%	2.224%
17	9.875	1152	1154	1158	rVB5	2043	2246	0.12%	0.012%
18	10.316	1221	1229	1245	rBV	276671	556974	29.61%	2.965%
19	10.687	1285	1292	1303	rBV	334307	570099	30.30%	3.035%
20	10.869	1315	1323	1347	rBV	268832	595804	31.67%	3.172%
21	11.022	1347	1349	1352	rVB4	2469	2646	0.14%	0.014%
22	11.093	1358	1361	1365	rVB5	1705	2198	0.12%	0.012%
23	11.269	1389	1391	1396	rBV6	1418	1916	0.10%	0.010%
24	11.622	1446	1451	1454	rBV7	1502	2987	0.16%	0.016%
25	12.198	1547	1549	1553	rBV5	1445	1896	0.10%	0.010%
26	12.304	1563	1567	1574	rVB9	3289	6933	0.37%	0.037%
27	12.916	1668	1671	1674	rVB5	1610	2114	0.11%	0.011%
28	13.381	1744	1750	1756	rVB7	5089	9652	0.51%	0.051%
29	13.504	1767	1771	1776	rVB8	1516	2091	0.11%	0.011%
30	13.769	1813	1816	1820	rVB6	1661	2325	0.12%	0.012%
31	13.963	1842	1849	1866	rBV	639131	951916	50.60%	5.068%
32	14.239	1889	1896	1908	rBV	696826	1026363	54.56%	5.464%
33	14.539	1941	1947	1955	rVV	509752	756913	40.23%	4.030%
34	14.804	1986	1992	2013	rBV2	114109	371974	19.77%	1.980%
35	15.245	2063	2067	2069	rBV4	1588	2340	0.12%	0.012%
36	15.369	2082	2088	2096	rVV2	36558	61368	3.26%	0.327%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP017994.D
 Acq On : 09 Nov 2023 18:24
 Operator : MA/JU
 Sample : PB156741BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK741

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

37	15.545	2111	2118	2132	rBV	868939	1259066	66.93%	6.703%
38	15.692	2135	2143	2156	rBV	278753	461005	24.51%	2.454%
39	16.128	2213	2217	2224	rVB9	1860	3101	0.16%	0.017%
40	16.545	2285	2288	2291	rVB4	1814	2228	0.12%	0.012%
41	16.980	2360	2362	2367	rVV6	2752	4557	0.24%	0.024%
42	17.110	2381	2384	2385	rBV2	2112	2405	0.13%	0.013%
43	17.322	2413	2420	2431	rBV	672951	962888	51.18%	5.126%
44	17.422	2431	2437	2453	rVV2	986518	1435952	76.33%	7.645%
45	17.657	2475	2477	2482	rVB6	1325	1920	0.10%	0.010%
46	18.186	2563	2567	2570	rBV5	4127	7165	0.38%	0.038%
47	18.263	2577	2580	2585	rVB3	3801	5282	0.28%	0.028%
48	19.245	2744	2747	2752	rVB5	12566	14950	0.79%	0.080%
49	19.322	2756	2760	2763	rVB3	10649	16233	0.86%	0.086%
50	19.674	2814	2820	2826	rBV	1375533	1730753	92.00%	9.214%
51	19.733	2826	2830	2845	rVB	60467	138784	7.38%	0.739%
52	20.598	2975	2977	2980	rVB	16596	13795	0.73%	0.073%
53	21.451	3117	3122	3131	rBV	759956	1079887	57.40%	5.749%
54	23.792	3513	3520	3530	rVB2	949725	1881245	100.00%	10.016%
55	23.957	3542	3548	3564	rVB	544461	1211192	64.38%	6.448%




Sum of corrected areas: 18783096

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP017994.D
Acq On : 09 Nov 2023 18:24
Operator : MA/JU
Sample : PB156741BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK741

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

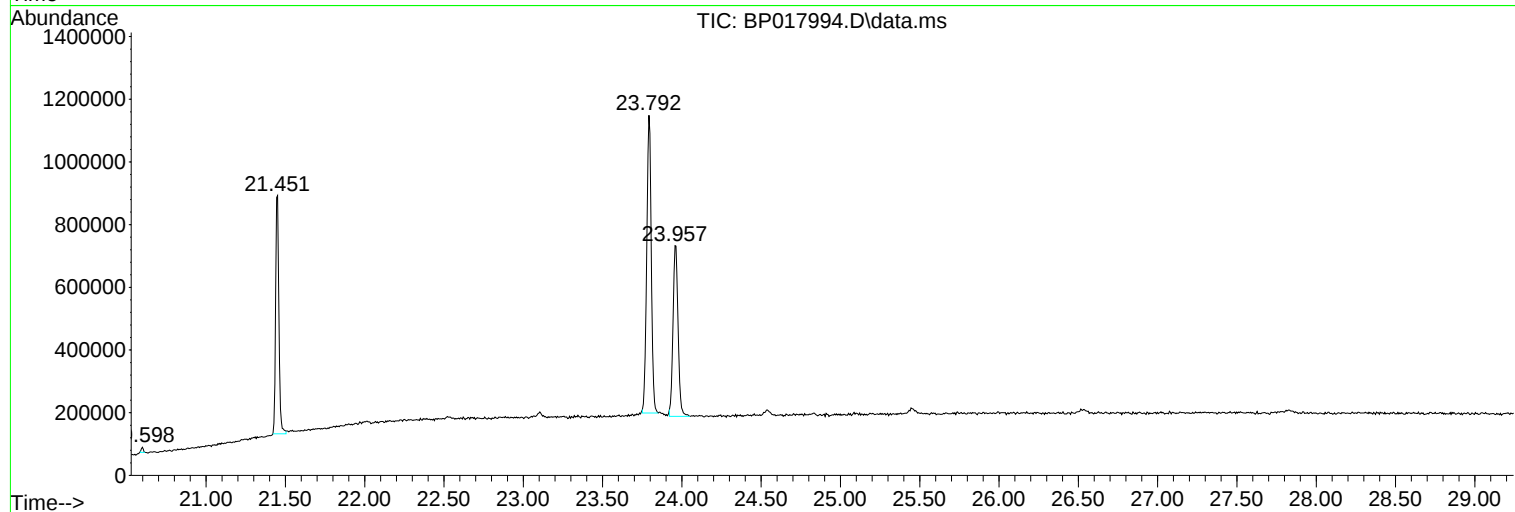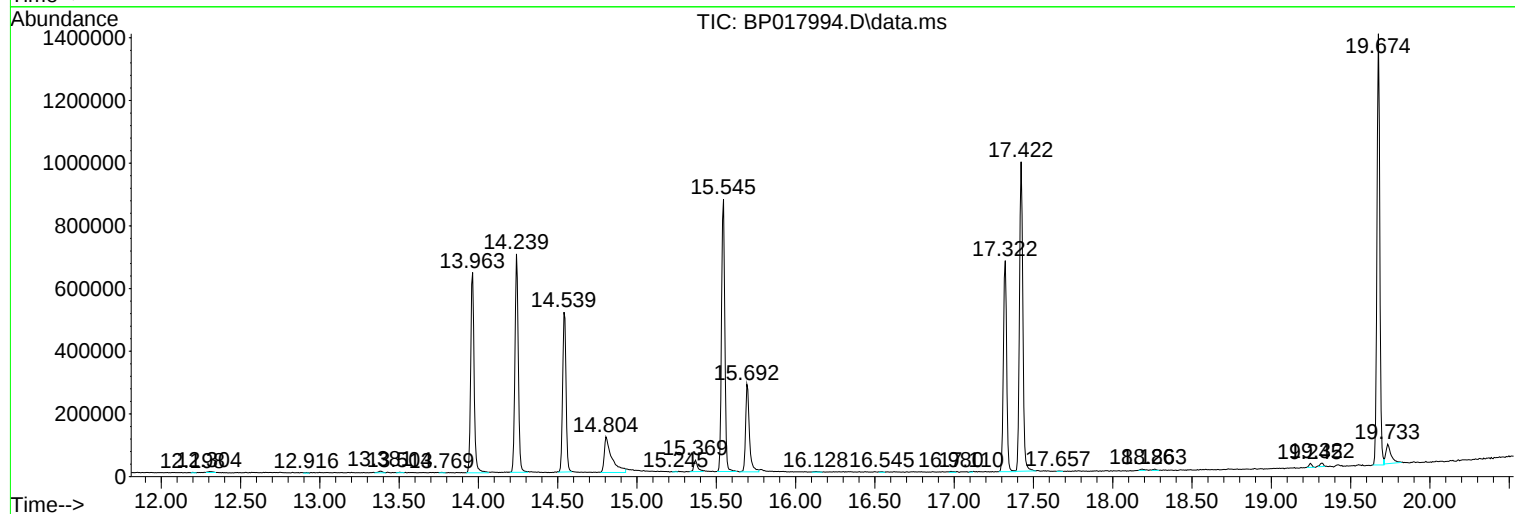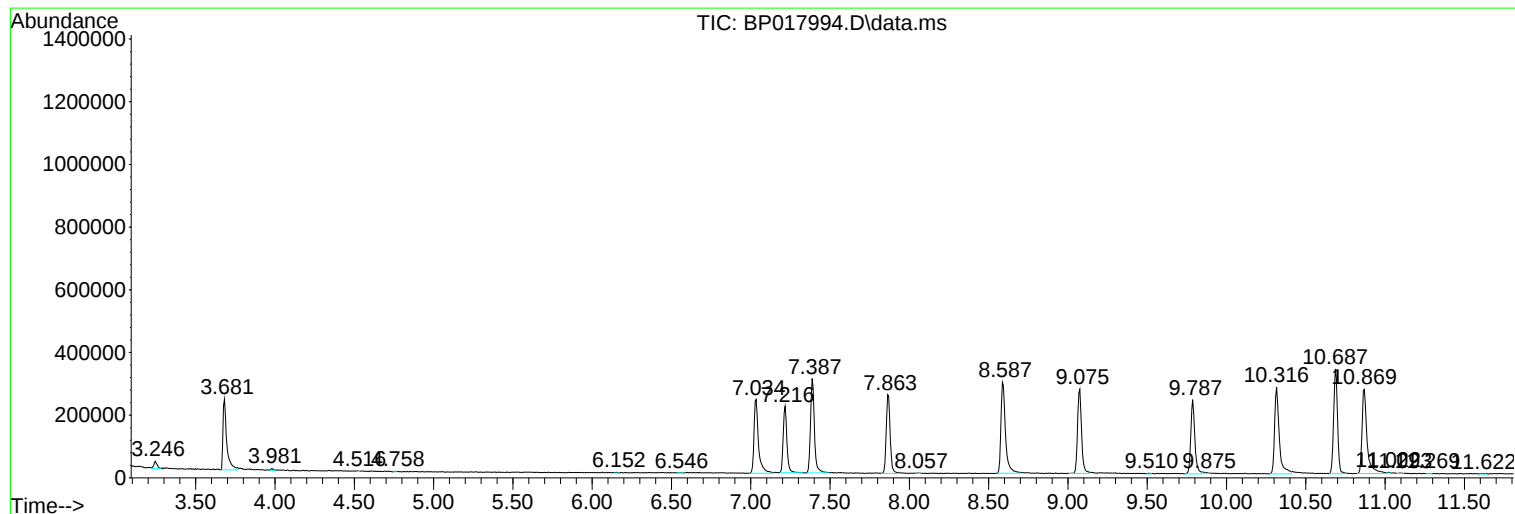

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP017994.D
Acq On : 09 Nov 2023 18:24
Operator : MA/JU
Sample : PB156741BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK741










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Phenol, 4,4'-(1-methylethyl... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
19.733	2.57 ng/ul	138784	Chrysene-d12	21.451

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenol, 4,4'-(1-methylethylidene...	228	C15H16O2	000080-05-7	91
2			Phenol, 4,4'-(1-methylethylidene...	228	C15H16O2	000080-05-7	87
3			Phenol, 4,4'-(1-methylethylidene...	228	C15H16O2	000080-05-7	87
4			Phenol, 4,4'-(1-methylethylidene...	228	C15H16O2	000080-05-7	87
5			3,4,6-Trichloro-guaiacol	226	C7H5Cl3O2	060712-44-9	64

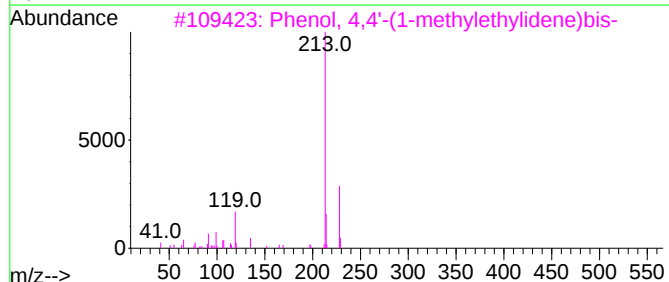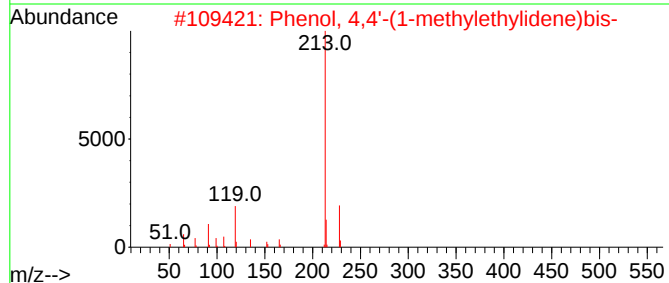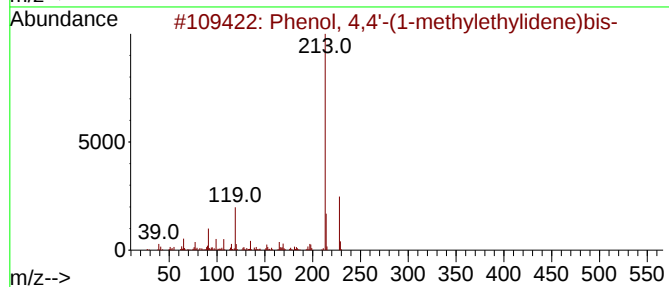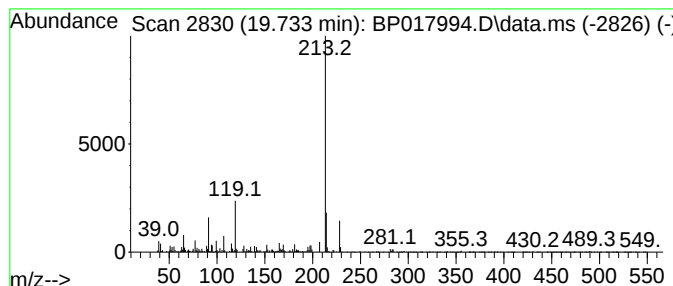

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP017994.D
Acq On : 09 Nov 2023 18:24
Operator : MA/JU
Sample : PB156741BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK741

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Phenol, 4,4'-(1...	19.733	2.6	ng/ul	138784	5	21.451	1079890	20.0