

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP017997.D
 Acq On : 09 Nov 2023 20:07
 Operator : MA/JU
 Sample : PB156742BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK742

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	24	27	33	rVB	23451	30024	1.50%	0.146%
2	3.681	97	101	116	rBV	230859	378570	18.87%	1.844%
3	3.975	149	151	158	rVB6	6276	9783	0.49%	0.048%
4	4.028	158	160	165	rBV5	2621	3645	0.18%	0.018%
5	5.081	337	339	342	rBV4	1595	2065	0.10%	0.010%
6	6.722	616	618	621	rVB4	2409	2367	0.12%	0.012%
7	7.028	664	670	686	rBV	267065	502940	25.07%	2.449%
8	7.216	695	702	714	rBV	235125	374155	18.65%	1.822%
9	7.387	725	731	743	rBV	323245	524736	26.16%	2.555%
10	7.863	806	812	822	rBV	251884	413585	20.62%	2.014%
11	8.587	928	935	958	rBV	327678	633588	31.59%	3.085%
12	8.728	958	959	964	rVB5	2836	2884	0.14%	0.014%
13	9.069	1008	1017	1034	rBV	291457	525690	26.21%	2.560%
14	9.234	1044	1045	1051	rVB6	2133	3441	0.17%	0.017%
15	9.293	1051	1055	1058	rBV6	1966	2788	0.14%	0.014%
16	9.787	1131	1139	1154	rBV	261093	471044	23.48%	2.294%
17	10.181	1203	1206	1210	rVB6	2009	2541	0.13%	0.012%
18	10.316	1221	1229	1247	rBV	303288	627102	31.27%	3.054%
19	10.687	1284	1292	1306	rBV	345587	578416	28.84%	2.817%
20	10.863	1315	1322	1338	rBV	278686	613429	30.58%	2.987%
21	11.087	1357	1360	1363	rVB5	2001	2663	0.13%	0.013%
22	11.698	1459	1464	1466	rBV5	1175	2206	0.11%	0.011%
23	11.863	1490	1492	1495	rBV4	2229	2199	0.11%	0.011%
24	12.304	1561	1567	1576	rBV10	4561	11338	0.57%	0.055%
25	13.375	1745	1749	1755	rBV7	5396	9681	0.48%	0.047%
26	13.492	1764	1769	1770	rBV5	2255	2871	0.14%	0.014%
27	13.963	1842	1849	1859	rBV	748154	1113328	55.51%	5.422%
28	14.239	1889	1896	1909	rBV	794932	1161615	57.91%	5.657%
29	14.539	1940	1947	1958	rVV	536749	803090	40.04%	3.911%
30	14.804	1985	1992	2009	rBV	140742	414275	20.65%	2.017%
31	15.369	2082	2088	2098	rBV	22817	40177	2.00%	0.196%
32	15.539	2111	2117	2132	rBV	1007283	1480884	73.83%	7.211%
33	15.692	2137	2143	2155	rBV	347396	530759	26.46%	2.585%
34	15.786	2157	2159	2162	rVB4	6813	6598	0.33%	0.032%
35	15.939	2183	2185	2189	rVB5	2020	2859	0.14%	0.014%
36	15.981	2189	2192	2195	rVV5	1718	2763	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP017997.D
 Acq On : 09 Nov 2023 20:07
 Operator : MA/JU
 Sample : PB156742BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK742

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

37	16.034	2199	2201	2206	rVB5	2139	2733	0.14%	0.013%
38	16.333	2249	2252	2255	rVB5	2840	3059	0.15%	0.015%
39	16.628	2300	2302	2305	rVB4	2092	2029	0.10%	0.010%
40	16.675	2307	2310	2313	rBV5	1605	2345	0.12%	0.011%
41	16.980	2357	2362	2366	rBV8	2889	4968	0.25%	0.024%
42	17.110	2380	2384	2386	rBV5	2629	3520	0.18%	0.017%
43	17.322	2413	2420	2431	rVV	707296	1033052	51.50%	5.031%
44	17.422	2431	2437	2453	rVV	1185370	1682262	83.87%	8.192%
45	17.869	2511	2513	2516	rVB4	2348	2444	0.12%	0.012%
46	18.028	2538	2540	2544	rBV5	2140	2572	0.13%	0.013%
47	18.186	2561	2567	2572	rBV10	5694	13438	0.67%	0.065%
48	18.263	2577	2580	2585	rVB3	4790	7841	0.39%	0.038%
49	18.298	2585	2586	2591	rBV5	2595	3628	0.18%	0.018%
50	19.239	2743	2746	2752	rVB4	14389	20359	1.02%	0.099%
51	19.316	2756	2759	2763	rVB2	12089	15836	0.79%	0.077%
52	19.416	2772	2776	2780	rBV7	8108	13523	0.67%	0.066%
53	19.674	2814	2820	2826	rBV	1512702	1995731	99.50%	9.719%
54	19.733	2826	2830	2841	rVB3	25640	69077	3.44%	0.336%
55	21.445	3116	3121	3133	rBV	840259	1164082	58.04%	5.669%
56	23.792	3513	3520	3532	rVB2	978831	2005761	100.00%	9.767%
57	23.957	3541	3548	3561	rVB	554098	1196833	59.67%	5.828%




Sum of corrected areas: 20535192

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP017997.D
Acq On : 09 Nov 2023 20:07
Operator : MA/JU
Sample : PB156742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK742

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

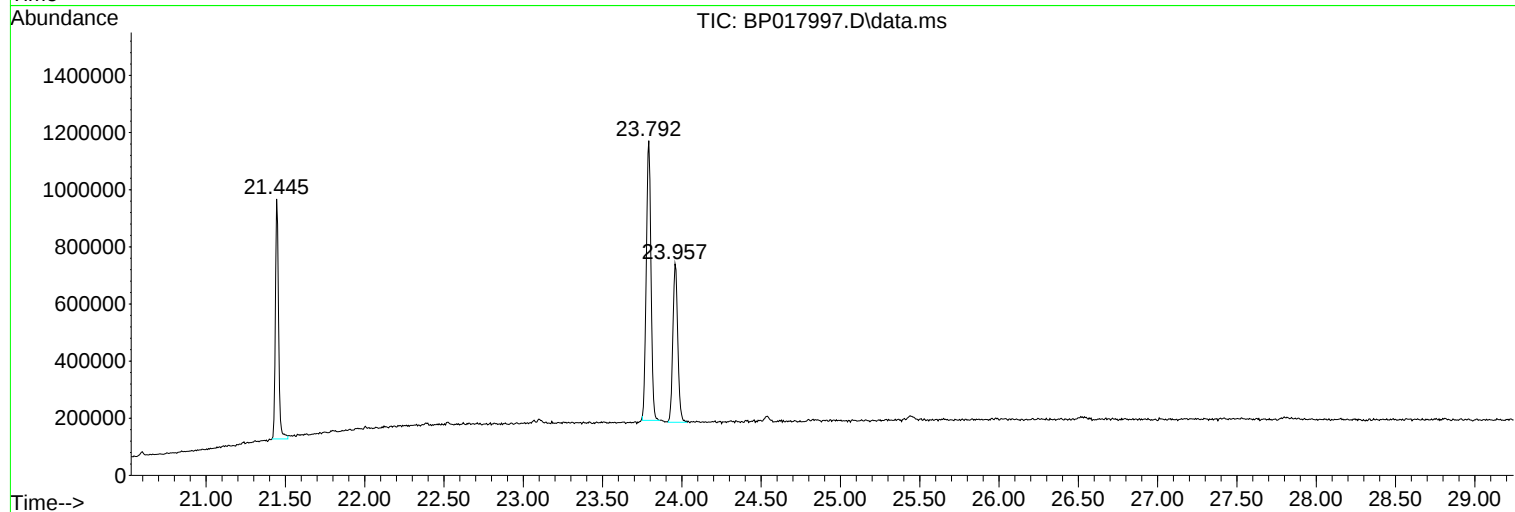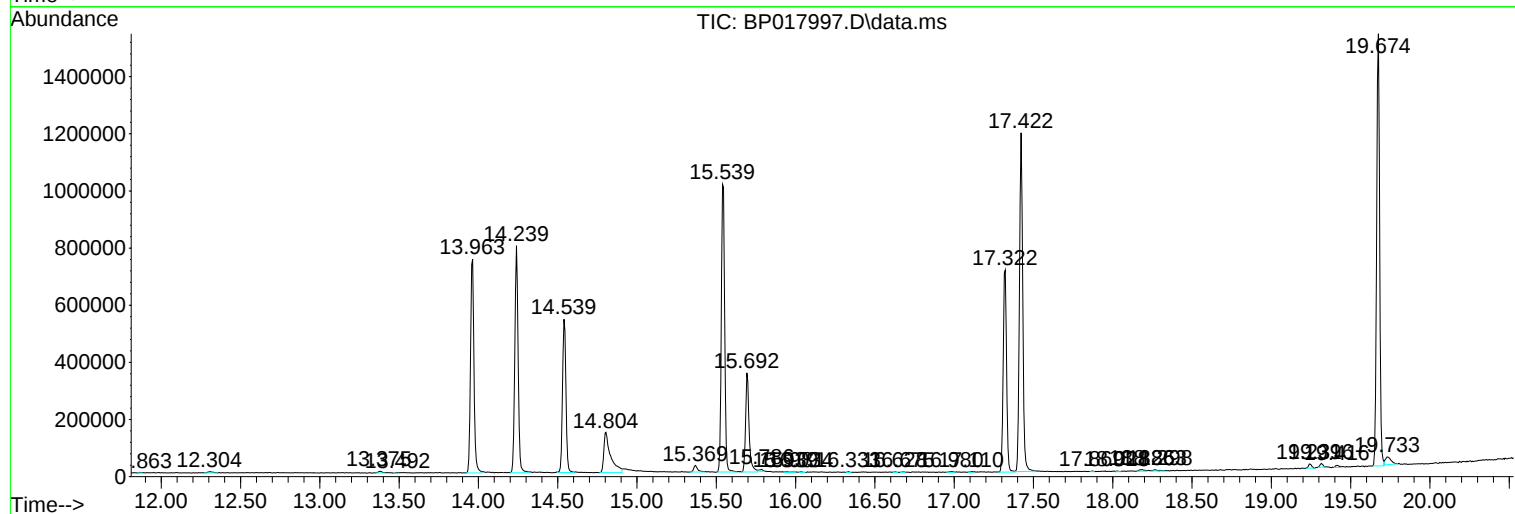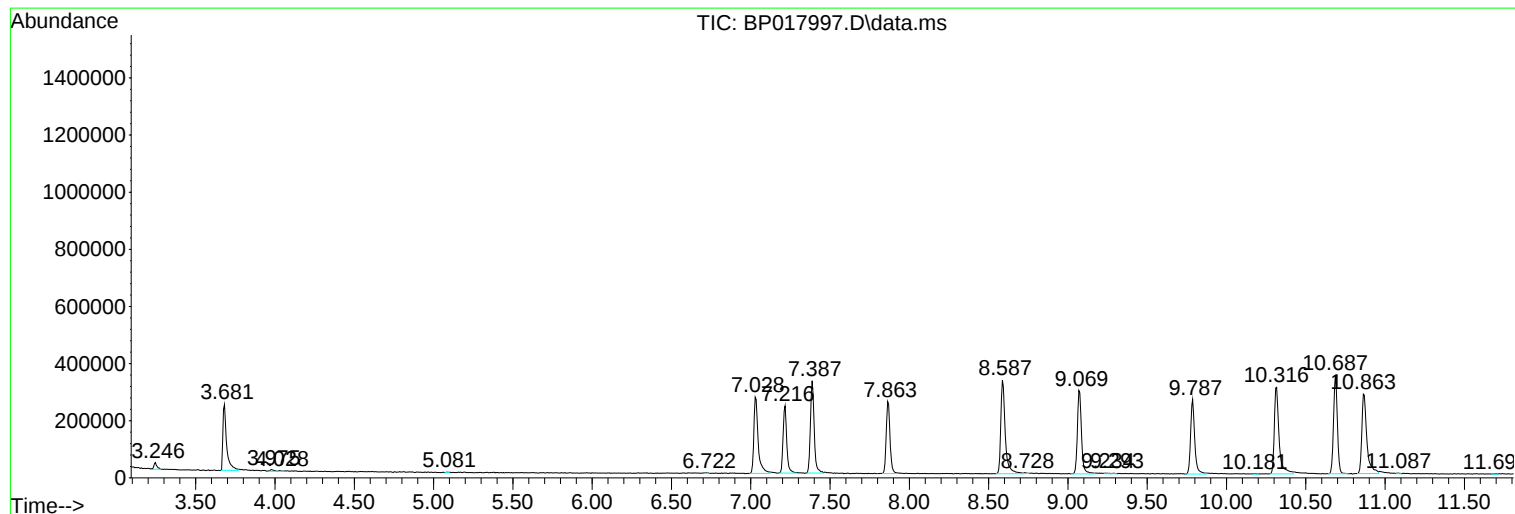

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP017997.D
Acq On : 09 Nov 2023 20:07
Operator : MA/JU
Sample : PB156742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK742

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP017997.D
Acq On : 09 Nov 2023 20:07
Operator : MA/JU
Sample : PB156742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK742

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------