

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018001.D
 Acq On : 09 Nov 2023 22:23
 Operator : MA/JU
 Sample : 05082-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH342

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018001.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	24	27	33	rVB	10656	11911	0.54%	0.072%
2	3.699	100	104	109	rBV	21145	36328	1.66%	0.219%
3	4.687	269	272	276	rBV6	2146	3223	0.15%	0.019%
4	5.111	341	344	346	rVB3	2160	2417	0.11%	0.015%
5	5.793	458	460	464	rBV5	1799	2506	0.11%	0.015%
6	6.746	620	622	624	rBV3	2063	2259	0.10%	0.014%
7	7.040	667	672	684	rBV	38372	91031	4.16%	0.548%
8	7.216	695	702	716	rBV	177724	301640	13.78%	1.816%
9	7.311	716	718	724	rVB7	2060	3697	0.17%	0.022%
10	7.387	724	731	751	rBV	189966	343957	15.71%	2.071%
11	7.863	802	812	824	rBV	202288	340836	15.57%	2.052%
12	8.593	930	936	953	rBV	131622	280141	12.79%	1.687%
13	9.069	1010	1017	1027	rBV	234652	426070	19.46%	2.565%
14	9.787	1132	1139	1153	rBV	207815	373737	17.07%	2.250%
15	10.316	1220	1229	1247	rBV	221775	479093	21.88%	2.885%
16	10.687	1284	1292	1300	rVV	271532	451427	20.62%	2.718%
17	10.869	1315	1323	1353	rBV	147807	357356	16.32%	2.152%
18	12.228	1550	1554	1559	rVV8	1260	2346	0.11%	0.014%
19	12.293	1563	1565	1566	rVV2	2701	2642	0.12%	0.016%
20	12.334	1570	1572	1574	rVV3	2640	2554	0.12%	0.015%
21	12.710	1633	1636	1639	rBV5	1745	2853	0.13%	0.017%
22	12.928	1670	1673	1676	rBV5	1961	2998	0.14%	0.018%
23	13.110	1701	1704	1708	rVB6	1272	2326	0.11%	0.014%
24	13.381	1742	1750	1754	rBV6	7377	13202	0.60%	0.079%
25	13.510	1766	1772	1774	rBV7	1778	2813	0.13%	0.017%
26	13.957	1842	1848	1863	rBV	653110	951479	43.46%	5.729%
27	14.240	1889	1896	1906	rBV	674290	981493	44.83%	5.910%
28	14.404	1921	1924	1929	rVB7	1848	3056	0.14%	0.018%
29	14.540	1939	1947	1961	rVV	409951	618567	28.25%	3.724%
30	14.840	1992	1998	2004	rBV7	13649	36423	1.66%	0.219%
31	14.940	2013	2015	2019	rVB5	3227	2824	0.13%	0.017%
32	15.369	2083	2088	2094	rBV	14777	24352	1.11%	0.147%
33	15.540	2110	2117	2133	rBV	883997	1290408	58.94%	7.770%
34	15.692	2138	2143	2155	rBV	335043	510376	23.31%	3.073%
35	16.504	2279	2281	2284	rBV4	1717	2568	0.12%	0.015%
36	17.110	2382	2384	2389	rVB6	1769	2320	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018001.D
 Acq On : 09 Nov 2023 22:23
 Operator : MA/JU
 Sample : 05082-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH342

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

37	17.322	2412	2420	2427	rBV	540527	782256	35.73%	4.710%
38	17.422	2430	2437	2451	rVV2	1138127	1645458	75.15%	9.908%
39	17.757	2490	2494	2497	rBV5	3137	4959	0.23%	0.030%
40	18.169	2559	2564	2572	rBV4	17182	31541	1.44%	0.190%
41	18.257	2577	2579	2581	rBV3	4063	3972	0.18%	0.024%
42	18.334	2590	2592	2598	rBV5	1976	4041	0.18%	0.024%
43	19.245	2743	2747	2750	rBV2	13970	18049	0.82%	0.109%
44	19.310	2755	2758	2763	rVB3	12928	20134	0.92%	0.121%
45	19.410	2771	2775	2785	rBV10	17808	29401	1.34%	0.177%
46	19.539	2795	2797	2802	rVB6	6540	8008	0.37%	0.048%
47	19.669	2814	2819	2826	rBV	1476120	2024831	92.48%	12.192%
48	21.445	3116	3121	3128	rBV	670191	907208	41.43%	5.462%
49	23.786	3512	3519	3528	rVB	1088360	2189544	100.00%	13.184%
50	23.957	3541	3548	3556	rVB	469365	975431	44.55%	5.873%




Sum of corrected areas: 16608062

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018001.D
Acq On : 09 Nov 2023 22:23
Operator : MA/JU
Sample : 05082-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH342

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

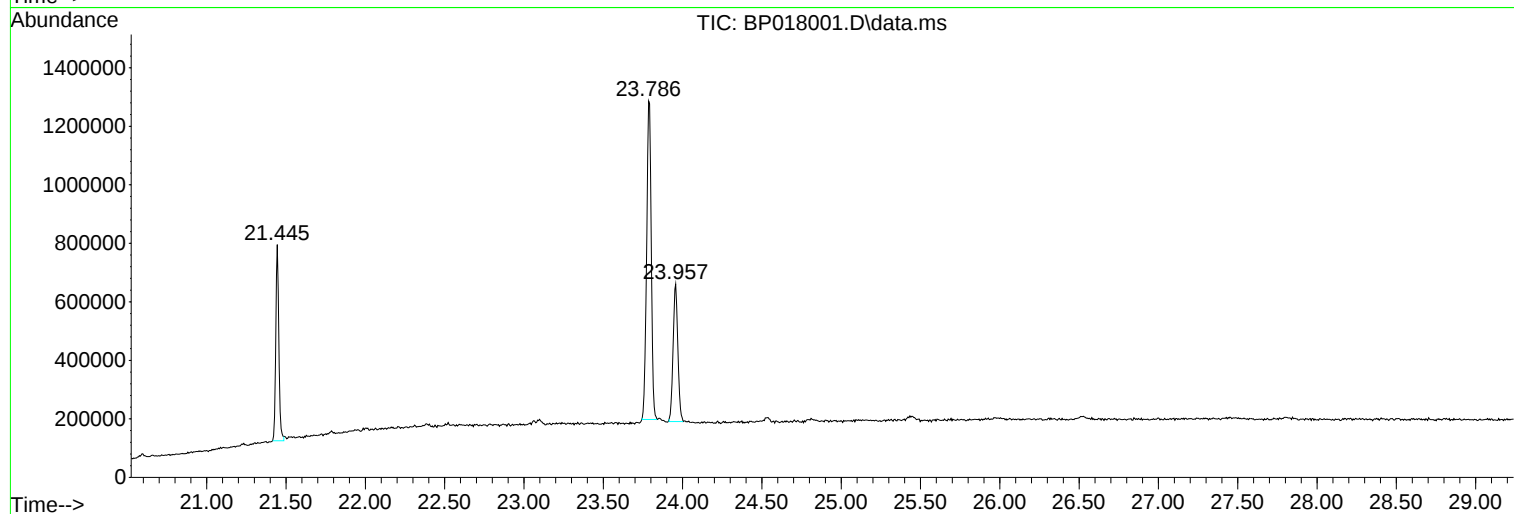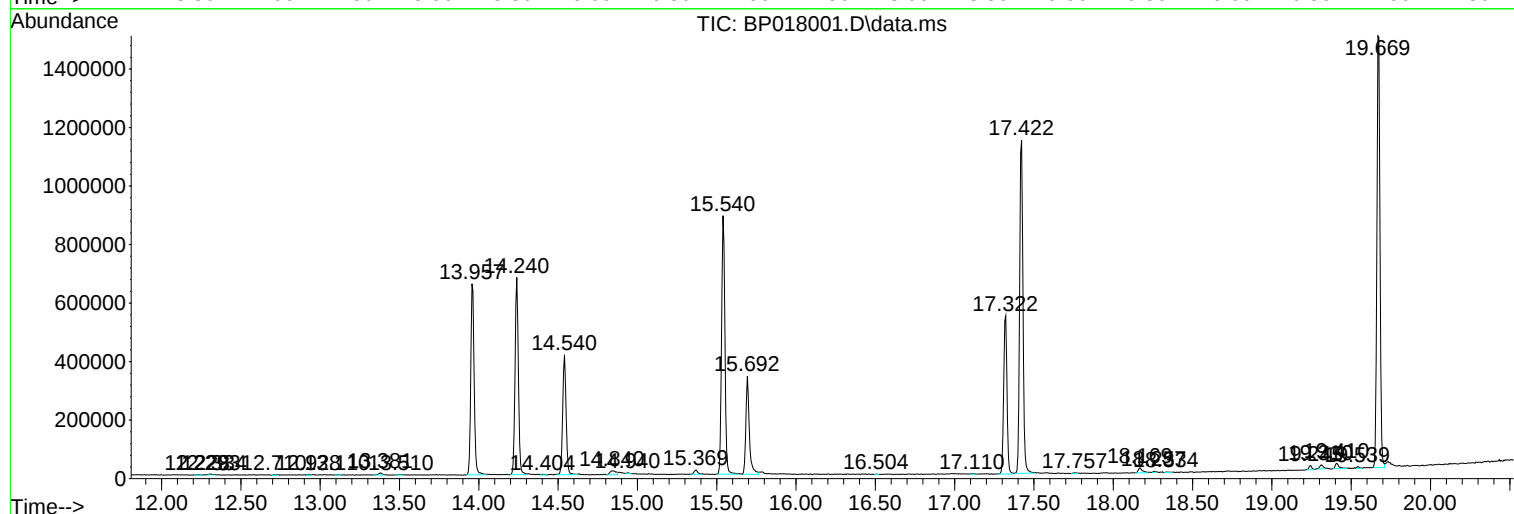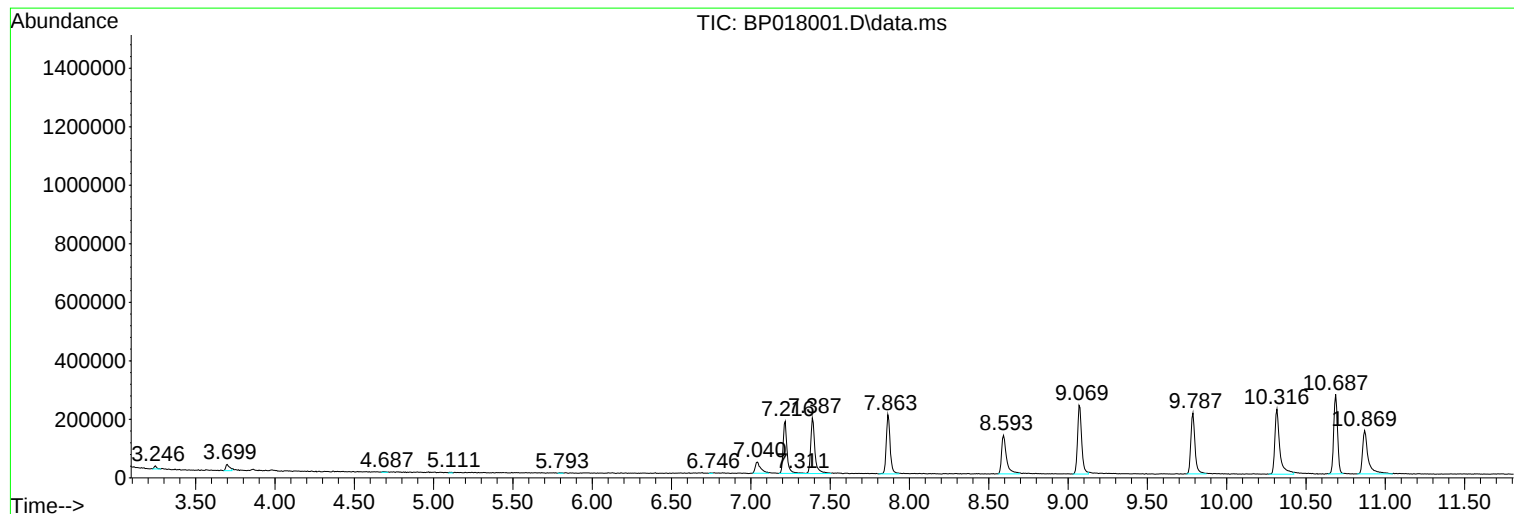

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018001.D
Acq On : 09 Nov 2023 22:23
Operator : MA/JU
Sample : 05082-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH342

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018001.D
Acq On : 09 Nov 2023 22:23
Operator : MA/JU
Sample : 05082-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH342

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------