

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018005.D
 Acq On : 10 Nov 2023 00:38
 Operator : MA/JU
 Sample : 05082-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	24	27	32	rVB	15760	19706	0.67%	0.082%
2	3.687	98	102	116	rBV	65846	120326	4.09%	0.503%
3	3.864	128	132	136	rVB4	6041	9818	0.33%	0.041%
4	3.975	149	151	158	rVB5	5159	7453	0.25%	0.031%
5	4.240	194	196	200	rVV5	2105	3143	0.11%	0.013%
6	4.434	228	229	234	rBV4	2429	3840	0.13%	0.016%
7	4.505	238	241	246	rVB6	2830	4180	0.14%	0.017%
8	6.316	545	549	553	rBV6	2808	3769	0.13%	0.016%
9	6.658	603	607	612	rVB8	1690	3443	0.12%	0.014%
10	7.034	665	671	684	rBV	66407	147330	5.01%	0.615%
11	7.210	695	701	715	rBV	280727	470818	16.02%	1.966%
12	7.387	724	731	745	rBV	305443	521173	17.73%	2.177%
13	7.863	805	812	823	rBV	263921	437703	14.89%	1.828%
14	8.046	840	843	849	rBV8	2837	5569	0.19%	0.023%
15	8.587	926	935	952	rBV	203147	411192	13.99%	1.717%
16	8.905	984	989	993	rBV8	1855	3592	0.12%	0.015%
17	9.069	1008	1017	1032	rBV	379107	664604	22.61%	2.776%
18	9.781	1132	1138	1150	rBV	316185	566449	19.27%	2.366%
19	10.310	1222	1228	1244	rBV	378357	739434	25.15%	3.088%
20	10.687	1284	1292	1303	rBV	360598	620420	21.10%	2.591%
21	10.863	1315	1322	1345	rBV	287379	630182	21.44%	2.632%
22	12.287	1561	1564	1572	rBV6	5489	10625	0.36%	0.044%
23	13.381	1745	1750	1754	rBV4	10606	17720	0.60%	0.074%
24	13.957	1842	1848	1861	rBV	997266	1407397	47.87%	5.878%
25	14.040	1861	1862	1867	rVV5	3527	3751	0.13%	0.016%
26	14.157	1877	1882	1884	rBV6	2026	3629	0.12%	0.015%
27	14.240	1889	1896	1905	rBV	998473	1469529	49.99%	6.137%
28	14.540	1939	1947	1958	rVB	578502	841275	28.62%	3.513%
29	14.834	1991	1997	2007	rBV5	22170	80355	2.73%	0.336%
30	15.287	2068	2074	2079	rBV2	12990	18705	0.64%	0.078%
31	15.369	2083	2088	2093	rBV	11872	18221	0.62%	0.076%
32	15.539	2110	2117	2127	rBV	1373334	1955910	66.53%	8.168%
33	15.692	2137	2143	2155	rBV	509113	769621	26.18%	3.214%
34	15.781	2155	2158	2164	rVB7	8724	15327	0.52%	0.064%
35	16.063	2201	2206	2211	rBV7	1980	3905	0.13%	0.016%
36	16.110	2211	2214	2218	rBV6	1899	3043	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018005.D
 Acq On : 10 Nov 2023 00:38
 Operator : MA/JU
 Sample : 05082-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH325

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

37	16.328	2248	2251	2255	rVB5	3305	3185	0.11%	0.013%
38	16.581	2288	2294	2295	rBV6	2306	3258	0.11%	0.014%
39	16.981	2359	2362	2368	rBV7	3590	6550	0.22%	0.027%
40	17.204	2398	2400	2405	rVB6	2582	2962	0.10%	0.012%
41	17.316	2413	2419	2430	rBV	743834	1070479	36.41%	4.471%
42	17.422	2430	2437	2453	rVV	1637386	2344809	79.76%	9.792%
43	17.945	2522	2526	2530	rBV6	3098	5012	0.17%	0.021%
44	18.163	2558	2563	2570	rBV2	56303	84379	2.87%	0.352%
45	18.516	2620	2623	2625	rBV3	3423	4244	0.14%	0.018%
46	18.728	2654	2659	2668	rVB3	8271	16742	0.57%	0.070%
47	19.239	2742	2746	2750	rBV2	21756	31334	1.07%	0.131%
48	19.310	2755	2758	2763	rVB2	23263	33608	1.14%	0.140%
49	19.404	2770	2774	2780	rBV4	32636	49831	1.70%	0.208%
50	19.539	2795	2797	2801	rVB5	9546	10215	0.35%	0.043%
51	19.669	2813	2819	2826	rBV	2213499	2909821	98.98%	12.152%
52	21.445	3116	3121	3128	rBV	871876	1182481	40.22%	4.938%
53	23.786	3512	3519	3530	rVB	1467146	2939835	100.00%	12.277%
54	23.957	3541	3548	3557	rVB	584098	1233177	41.95%	5.150%




Sum of corrected areas: 23945079

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018005.D
Acq On : 10 Nov 2023 00:38
Operator : MA/JU
Sample : 05082-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

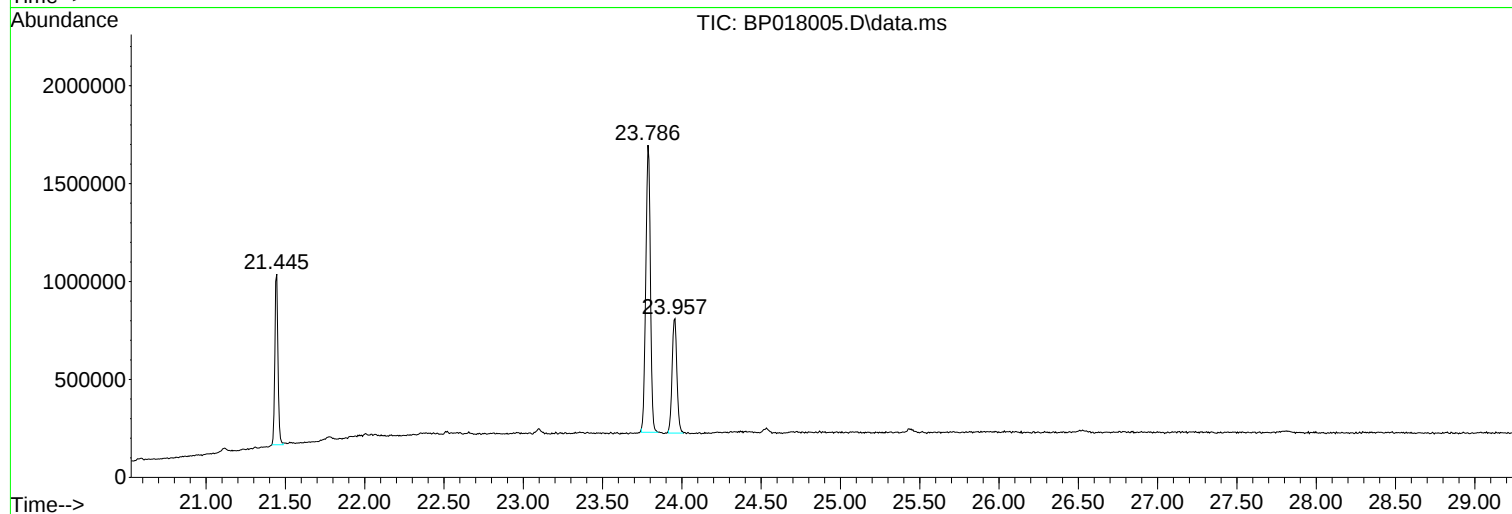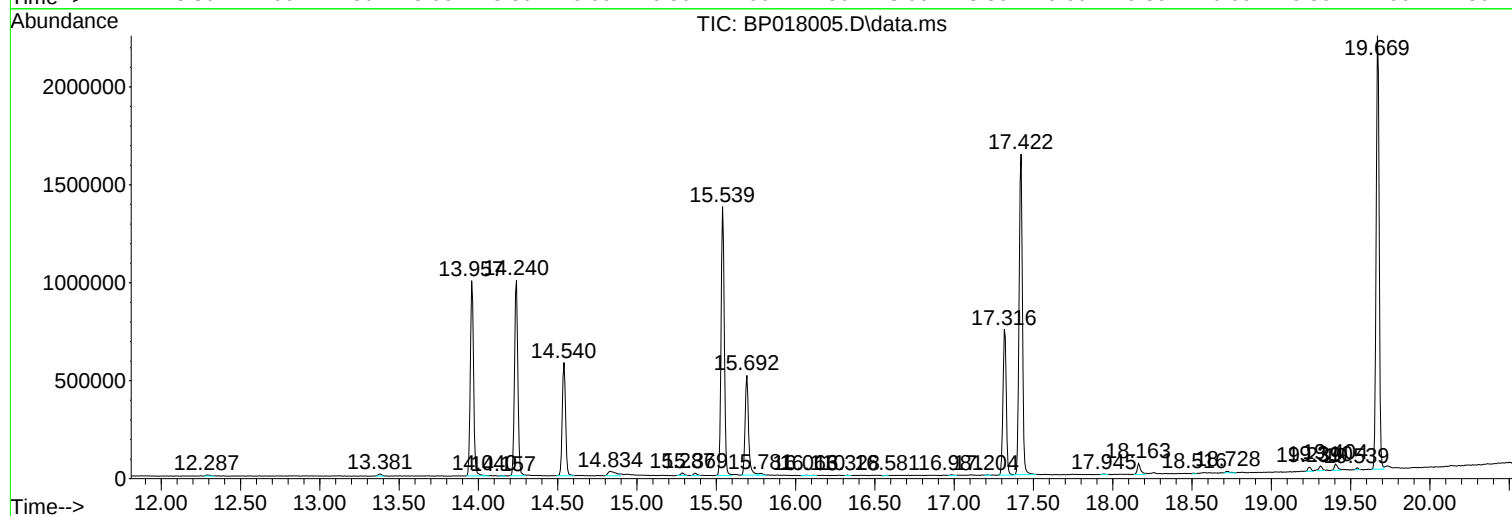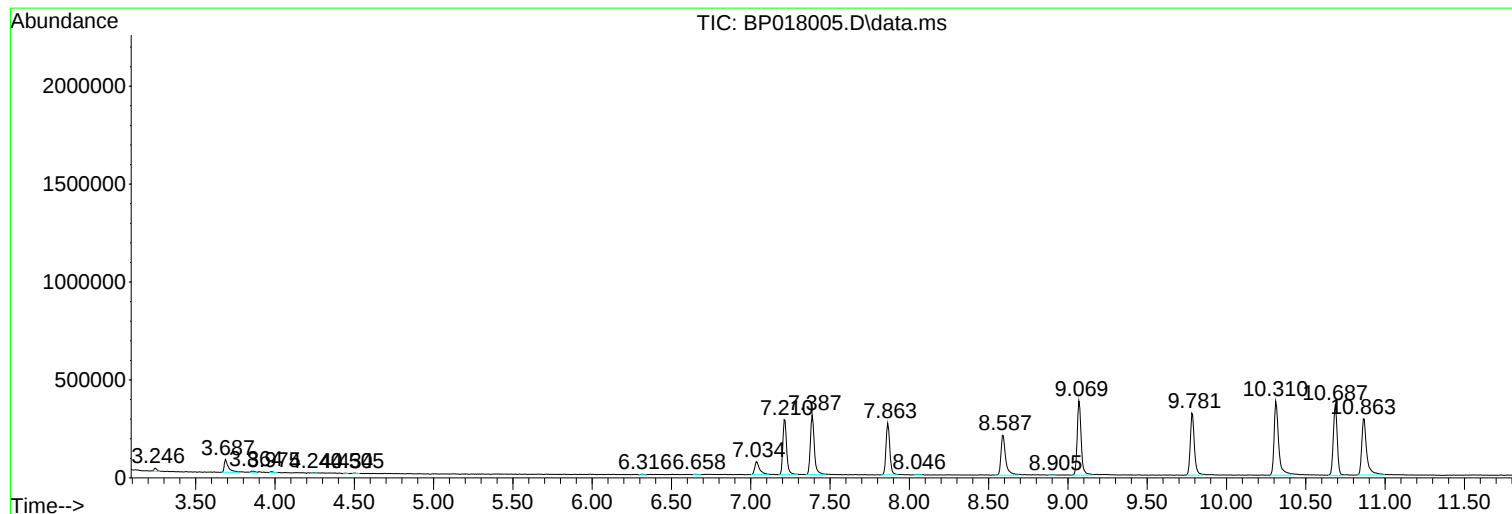

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018005.D
Acq On : 10 Nov 2023 00:38
Operator : MA/JU
Sample : 05082-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018005.D
Acq On : 10 Nov 2023 00:38
Operator : MA/JU
Sample : 05082-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------