

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018014.D
 Acq On : 10 Nov 2023 06:18
 Operator : MA/JU
 Sample : PB156753BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK753

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	33	rVB	22624	30509	1.40%	0.144%
2	3.675	97	100	115	rBV	258111	411447	18.90%	1.939%
3	5.564	416	421	424	rBV7	1647	2541	0.12%	0.012%
4	7.028	664	670	688	rBV	297816	534730	24.57%	2.520%
5	7.211	695	701	712	rBV	244014	386441	17.75%	1.821%
6	7.387	724	731	746	rBV	328915	563675	25.90%	2.656%
7	7.863	806	812	826	rVV	290249	474863	21.82%	2.238%
8	8.587	928	935	955	rBV	350585	667927	30.69%	3.148%
9	8.828	973	976	980	rBV6	1455	2274	0.10%	0.011%
10	9.069	1010	1017	1027	rBV	312052	536896	24.67%	2.530%
11	9.434	1076	1079	1084	rBV7	2075	2518	0.12%	0.012%
12	9.781	1130	1138	1152	rBV	264594	491730	22.59%	2.317%
13	10.310	1220	1228	1245	rBV	317520	652476	29.98%	3.075%
14	10.681	1284	1291	1301	rBV	377876	647918	29.77%	3.053%
15	10.863	1315	1322	1339	rBV	307352	651259	29.92%	3.069%
16	11.110	1361	1364	1369	rVB7	1687	2709	0.12%	0.013%
17	11.310	1393	1398	1400	rVB6	1766	2447	0.11%	0.012%
18	12.299	1564	1566	1567	rBV2	2547	2258	0.10%	0.011%
19	12.310	1567	1568	1574	rVB6	2700	3154	0.14%	0.015%
20	13.028	1688	1690	1697	rVB8	1273	2375	0.11%	0.011%
21	13.381	1744	1750	1755	rBV8	5836	11623	0.53%	0.055%
22	13.957	1842	1848	1862	rBV	757372	1086311	49.91%	5.120%
23	14.234	1889	1895	1907	rBV	777562	1160225	53.31%	5.468%
24	14.540	1938	1947	1956	rBV	560405	857960	39.42%	4.043%
25	14.616	1959	1960	1965	rVB5	2493	3124	0.14%	0.015%
26	14.798	1984	1991	2015	rBV2	134326	439592	20.20%	2.072%
27	15.363	2083	2087	2093	rBV4	5770	8609	0.40%	0.041%
28	15.540	2109	2117	2131	rBV	1051327	1474607	67.75%	6.949%
29	15.692	2137	2143	2155	rBV2	313474	505618	23.23%	2.383%
30	15.781	2155	2158	2165	rVB9	8191	15012	0.69%	0.071%
31	16.428	2264	2268	2272	rBV7	1352	2194	0.10%	0.010%
32	16.575	2291	2293	2297	rVB5	1892	2301	0.11%	0.011%
33	16.792	2327	2330	2335	rVB7	1329	2609	0.12%	0.012%
34	16.986	2358	2363	2366	rBV6	2715	3992	0.18%	0.019%
35	17.110	2380	2384	2389	rVB8	3113	4496	0.21%	0.021%
36	17.316	2413	2419	2430	rBV	801695	1103848	50.71%	5.202%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018014.D
 Acq On : 10 Nov 2023 06:18
 Operator : MA/JU
 Sample : PB156753BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK753

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

37	17.416	2430	2436	2454	rVV	1107650	1675066	76.96%	7.894%
38	18.551	2626	2629	2632	rBV4	2848	4723	0.22%	0.022%
39	19.245	2742	2747	2750	rBV3	13781	18695	0.86%	0.088%
40	19.316	2755	2759	2762	rVV3	13695	18715	0.86%	0.088%
41	19.669	2813	2819	2830	rBV	1533262	2019134	92.77%	9.516%
42	21.445	3116	3121	3129	rBV	906099	1251844	57.51%	5.900%
43	23.786	3511	3519	3533	rVB2	1076243	2176574	100.00%	10.258%
44	23.951	3540	3547	3557	rVB	615203	1302036	59.82%	6.136%




Sum of corrected areas: 21219055

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018014.D
Acq On : 10 Nov 2023 06:18
Operator : MA/JU
Sample : PB156753BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK753

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

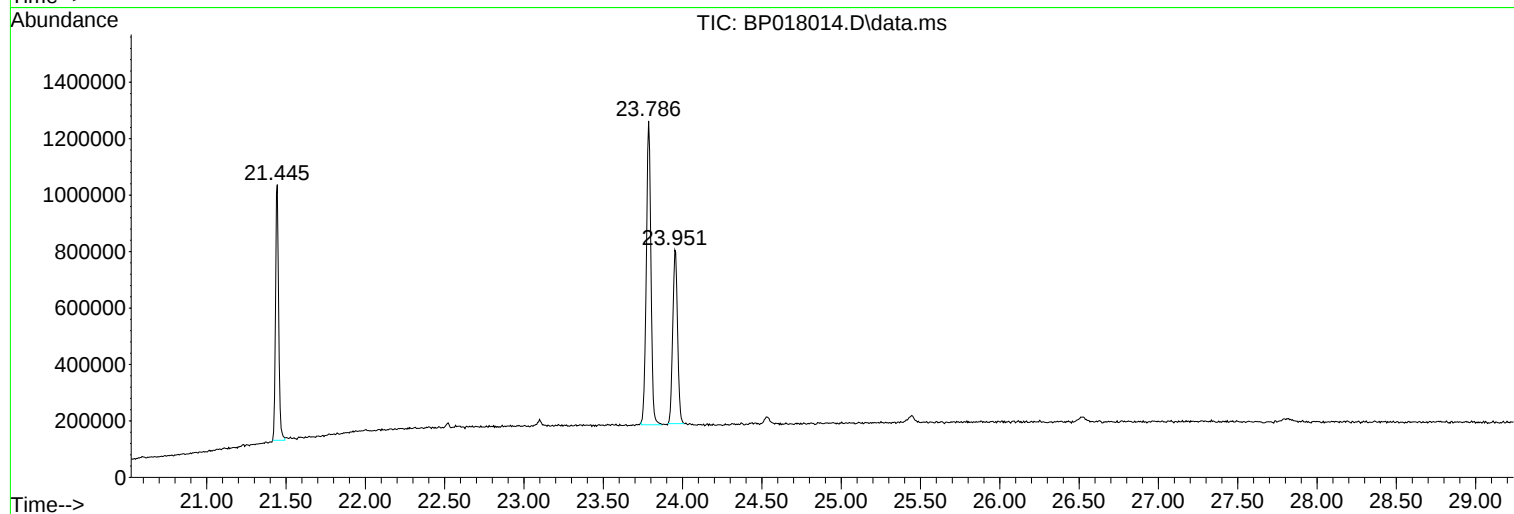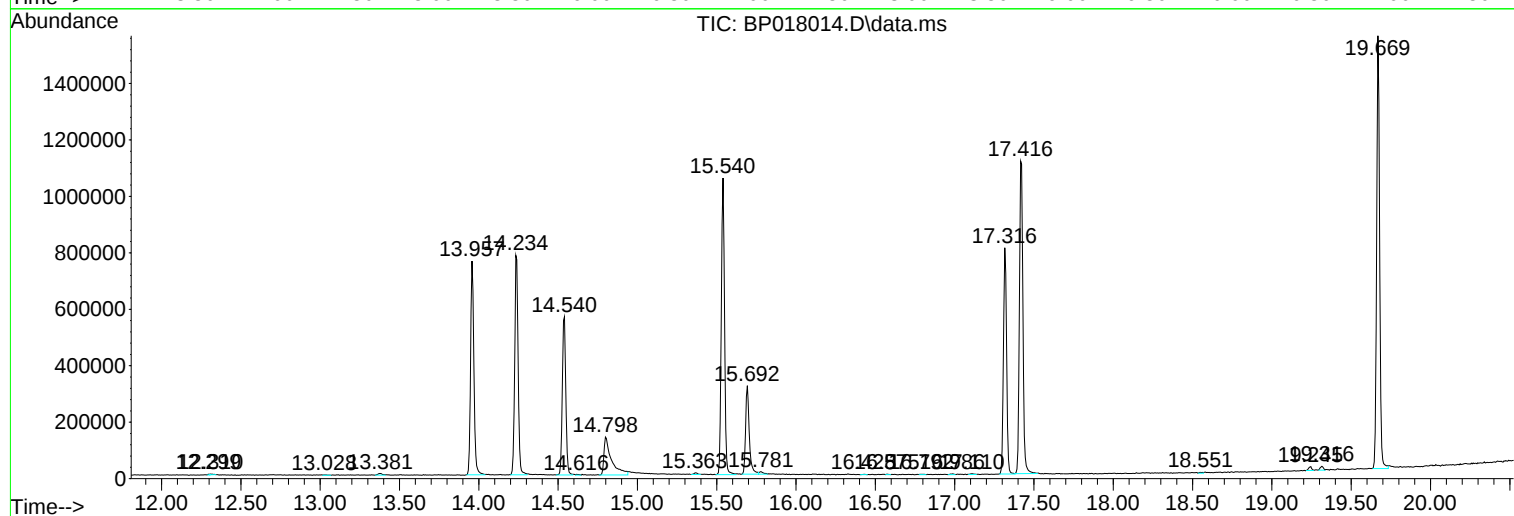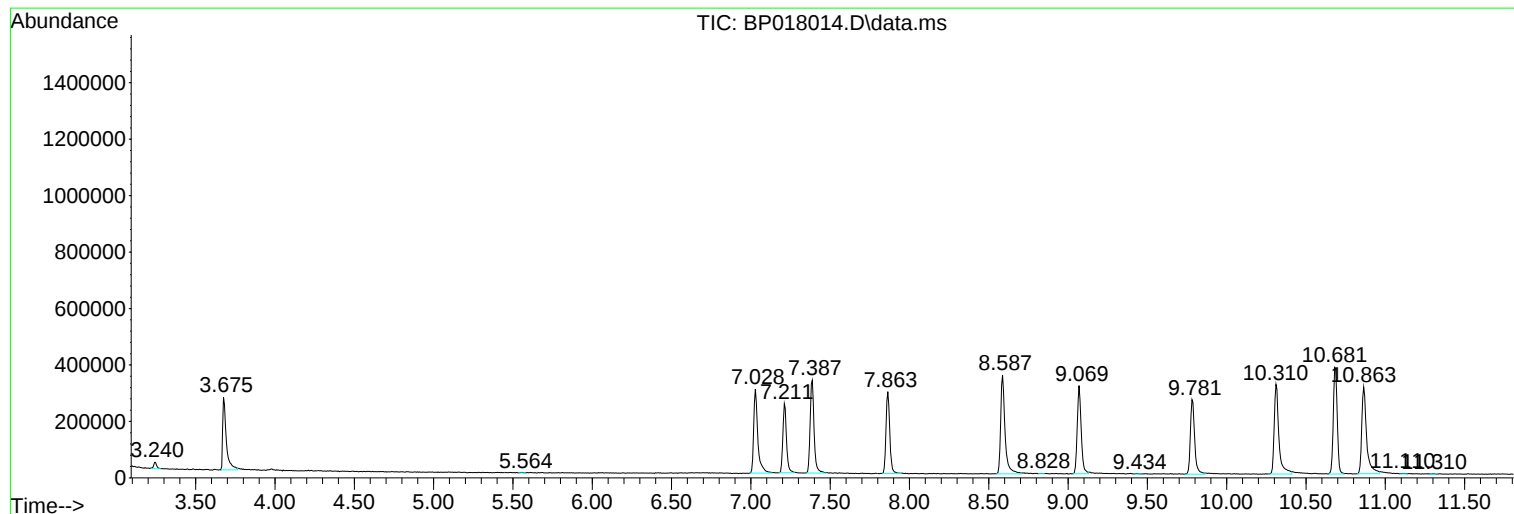

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018014.D
Acq On : 10 Nov 2023 06:18
Operator : MA/JU
Sample : PB156753BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK753

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018014.D
Acq On : 10 Nov 2023 06:18
Operator : MA/JU
Sample : PB156753BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK753

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------