

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018024.D
 Acq On : 10 Nov 2023 11:57
 Operator : MA/JU
 Sample : 05091-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKI8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.717	103	107	108	rBV3	5055	7867	0.52%	0.063%
2	3.858	127	131	138	rVB2	14253	22690	1.50%	0.182%
3	4.905	305	309	316	rVB	19236	31319	2.08%	0.251%
4	5.034	329	331	334	rVB4	2140	1923	0.13%	0.015%
5	5.475	403	406	408	rBV4	2054	2687	0.18%	0.022%
6	5.611	426	429	433	rBV6	1741	3071	0.20%	0.025%
7	5.675	438	440	443	rBV4	1954	2557	0.17%	0.021%
8	5.822	462	465	468	rBV3	2015	2258	0.15%	0.018%
9	6.346	552	554	555	rBV2	2176	1981	0.13%	0.016%
10	6.722	615	618	619	rBV3	1823	2214	0.15%	0.018%
11	7.034	665	671	688	rBV2	82227	198576	13.16%	1.593%
12	7.211	696	701	712	rVV	71612	123006	8.15%	0.987%
13	7.387	725	731	748	rVV	101450	181783	12.05%	1.458%
14	7.505	748	751	755	rVB6	2083	3184	0.21%	0.026%
15	7.593	763	766	769	rBV5	1543	2148	0.14%	0.017%
16	7.793	797	800	801	rBV3	1757	2059	0.14%	0.017%
17	7.863	804	812	826	rBV	350156	578824	38.36%	4.644%
18	8.599	931	937	950	rBV2	44784	102275	6.78%	0.821%
19	8.722	952	958	974	rVV	103498	200072	13.26%	1.605%
20	9.069	1009	1017	1028	rBV	95778	185016	12.26%	1.484%
21	9.258	1048	1049	1053	rVB4	2460	2741	0.18%	0.022%
22	9.299	1053	1056	1057	rBV3	2633	2345	0.16%	0.019%
23	9.481	1084	1087	1090	rVB5	1804	2397	0.16%	0.019%
24	9.787	1131	1139	1149	rBV	81920	159860	10.59%	1.283%
25	9.975	1164	1171	1177	rBV7	8049	23836	1.58%	0.191%
26	10.157	1198	1202	1209	rBV5	9124	19605	1.30%	0.157%
27	10.322	1223	1230	1245	rVV	85013	191597	12.70%	1.537%
28	10.687	1284	1292	1299	rBV	465336	786704	52.14%	6.311%
29	10.875	1317	1324	1340	rBV2	50595	124816	8.27%	1.001%
30	11.022	1346	1349	1350	rVB3	1836	1883	0.12%	0.015%
31	11.075	1355	1358	1361	rVB5	1925	2608	0.17%	0.021%
32	11.216	1379	1382	1384	rBV4	1956	2286	0.15%	0.018%
33	11.234	1384	1385	1387	rVV2	4108	2709	0.18%	0.022%
34	11.275	1387	1392	1395	rVV7	4011	8535	0.57%	0.068%
35	11.310	1395	1398	1399	rVV3	3071	3468	0.23%	0.028%
36	11.340	1401	1403	1407	rVB5	2576	2850	0.19%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018024.D
 Acq On : 10 Nov 2023 11:57
 Operator : MA/JU
 Sample : 05091-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKI8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

37	11.740	1466	1471	1472	rBV5	2159	2602	0.17%	0.021%
38	12.193	1545	1548	1550	rBV4	1888	1990	0.13%	0.016%
39	12.275	1560	1562	1567	rVB6	2850	3339	0.22%	0.027%
40	12.369	1575	1578	1580	rVB4	2230	2069	0.14%	0.017%
41	12.557	1608	1610	1615	rVB6	1536	2232	0.15%	0.018%
42	12.604	1615	1618	1621	rBV5	1697	2111	0.14%	0.017%
43	12.740	1637	1641	1644	rVB6	2004	2855	0.19%	0.023%
44	12.969	1675	1680	1683	rVB7	1543	2695	0.18%	0.022%
45	13.275	1727	1732	1734	rVB6	2121	2332	0.15%	0.019%
46	13.375	1743	1749	1754	rBV3	18413	30945	2.05%	0.248%
47	13.793	1817	1820	1824	rVV5	3395	4066	0.27%	0.033%
48	13.869	1829	1833	1834	rVB4	2125	2170	0.14%	0.017%
49	13.957	1841	1848	1855	rBV	239501	352943	23.39%	2.832%
50	14.022	1855	1859	1866	rVV10	12179	22572	1.50%	0.181%
51	14.081	1866	1869	1872	rVB5	1813	2497	0.17%	0.020%
52	14.181	1881	1886	1889	rBV7	1713	3034	0.20%	0.024%
53	14.234	1889	1895	1909	rVV	270225	411000	27.24%	3.297%
54	14.369	1915	1918	1923	rVB7	1827	2767	0.18%	0.022%
55	14.540	1937	1947	1955	rBV	713537	1060542	70.29%	8.508%
56	14.622	1960	1961	1964	rVV3	3589	3103	0.21%	0.025%
57	14.834	1992	1997	2004	rBV4	17874	52405	3.47%	0.420%
58	14.904	2007	2009	2010	rVV2	6020	5654	0.37%	0.045%
59	14.928	2012	2013	2016	rVV3	7164	8051	0.53%	0.065%
60	14.951	2016	2017	2020	rVV3	5573	5562	0.37%	0.045%
61	15.010	2024	2027	2032	rVB7	3576	7019	0.47%	0.056%
62	15.163	2051	2053	2057	rBV5	1933	2000	0.13%	0.016%
63	15.287	2071	2074	2077	rBV5	1614	1868	0.12%	0.015%
64	15.369	2084	2088	2091	rBV4	4065	5349	0.35%	0.043%
65	15.540	2108	2117	2124	rBV	354942	521451	34.56%	4.183%
66	15.698	2139	2144	2153	rBV2	45432	75861	5.03%	0.609%
67	15.922	2179	2182	2187	rVV6	4035	5560	0.37%	0.045%
68	15.992	2191	2194	2197	rBV5	2084	2493	0.17%	0.020%
69	16.092	2204	2211	2215	rBV9	2418	5322	0.35%	0.043%
70	16.145	2217	2220	2222	rVV4	1841	2304	0.15%	0.018%
71	16.198	2222	2229	2232	rVB9	3192	6668	0.44%	0.053%
72	16.322	2246	2250	2255	rVB8	2471	3799	0.25%	0.030%
73	16.481	2274	2277	2281	rBV4	4905	6319	0.42%	0.051%
74	16.528	2283	2285	2289	rVB4	1839	2015	0.13%	0.016%
75	16.669	2307	2309	2313	rBV5	2203	3138	0.21%	0.025%
76	16.787	2326	2329	2334	rBV6	3491	5369	0.36%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
 Data File : BP018024.D
 Acq On : 10 Nov 2023 11:57
 Operator : MA/JU
 Sample : 05091-11
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCK18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
 Title : SVOA CALIBRATION

77	16.839	2334	2338	2344	rVV7	5475	9734	0.65%	0.078%
78	16.992	2360	2364	2367	rVB5	3985	6116	0.41%	0.049%
79	17.034	2367	2371	2373	rBV5	2565	3134	0.21%	0.025%
80	17.316	2411	2419	2431	rBV	908748	1341853	88.93%	10.765%
81	17.416	2431	2436	2448	rVV2	380318	590400	39.13%	4.737%
82	17.522	2451	2454	2460	rVB7	7279	12446	0.82%	0.100%
83	17.681	2477	2481	2483	rBV5	2212	3627	0.24%	0.029%
84	17.810	2499	2503	2509	rBV8	4769	9641	0.64%	0.077%
85	17.992	2530	2534	2537	rBV5	2743	3305	0.22%	0.027%
86	18.086	2547	2550	2555	rBV2	5774	6746	0.45%	0.054%
87	18.163	2558	2563	2570	rBV3	53017	86420	5.73%	0.693%
88	18.422	2605	2607	2608	rBV2	3165	2610	0.17%	0.021%
89	18.563	2626	2631	2635	rBV8	11981	19690	1.30%	0.158%
90	18.769	2663	2666	2671	rVB2	22456	30053	1.99%	0.241%
91	18.992	2700	2704	2707	rBV	25325	34955	2.32%	0.280%
92	19.028	2707	2710	2714	rVB3	12149	17585	1.17%	0.141%
93	19.339	2760	2763	2771	rVB	29600	40828	2.71%	0.328%
94	19.410	2771	2775	2780	rBV2	29174	42270	2.80%	0.339%
95	19.669	2814	2819	2832	rBV	572675	836516	55.44%	6.711%
96	20.128	2894	2897	2901	rBV5	15415	22387	1.48%	0.180%
97	21.086	3057	3060	3061	rBV2	32011	33258	2.20%	0.267%
98	21.445	3116	3121	3127	rBV	1147860	1479170	98.03%	11.867%
99	23.786	3513	3519	3526	rVB2	340137	683205	45.28%	5.481%
100	23.957	3541	3548	3558	rVB	735905	1508856	100.00%	12.105%




Sum of corrected areas: 12464626

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018024.D
Acq On : 10 Nov 2023 11:57
Operator : MA/JU
Sample : 05091-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCK18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

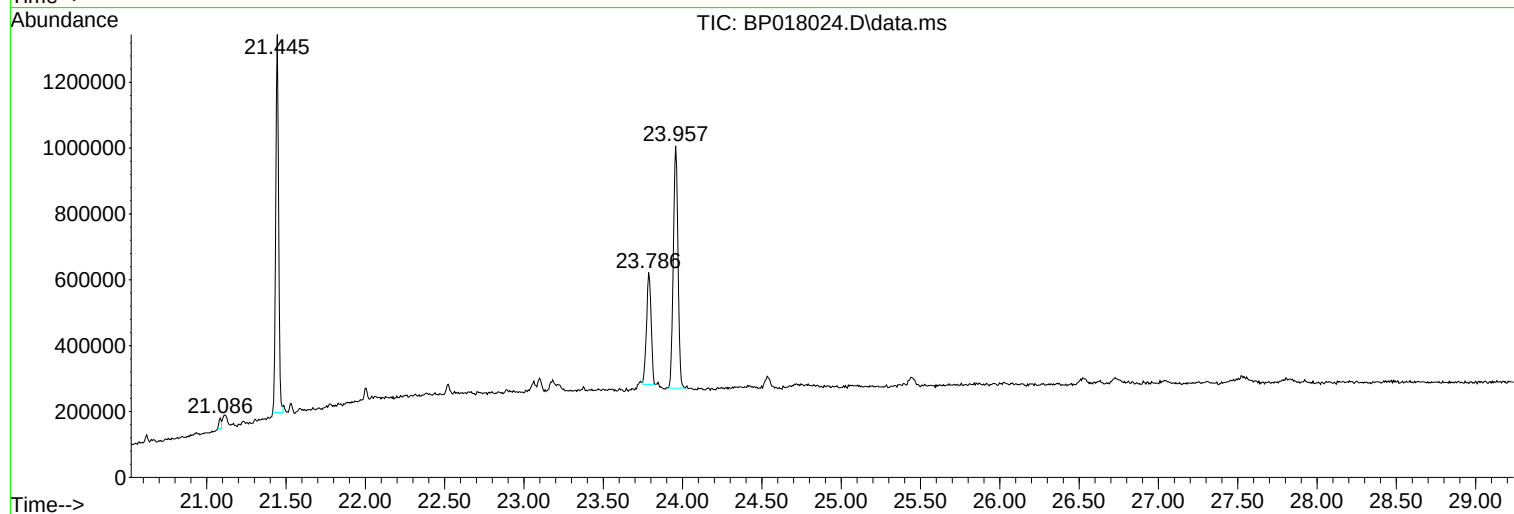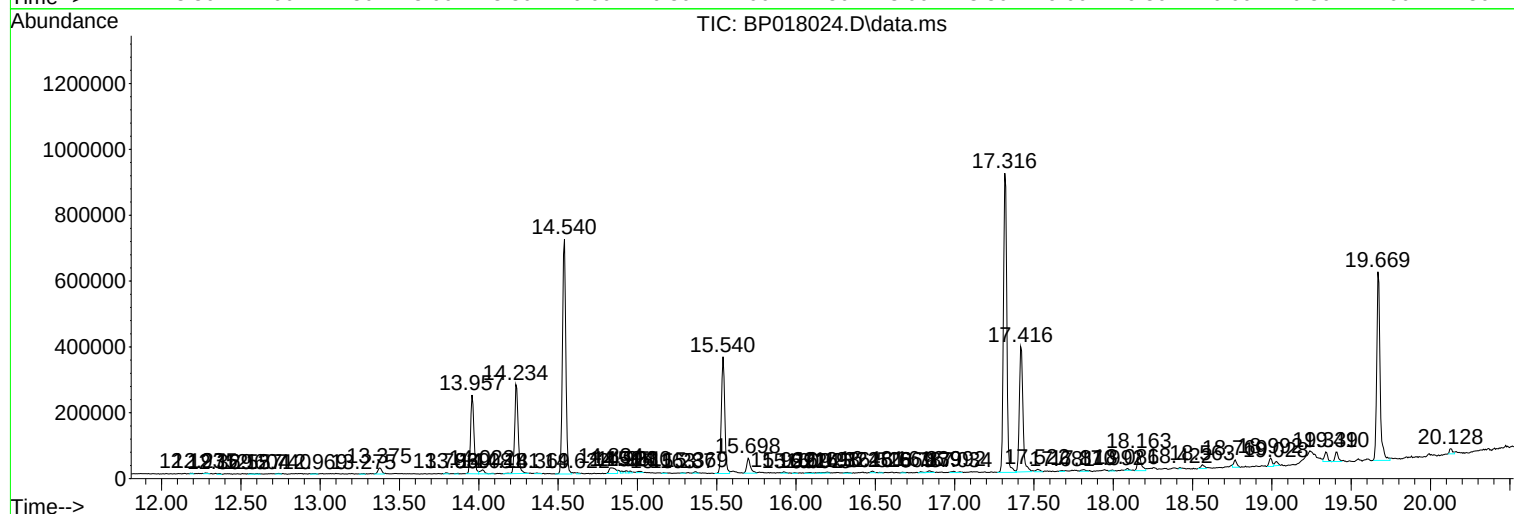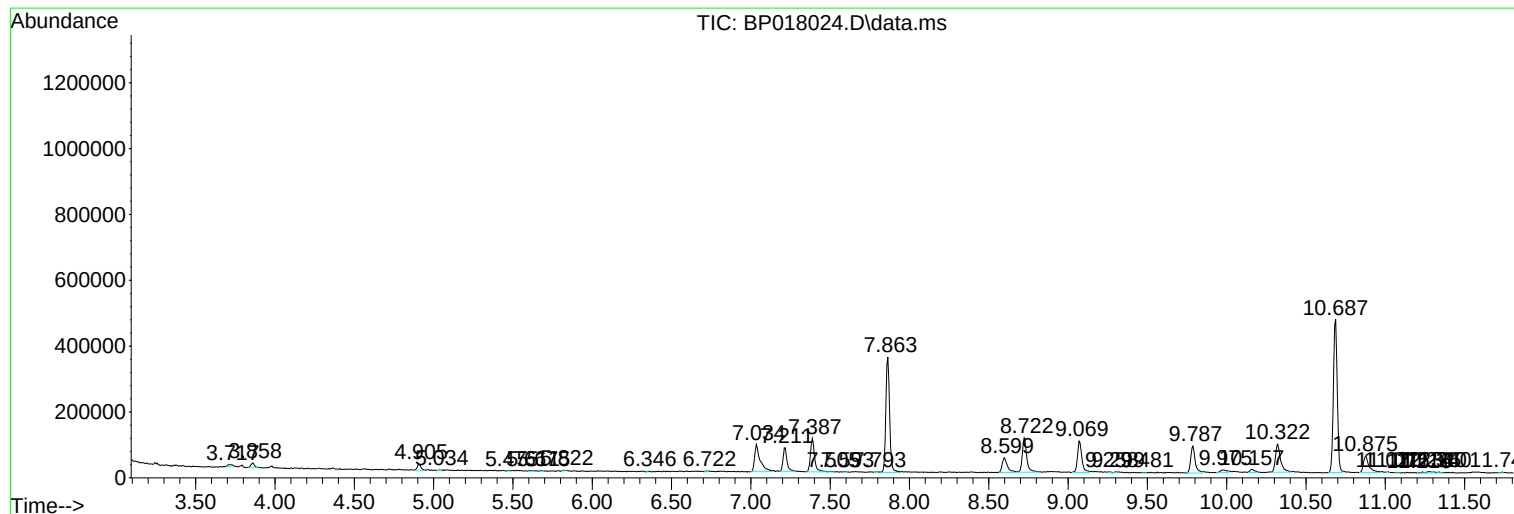

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018024.D
Acq On : 10 Nov 2023 11:57
Operator : MA/JU
Sample : 05091-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCK18










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Aceto phenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.722	6.91 ng/ul	200072	1,4-Dichlorobenzene-d4	7.863

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Acetophenone			120	C8H8O	000098-86-2	97
2	Acetophenone			120	C8H8O	000098-86-2	94
3	Acetophenone			120	C8H8O	000098-86-2	91
4	Acetophenone			120	C8H8O	000098-86-2	91
5	Acetophenone			120	C8H8O	000098-86-2	91

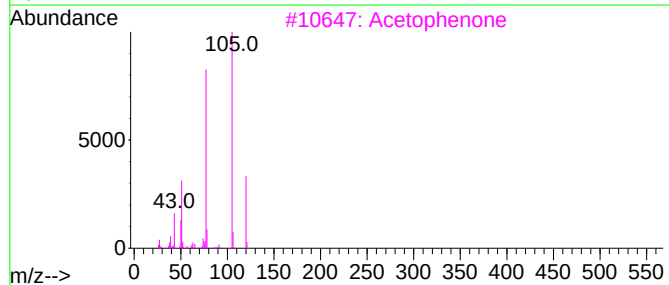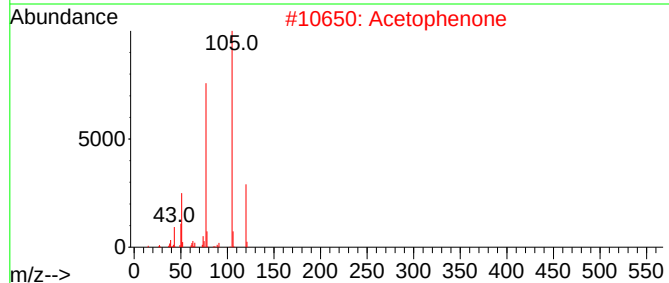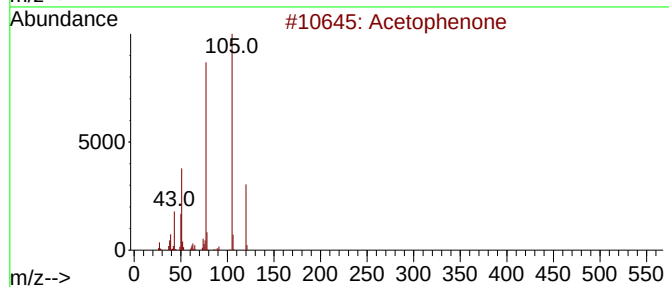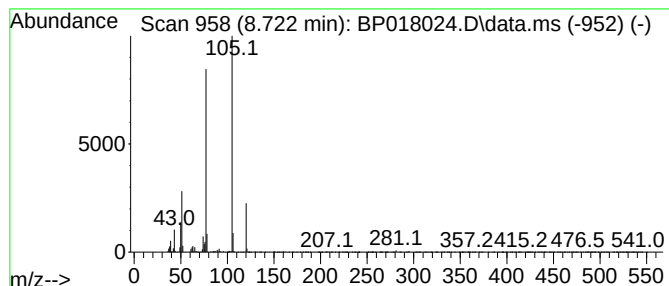

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110923\
Data File : BP018024.D
Acq On : 10 Nov 2023 11:57
Operator : MA/JU
Sample : 05091-11
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCK18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Aceto phenone	8.722	6.9	ng/u1	200072	1	7.863	578824	20.0