




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022953.D
Acq On : 09 Nov 2024 05:47
Operator : RC/JU
Sample : P4744-11
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP65

Manual IntegrationsAPPROVED

Quant Time: Nov 09 06:16:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

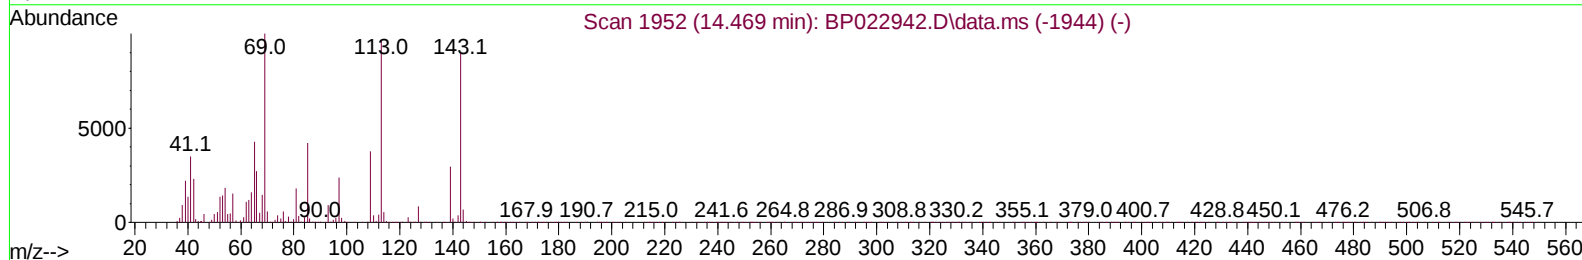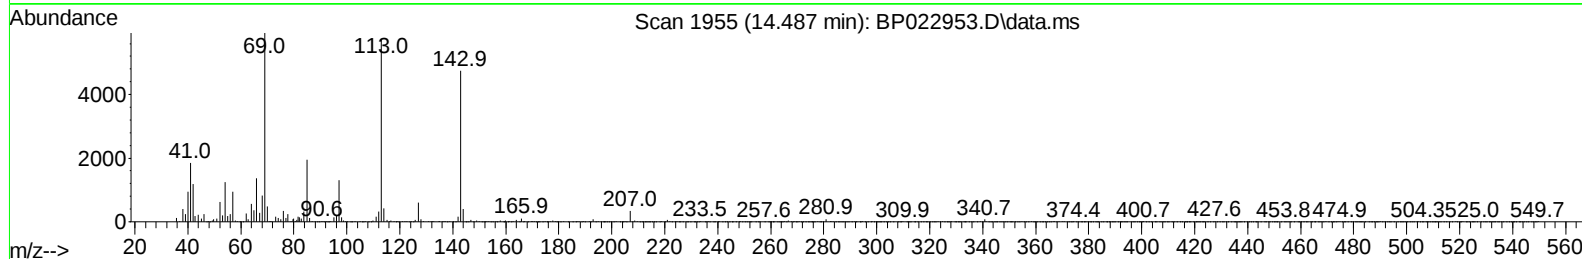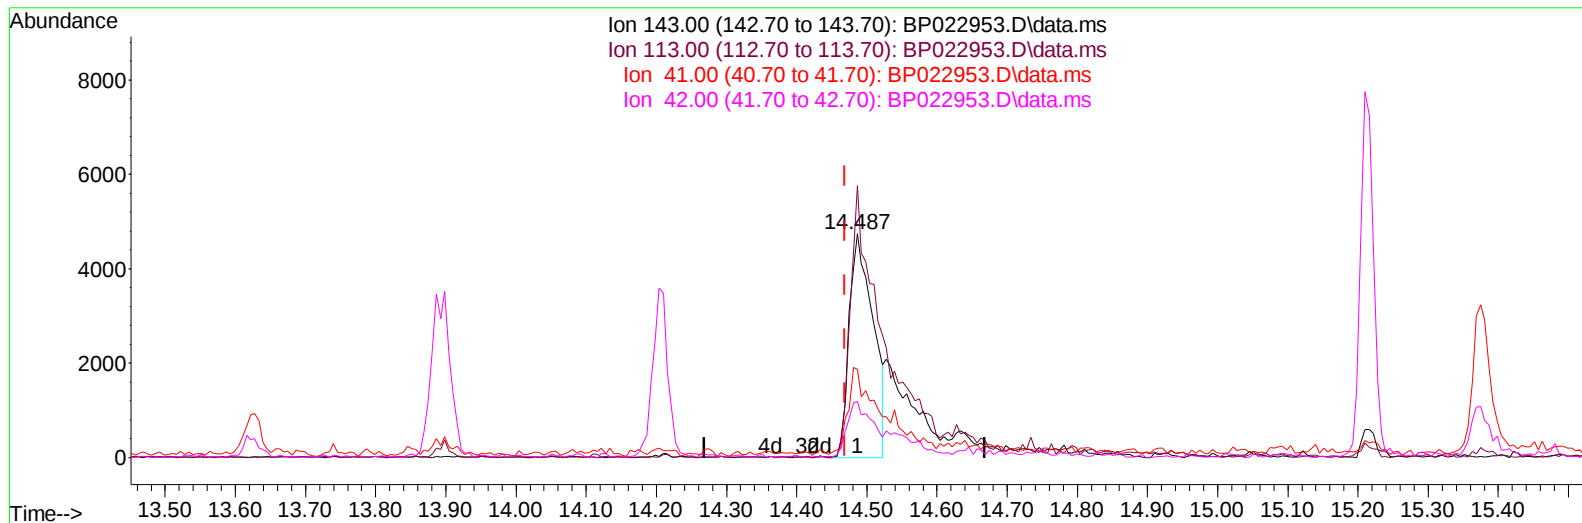

TIC: BP022953.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.487min (+ 0.018) 5.94 ng/u1

response 11220

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	121.40
41.00	39.20	39.26
42.00	25.90	24.95




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022953.D
Acq On : 09 Nov 2024 05:47
Operator : RC/JU
Sample : P4744-11
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP65

Manual IntegrationsAPPROVED

Quant Time: Nov 09 06:16:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

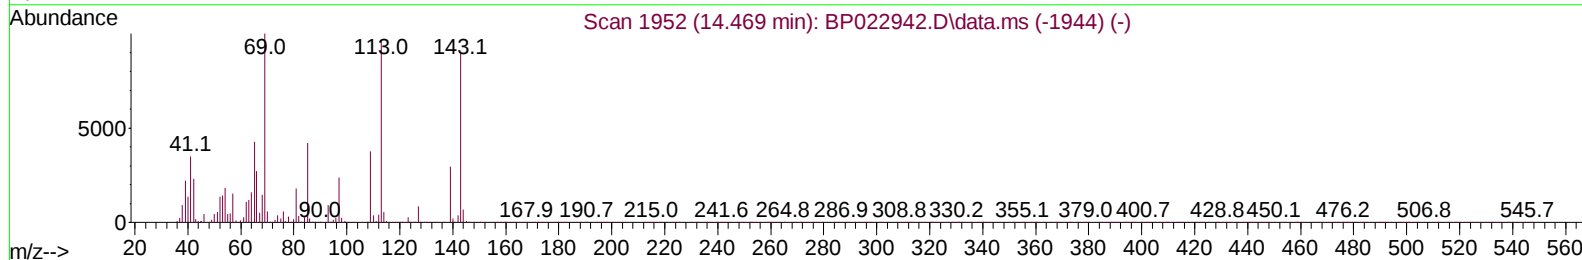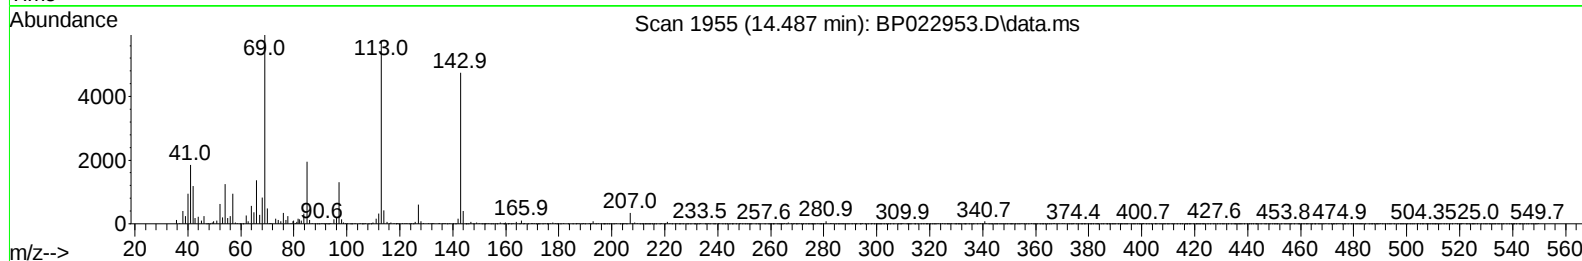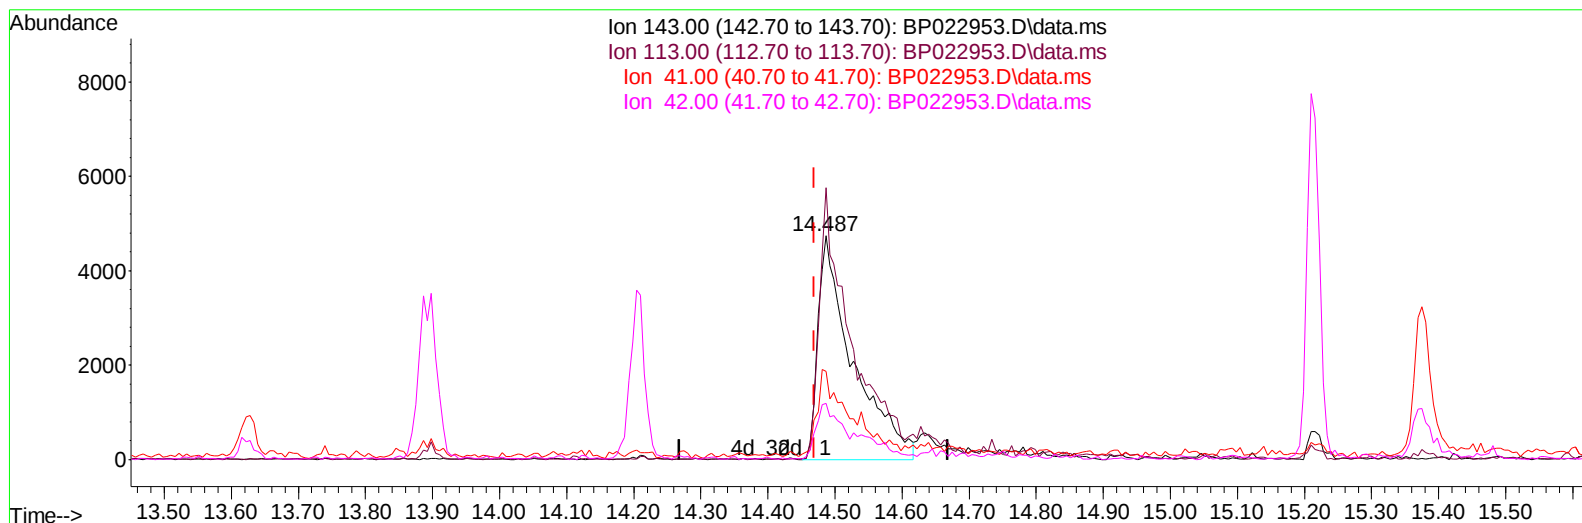

TIC: BP022953.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.487min (+ 0.018) 9.03 ng/ul m

response 17060

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	121.40
41.00	39.20	39.26
42.00	25.90	24.95

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022953.D
 Acq On : 09 Nov 2024 05:47
 Operator : RC/JU
 Sample : P4744-11
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP65

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 09 06:17:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 08 23:49:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	59724	20.000	ng/ul	0.00
20) Naphthalene-d8	10.340	136	216523	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.204	164	174504	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.016	188	458041	20.000	ng/ul	-0.02
79) Chrysene-d12	21.457	240	648176	20.000	ng/ul	# 0.00
88) Perylene-d12	24.674	264	802525	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	6154	4.953	ng/uL	0.00
4) Pyridine-d5	3.569	84	14415	3.905	ng/ul	0.01
7) Phenol-d5	6.799	99	40893	9.261	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	85324	32.890	ng/ul	0.00
11) 2-Chlorophenol-d4	7.140	132	102669	31.748	ng/ul	0.00
15) 4-Methylphenol-d8	8.304	113	76868	21.155	ng/ul	0.00
21) Nitrobenzene-d5	8.740	128	56012	37.159	ng/ul	0.00
24) 2-Nitrophenol-d4	9.451	143	67410	37.511	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.987	165	133164	35.384	ng/ul	0.00
31) 4-Chloroaniline-d4	10.498	131	76696	17.083	ng/ul	0.00
46) Dimethylphthalate-d6	13.628	166	513112	40.798	ng/ul	0.01
49) Acenaphthylene-d8	13.892	160	491944	37.487	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.487	143	17060m	9.026	ng/ul	0.02
60) Fluorene-d10	15.216	176	442194	40.101	ng/ul	-0.02
65) 4,6-Dinitro-2-methylph...	15.375	200	98371	35.851	ng/ul	0.00
73) Anthracene-d10	17.116	188	780745	40.257	ng/ul	0.00
81) Pyrene-d10	19.504	212	1107794	37.105	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.451	264	1561645	40.851	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022953.D
Acq On : 09 Nov 2024 05:47
Operator : RC/JU
Sample : P4744-11
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP65

Manual IntegrationsAPPROVED

Quant Time: Nov 09 06:17:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

