




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022961.D
Acq On : 09 Nov 2024 11:10
Operator : RC/JU
Sample : P4744-17
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP72

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:30:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

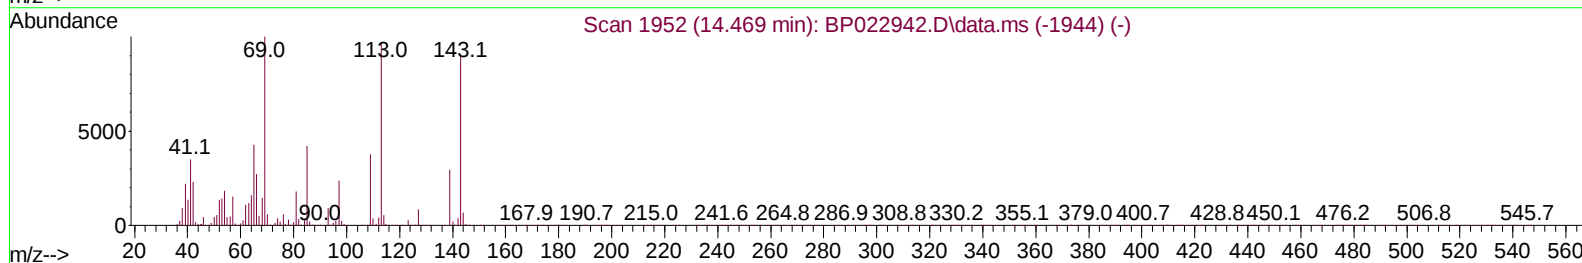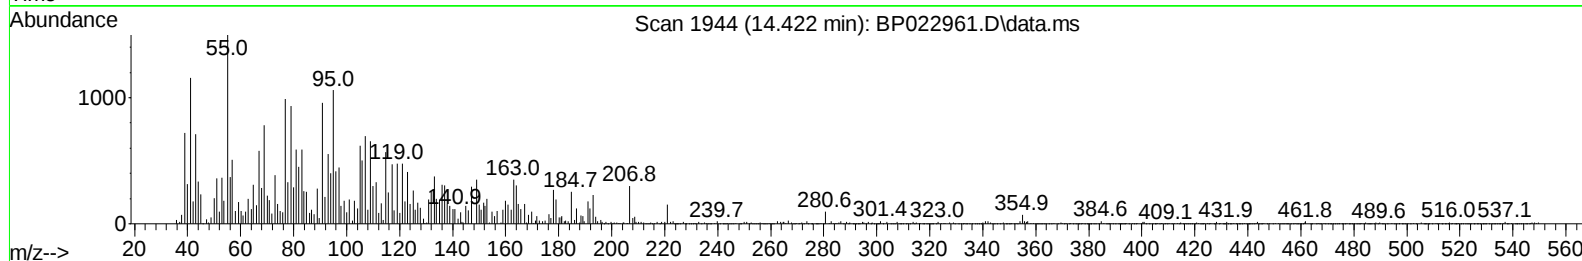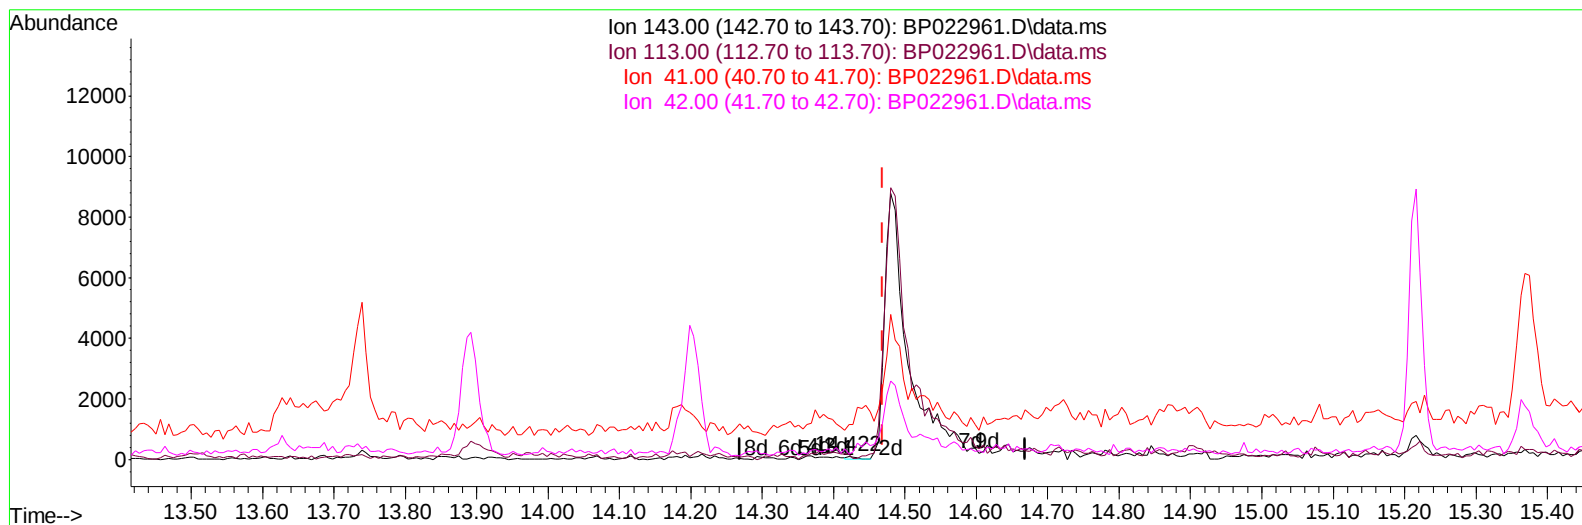

TIC: BP022961.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.422min (-0.047) 0.04 ng/u1

response 91

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	151.40#
41.00	39.20	1083.18#
42.00	25.90	165.42#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022961.D
Acq On : 09 Nov 2024 11:10
Operator : RC/JU
Sample : P4744-17
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP72

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:30:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

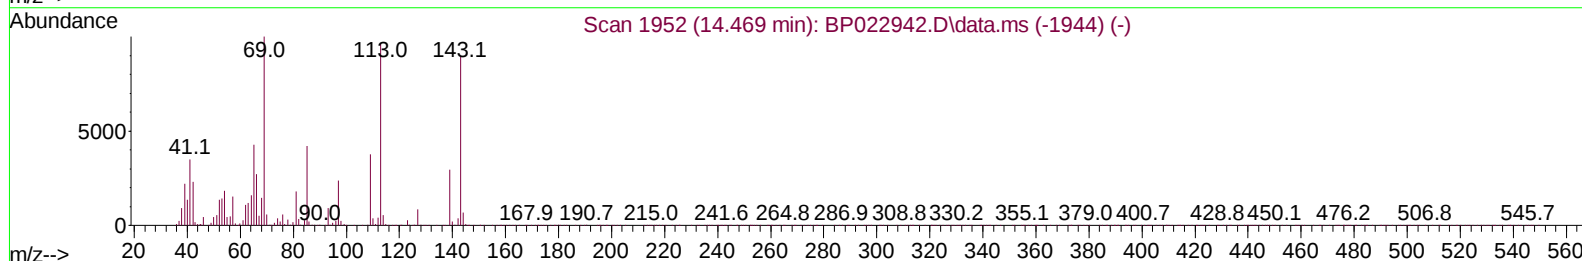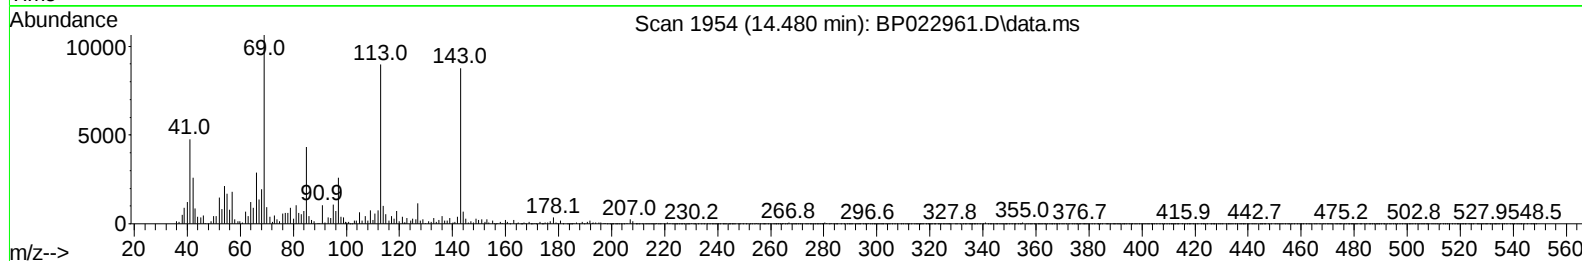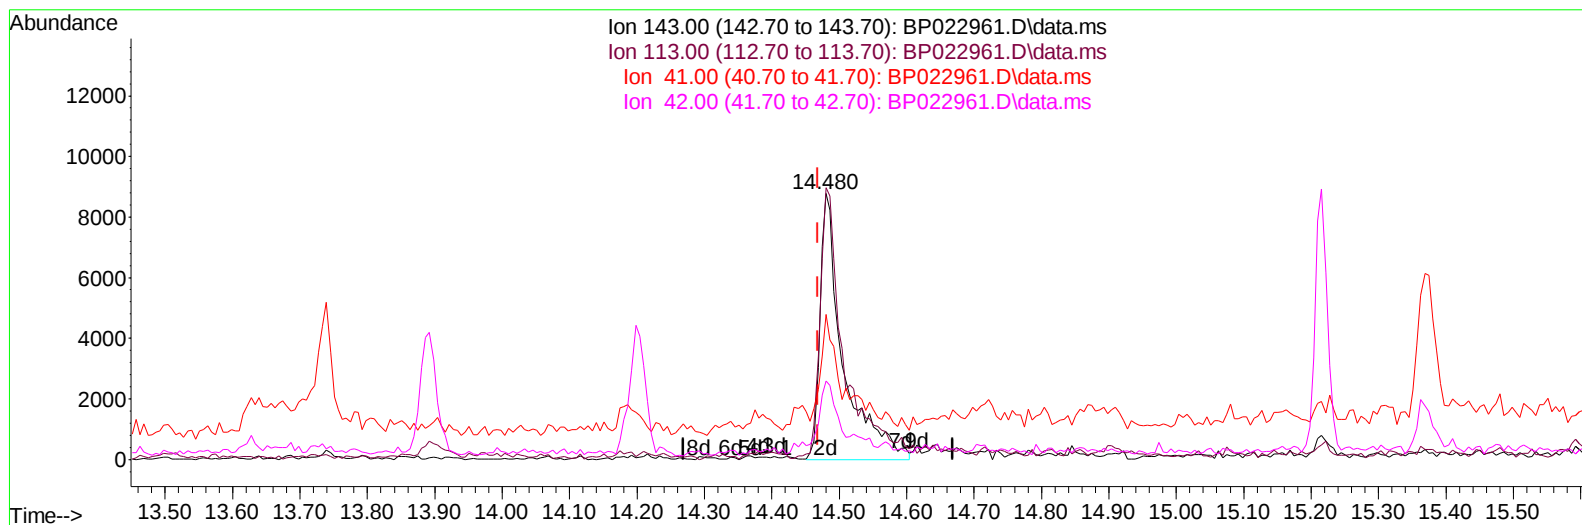

TIC: BP022961.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.480min (+ 0.012) 8.67 ng/ul m

response 20954

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	102.08
41.00	39.20	54.43#
42.00	25.90	29.40

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022961.D
 Acq On : 09 Nov 2024 11:10
 Operator : RC/JU
 Sample : P4744-17
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP72

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 09 22:31:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 08 23:49:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	69026	20.000	ng/ul	0.00
20) Naphthalene-d8	10.345	136	267531	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.204	164	223136	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.016	188	636110	20.000	ng/ul	-0.02
79) Chrysene-d12	21.445	240	800203	20.000	ng/ul	-0.01
88) Perylene-d12	24.668	264	987101	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	5691	3.963	ng/uL	0.00
4) Pyridine-d5	3.569	84	34283	8.035	ng/ul	0.01
7) Phenol-d5	6.798	99	41839	8.198	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.946	67	82677	27.575	ng/ul	0.00
11) 2-Chlorophenol-d4	7.140	132	101649	27.197	ng/ul	0.00
15) 4-Methylphenol-d8	8.304	113	83716	19.935	ng/ul	0.00
21) Nitrobenzene-d5	8.740	128	55117	29.593	ng/ul	0.00
24) 2-Nitrophenol-d4	9.451	143	69755	31.415	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.992	165	156525	33.662	ng/ul	0.00
31) 4-Chloroaniline-d4	10.492	131	122274	22.042	ng/ul	0.00
46) Dimethylphthalate-d6	13.622	166	542545	33.736	ng/ul	0.00
49) Acenaphthylene-d8	13.892	160	547425	32.623	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.480	143	20954m	8.670	ng/ul	0.01
60) Fluorene-d10	15.216	176	486021	34.470	ng/ul	-0.02
65) 4,6-Dinitro-2-methylph...	15.369	200	109198	28.656	ng/ul	0.00
73) Anthracene-d10	17.110	188	929689	34.518	ng/ul	-0.01
81) Pyrene-d10	19.504	212	1284770	34.857	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.445	264	1625646	34.574	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022961.D
Acq On : 09 Nov 2024 11:10
Operator : RC/JU
Sample : P4744-17
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP72

Manual IntegrationsAPPROVED

Quant Time: Nov 09 22:31:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

