




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022966.D
Acq On : 09 Nov 2024 14:34
Operator : RC/JU
Sample : PB164806BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK806

Manual IntegrationsAPPROVED

Quant Time: Nov 09 23:09:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

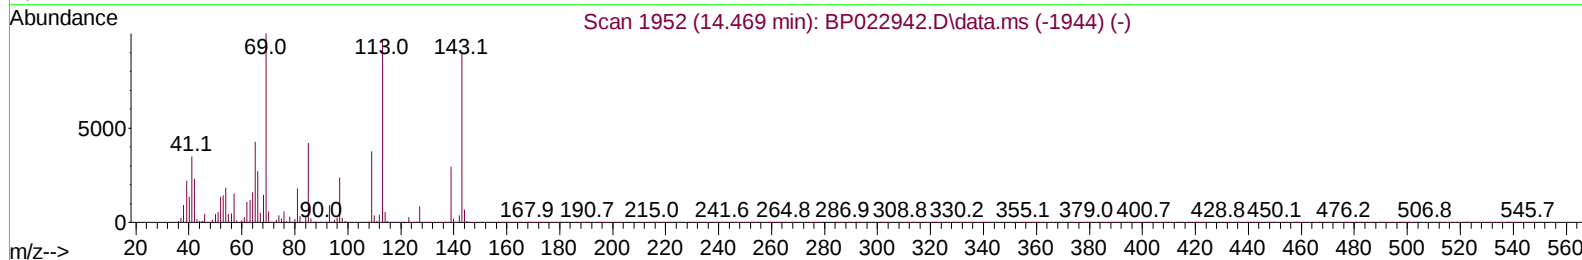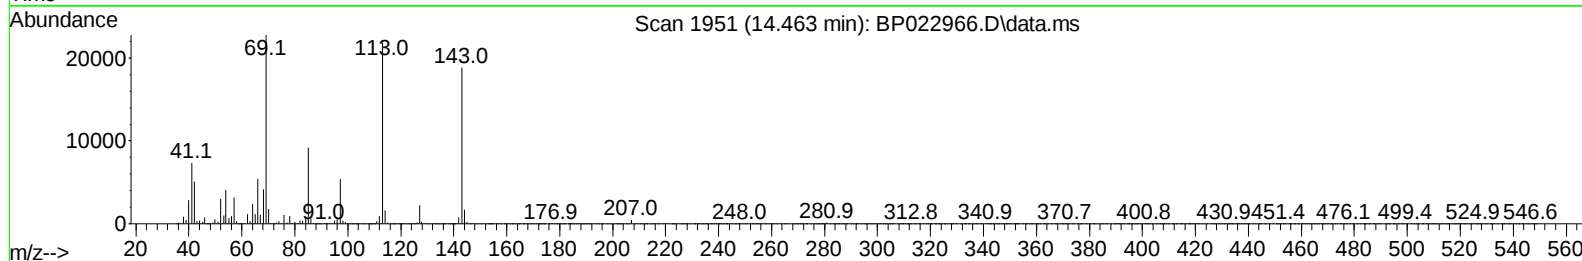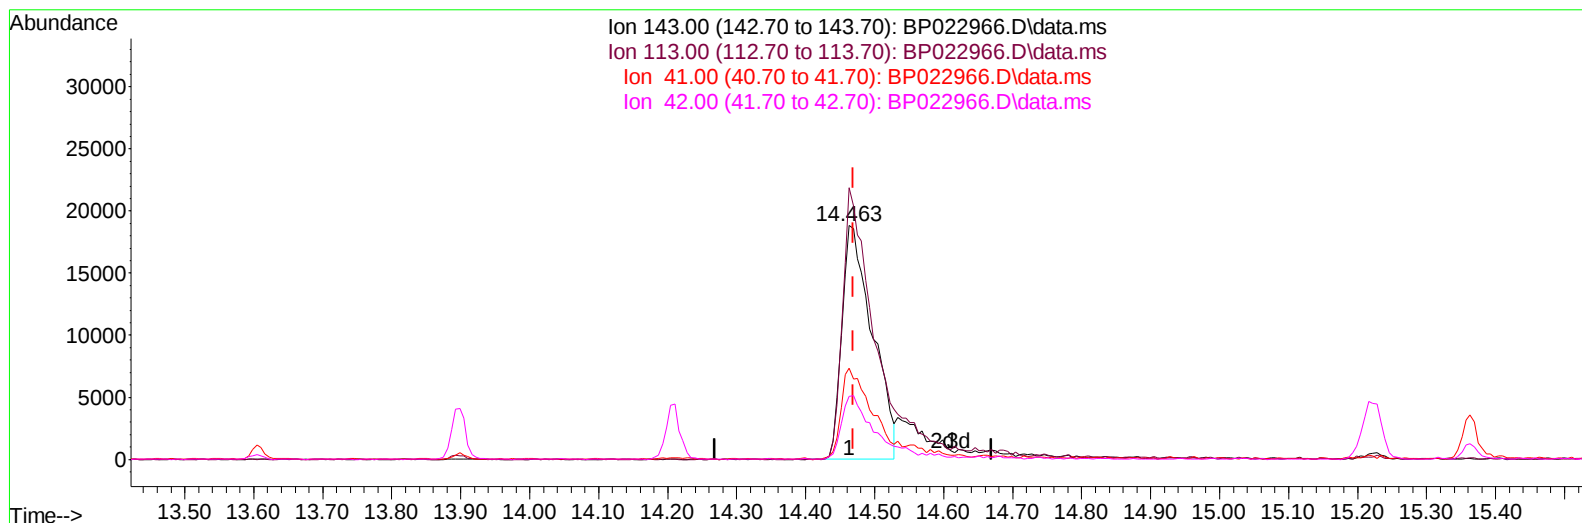

TIC: BP022966.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.463min (-0.006) 25.06 ng/u1

response 57545

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	116.16
41.00	39.20	39.18
42.00	25.90	27.06




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022966.D
Acq On : 09 Nov 2024 14:34
Operator : RC/JU
Sample : PB164806BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK806

Manual IntegrationsAPPROVED

Quant Time: Nov 09 23:09:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

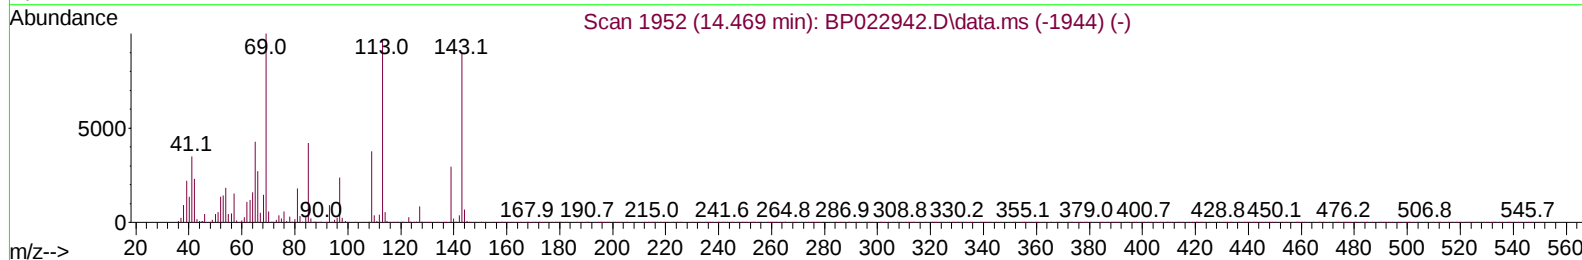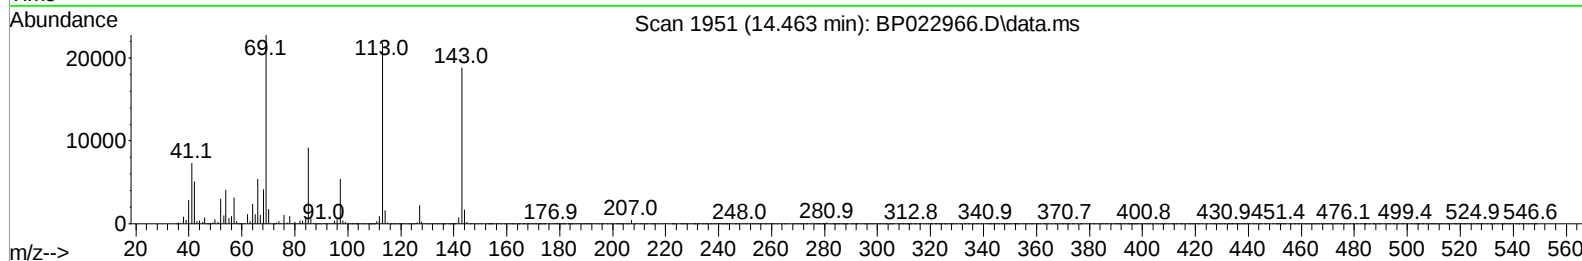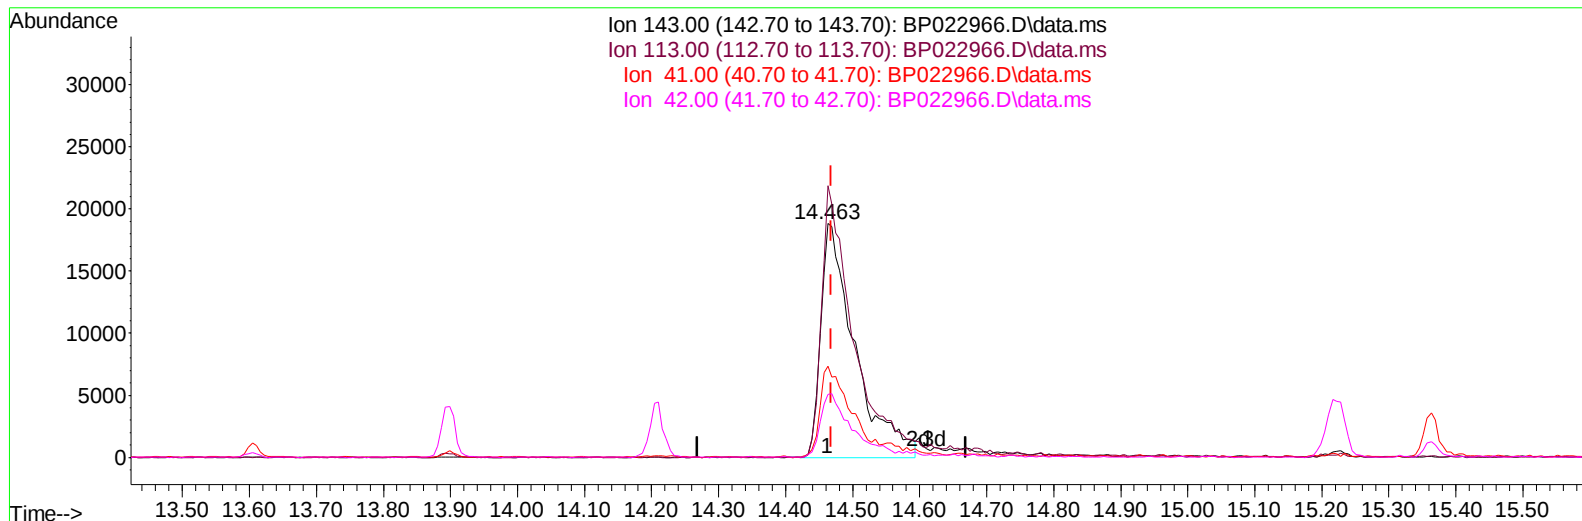

TIC: BP022966.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.463min (-0.006) 28.97 ng/ul m

response 66519

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	116.16
41.00	39.20	39.18
42.00	25.90	27.06

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022966.D
 Acq On : 09 Nov 2024 14:34
 Operator : RC/JU
 Sample : PB164806BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK806

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 09 23:10:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 08 23:49:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	66282	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.340	136	259734	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.210	164	211966	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.016	188	539307	20.000	ng/ul	-0.02
79) Chrysene-d12	21.439	240	631733	20.000	ng/ul	-0.02
88) Perylene-d12	24.674	264	715333	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	8897	6.452	ng/uL	0.00
4) Pyridine-d5	3.552	84	116697	28.484	ng/ul	0.00
7) Phenol-d5	6.793	99	148796	30.364	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.934	67	86699	30.113	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.134	132	114623	31.938	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	122933	30.485	ng/ul	0.00
21) Nitrobenzene-d5	8.728	128	57464	31.780	ng/ul	0.00
24) 2-Nitrophenol-d4	9.440	143	70126	32.531	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.987	165	134873	29.876	ng/ul	0.00
31) 4-Chloroaniline-d4	10.493	131	161913	30.063	ng/ul	0.00
46) Dimethylphthalate-d6	13.604	166	521602	34.143	ng/ul	-0.01
49) Acenaphthylene-d8	13.898	160	515512	32.340	ng/ul	0.00
54) 4-Nitrophenol-d4	14.463	143	66519m	28.974	ng/ul	0.00
60) Fluorene-d10	15.222	176	432135	32.263	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.363	200	89679	27.758	ng/ul	0.00
73) Anthracene-d10	17.116	188	769668	33.706	ng/ul	0.00
81) Pyrene-d10	19.498	212	982753	33.774	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.451	264	1162084	34.105	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022966.D
Acq On : 09 Nov 2024 14:34
Operator : RC/JU
Sample : PB164806BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK806

Manual IntegrationsAPPROVED

Quant Time: Nov 09 23:10:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

