




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022974.D
Acq On : 09 Nov 2024 19:57
Operator : RC/JU
Sample : P4746-19
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP92

Manual IntegrationsAPPROVED

Quant Time: Nov 09 23:29:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

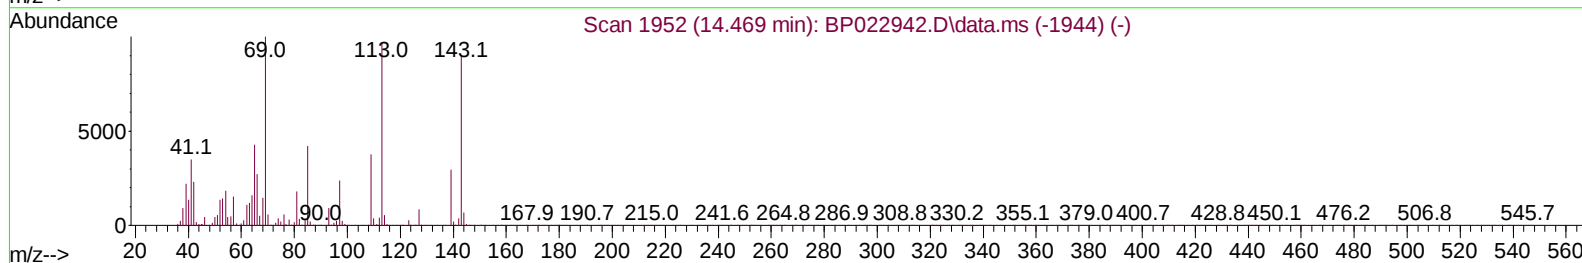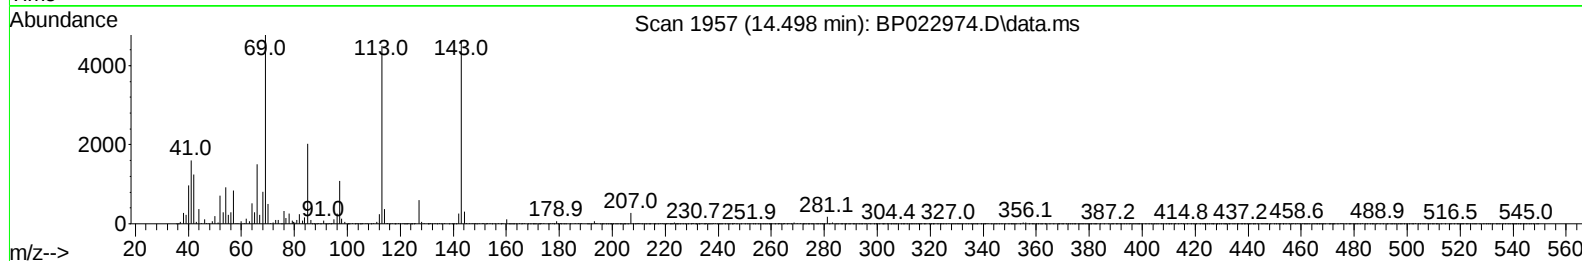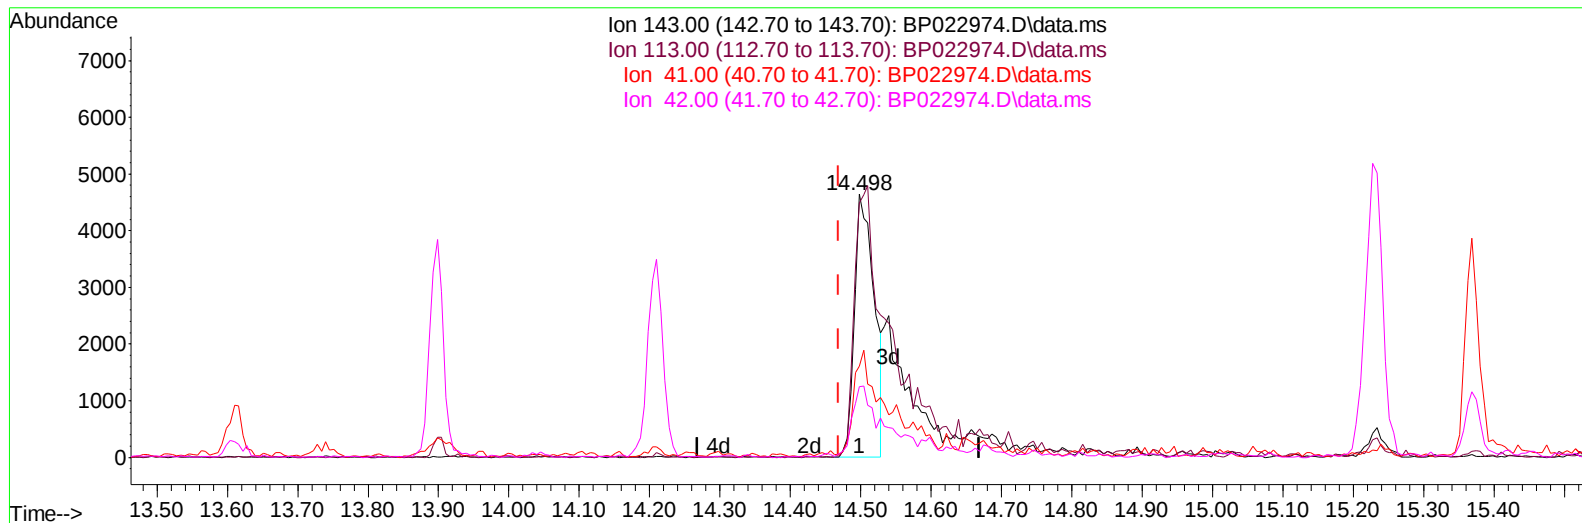

TIC: BP022974.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.498min (+ 0.029) 5.07 ng/u1

response 8958

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	96.73
41.00	39.20	34.63
42.00	25.90	26.98




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022974.D
Acq On : 09 Nov 2024 19:57
Operator : RC/JU
Sample : P4746-19
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP92

Manual IntegrationsAPPROVED

Quant Time: Nov 09 23:29:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

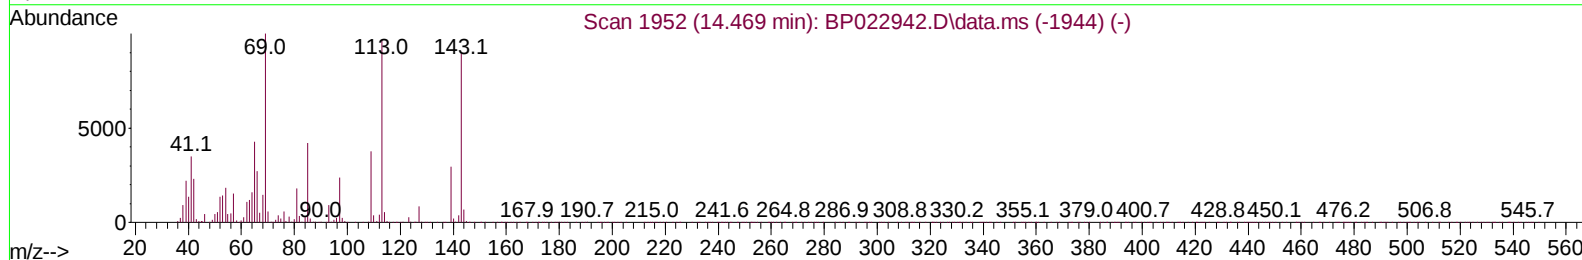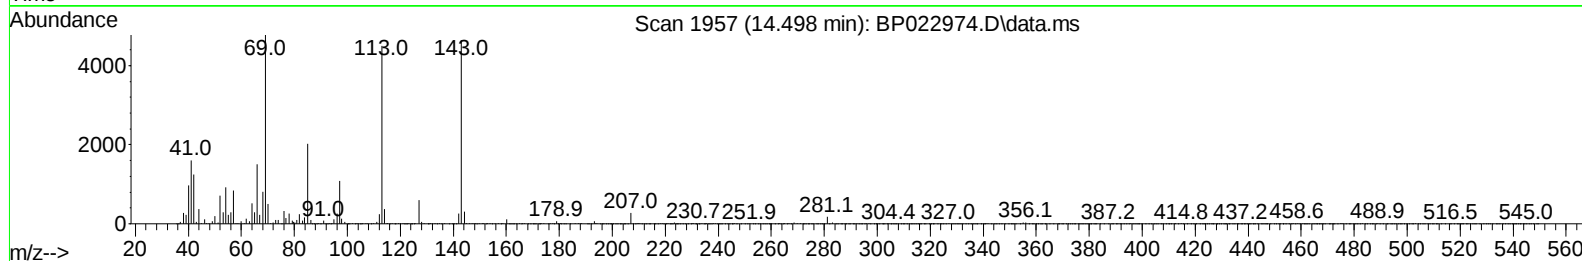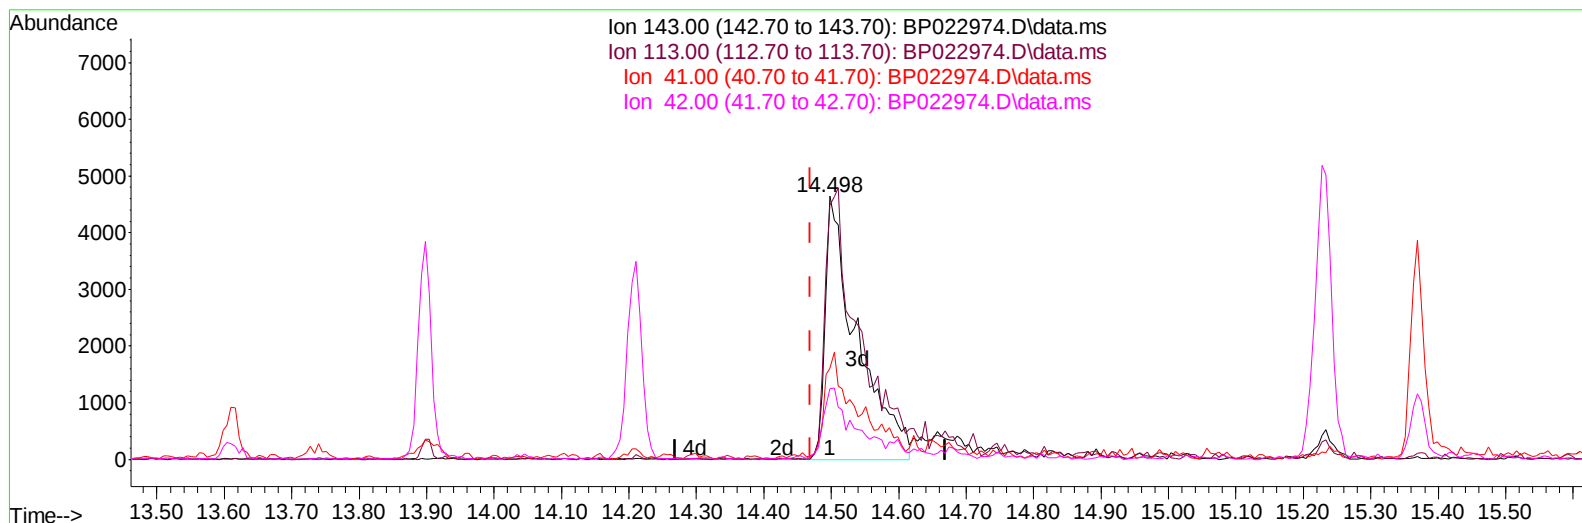

TIC: BP022974.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.498min (+ 0.029) 8.57 ng/ul m

response 15151

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	96.73
41.00	39.20	34.63
42.00	25.90	26.98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022974.D
 Acq On : 09 Nov 2024 19:57
 Operator : RC/JU
 Sample : P4746-19
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP92

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 09 23:30:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 08 23:49:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	53911	20.000	ng/ul	0.00
20) Naphthalene-d8	10.340	136	205780	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.210	164	163133	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.016	188	409575	20.000	ng/ul	-0.02
79) Chrysene-d12	21.451	240	521833	20.000	ng/ul	0.00
88) Perylene-d12	24.668	264	651079	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	5328	4.750	ng/uL	0.00
4) Pyridine-d5	3.569	84	19497	5.851	ng/ul	0.01
7) Phenol-d5	6.805	99	37670	9.451	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.940	67	68471	29.239	ng/ul	0.00
11) 2-Chlorophenol-d4	7.140	132	81397	27.884	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	69277	21.121	ng/ul	0.00
21) Nitrobenzene-d5	8.734	128	45317	31.633	ng/ul	0.00
24) 2-Nitrophenol-d4	9.451	143	53564	31.363	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.993	165	100747	28.168	ng/ul	0.00
31) 4-Chloroaniline-d4	10.493	131	107767	25.256	ng/ul	0.00
46) Dimethylphthalate-d6	13.610	166	413801	35.195	ng/ul	0.00
49) Acenaphthylene-d8	13.898	160	394127	32.126	ng/ul	0.00
54) 4-Nitrophenol-d4	14.498	143	15151m	8.575	ng/ul	0.03
60) Fluorene-d10	15.228	176	356945	34.627	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	73631	30.010	ng/ul	0.00
73) Anthracene-d10	17.116	188	653427	37.679	ng/ul	0.00
81) Pyrene-d10	19.492	212	855530	35.594	ng/ul	-0.02
92) Benzo(a)pyrene-d12	24.451	264	1144964	36.918	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022974.D
Acq On : 09 Nov 2024 19:57
Operator : RC/JU
Sample : P4746-19
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP92

Manual IntegrationsAPPROVED

Quant Time: Nov 09 23:30:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

