




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022991.D
Acq On : 10 Nov 2024 08:11
Operator : RC/JU
Sample : P4746-07
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP82

Manual IntegrationsAPPROVED

Quant Time: Nov 10 22:36:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

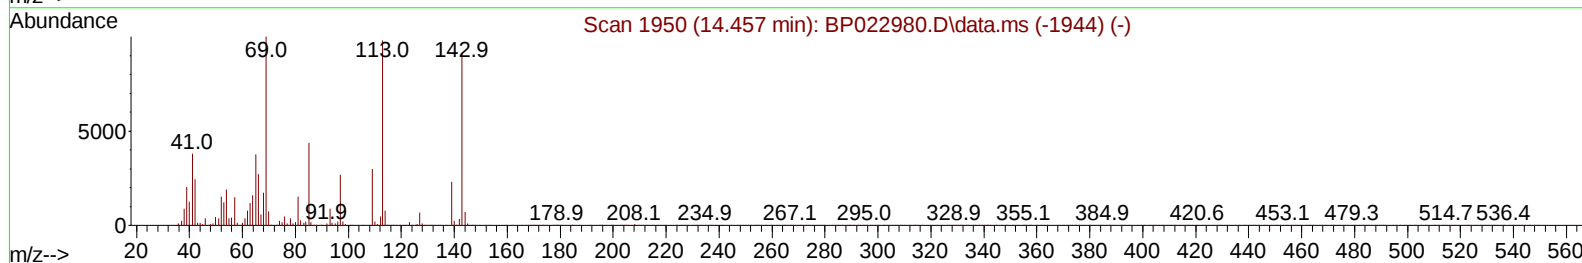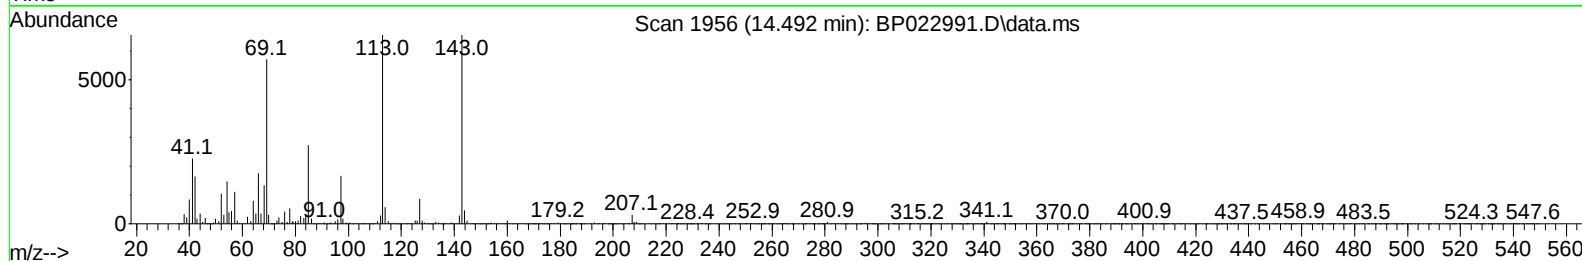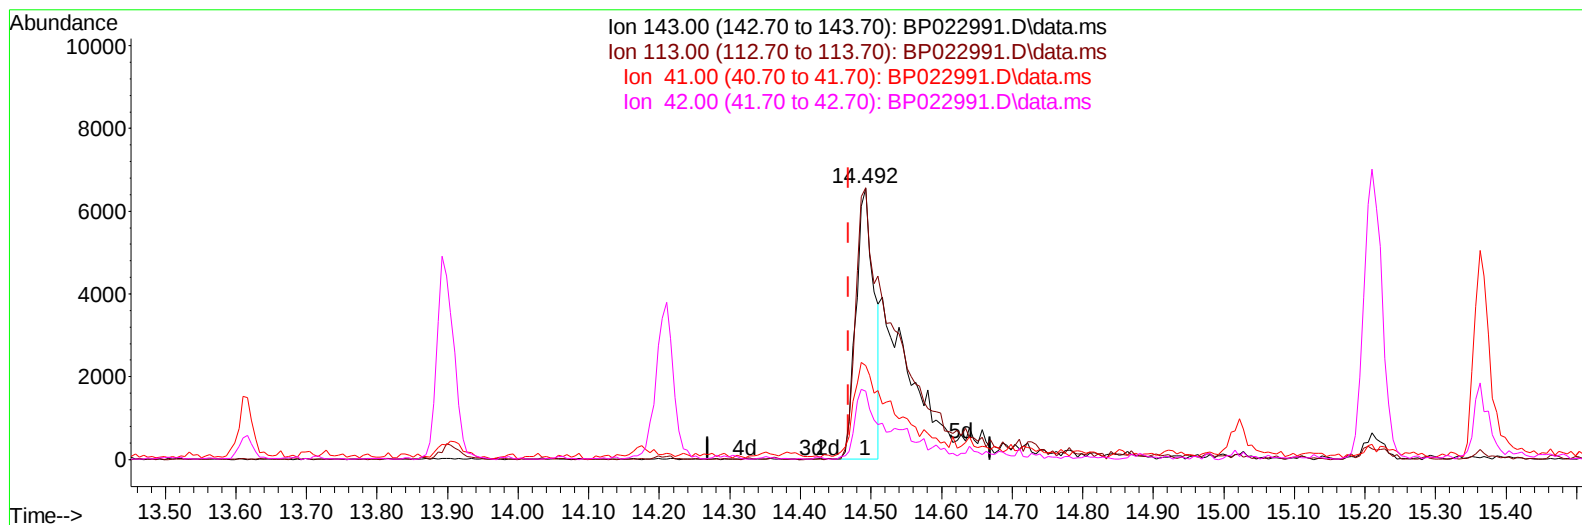

TIC: BP022991.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.492min (+ 0.024) 5.04 ng/u1

response 11718

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	100.05
41.00	39.20	34.51
42.00	25.90	25.20




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022991.D
Acq On : 10 Nov 2024 08:11
Operator : RC/JU
Sample : P4746-07
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP82

Manual IntegrationsAPPROVED

Quant Time: Nov 10 22:36:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

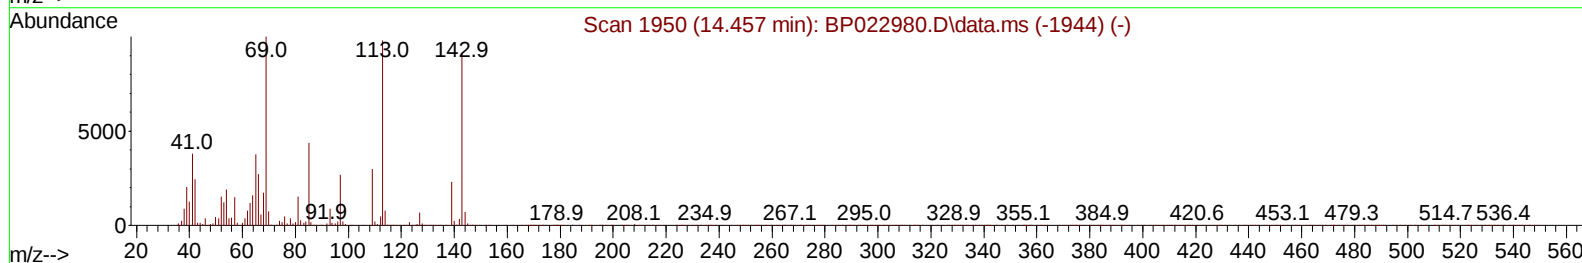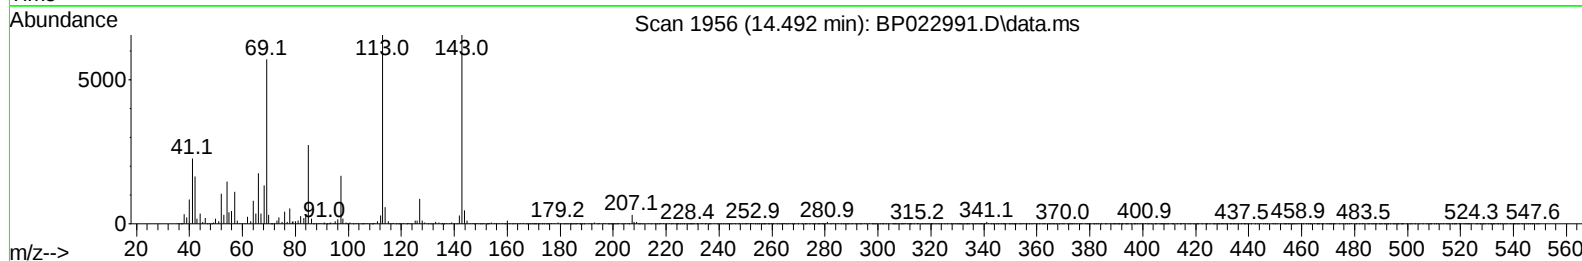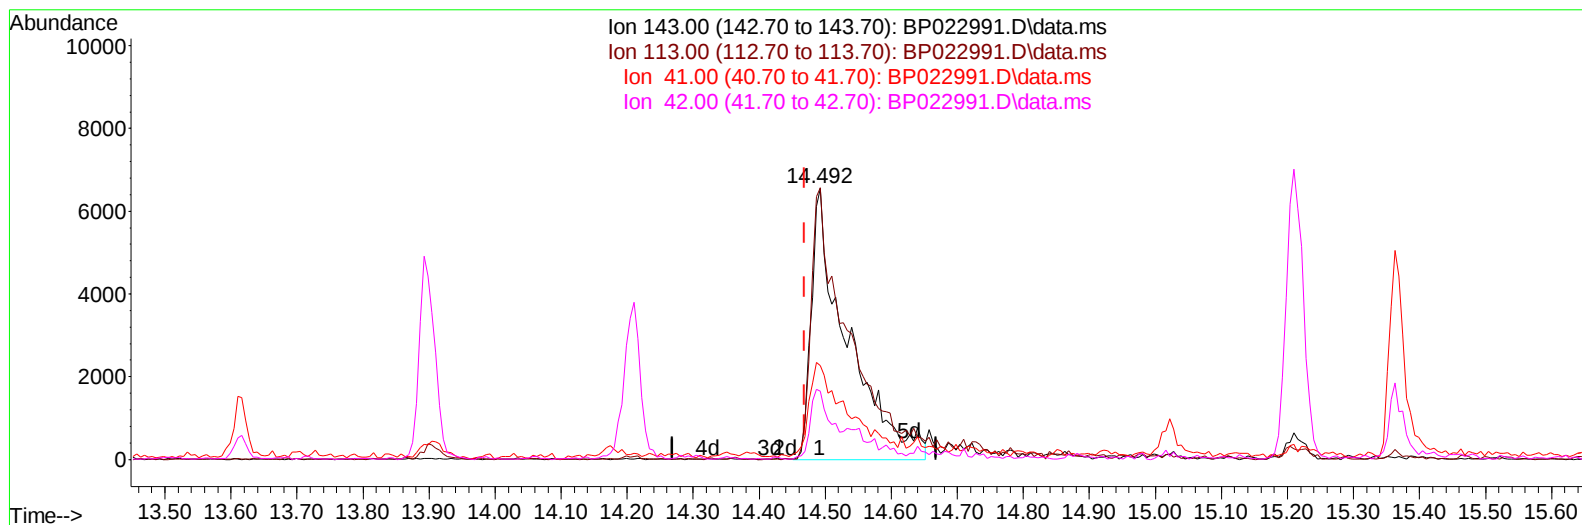

TIC: BP022991.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.492min (+ 0.024) 10.63 ng/ul m

response 24733

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	100.05
41.00	39.20	34.51
42.00	25.90	25.20

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022991.D
 Acq On : 10 Nov 2024 08:11
 Operator : RC/JU
 Sample : P4746-07
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP82

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2024
 Supervised By :mohammad ahmed 11/11/2024

Quant Time: Nov 10 22:48:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 08 23:49:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	68888	20.000	ng/ul	0.00
20) Naphthalene-d8	10.340	136	258575	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.210	164	214734	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.010	188	546936	20.000	ng/ul	#-0.02
79) Chrysene-d12	21.445	240	605470	20.000	ng/ul	-0.01
88) Perylene-d12	24.674	264	674030	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	9705	6.772	ng/uL	0.00
4) Pyridine-d5	3.558	84	46764	10.983	ng/ul	0.00
7) Phenol-d5	6.799	99	56465	11.087	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	115182	38.493	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	133212	35.713	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	104504	24.934	ng/ul	0.00
21) Nitrobenzene-d5	8.734	128	73708	40.946	ng/ul	0.00
24) 2-Nitrophenol-d4	9.446	143	91004	42.405	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.987	165	174827	38.900	ng/ul	0.00
31) 4-Chloroaniline-d4	10.493	131	186070	34.704	ng/ul	0.00
46) Dimethylphthalate-d6	13.616	166	682173	44.078	ng/ul	0.00
49) Acenaphthylene-d8	13.898	160	667566	41.339	ng/ul	0.00
54) 4-Nitrophenol-d4	14.492	143	24733m	10.634	ng/ul	0.02
60) Fluorene-d10	15.210	176	580859	42.808	ng/ul	-0.02
65) 4,6-Dinitro-2-methylph...	15.363	200	127072	38.784	ng/ul	0.00
73) Anthracene-d10	17.122	188	1042376	45.012	ng/ul	0.00
81) Pyrene-d10	19.504	212	1336151	47.911	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.451	264	1536456	47.855	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022991.D
Acq On : 10 Nov 2024 08:11
Operator : RC/JU
Sample : P4746-07
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP82

Manual IntegrationsAPPROVED

Quant Time: Nov 10 22:48:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :mohammad ahmed 11/11/2024

