

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022967.D
 Acq On : 09 Nov 2024 15:14
 Operator : RC/JU
 Sample : P4746-22
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP03

Quant Time: Nov 09 23:11:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 08 23:49:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	51050	20.000	ng/u1	0.00
20) Naphthalene-d8	10.346	136	194610	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.216	164	160131	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.022	188	411406	20.000	ng/u1	-0.01
79) Chrysene-d12	21.445	240	481665	20.000	ng/u1	-0.01
88) Perylene-d12	24.668	264	577820	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	11039	10.394	ng/uL	0.00
4) Pyridine-d5	3.558	84	111430	35.314	ng/u1	0.00
7) Phenol-d5	6.799	99	147170	38.993	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	86634	39.069	ng/u1	0.00
11) 2-Chlorophenol-d4	7.140	132	111775	40.437	ng/u1	0.00
15) 4-Methylphenol-d8	8.310	113	125021	40.253	ng/u1	0.00
21) Nitrobenzene-d5	8.740	128	55872	41.239	ng/u1	0.00
24) 2-Nitrophenol-d4	9.452	143	70140	43.425	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.993	165	135747	40.132	ng/u1	0.00
31) 4-Chloroaniline-d4	10.493	131	163301	40.468	ng/u1	0.00
46) Dimethylphthalate-d6	13.616	166	527828	45.735	ng/u1	0.00
49) Acenaphthylene-d8	13.904	160	521395	43.297	ng/u1	0.00
54) 4-Nitrophenol-d4	14.463	143	69544	40.097	ng/u1	0.00
60) Fluorene-d10	15.228	176	443273	43.808	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.375	200	97243	39.457	ng/u1	0.00
73) Anthracene-d10	17.128	188	789000	45.295	ng/u1	0.00
81) Pyrene-d10	19.498	212	1029552	46.406	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.451	264	1306228	47.458	ng/u1	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.181	88	4689	3.821	ng/uL	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022967.D
Acq On : 09 Nov 2024 15:14
Operator : RC/JU
Sample : P4746-22
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP03

Quant Time: Nov 09 23:11:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 08 23:49:48 2024
Response via : Initial Calibration

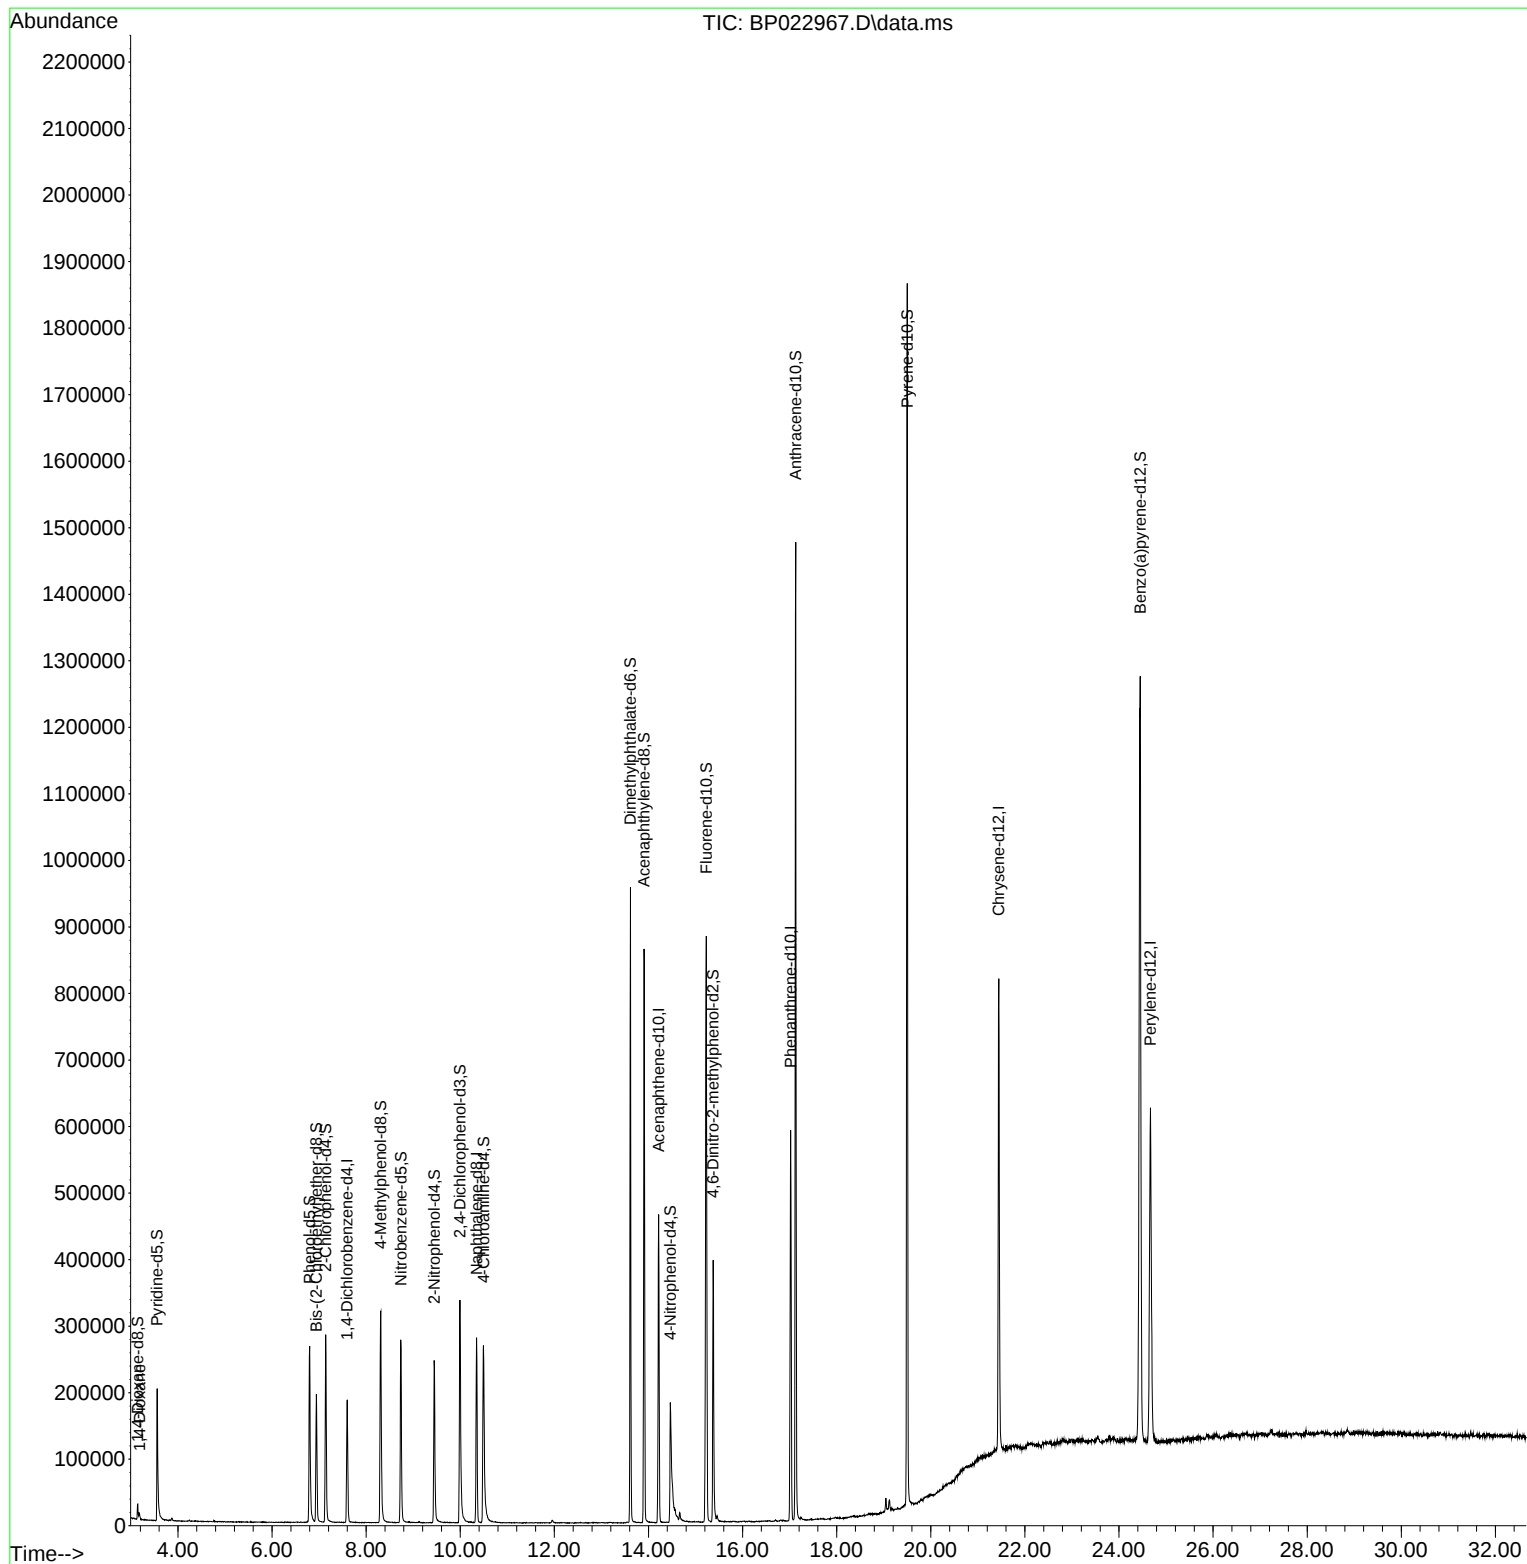

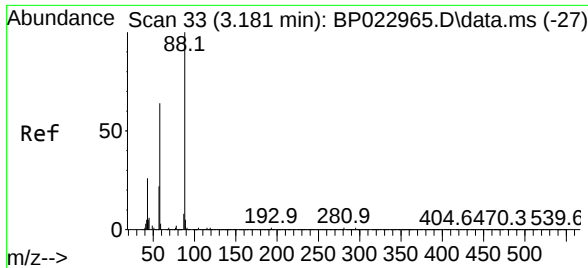

#2
 1,4-Dioxane
 Concen: 3.821 ng/uL
 RT: 3.181 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: BP022967.D
 Acq: 09 Nov 2024 15:14

Instrument :
 BNA_P
 ClientSampleId :
 GCP03

Tgt Ion: 88	Resp:	4689
Ion	Ratio	Lower Upper
88	100	
43	29.1	24.2 36.4
58	64.7	59.2 88.8

