

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022967.D
 Acq On : 09 Nov 2024 15:14
 Operator : RC/JU
 Sample : P4746-22
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	23	27	30	rBV	22946	29651	1.01%	0.135%
2	3.175	30	32	38	rVB	10233	14432	0.49%	0.066%
3	3.558	93	97	116	rBV	198295	322577	11.01%	1.465%
4	3.870	146	150	154	rBV3	3661	5603	0.19%	0.025%
5	6.799	641	648	666	rBV	264321	468303	15.98%	2.127%
6	6.940	666	672	686	rVB	191667	315868	10.78%	1.435%
7	7.140	699	706	716	rBV	281586	453681	15.48%	2.061%
8	7.599	776	784	794	rBV	184302	316087	10.79%	1.436%
9	8.310	896	905	923	rBV	317699	604843	20.64%	2.748%
10	8.734	971	977	994	rBV	274521	472066	16.11%	2.144%
11	9.446	1088	1098	1110	rBV	244361	442601	15.11%	2.011%
12	9.993	1183	1191	1216	rBV	334725	672502	22.95%	3.055%
13	10.346	1243	1251	1260	rBV	277924	436401	14.89%	1.982%
14	10.493	1268	1276	1301	rBV	266163	629229	21.48%	2.858%
15	11.957	1519	1525	1532	rBV5	3917	8538	0.29%	0.039%
16	13.545	1789	1795	1801	rBV5	1610	3710	0.13%	0.017%
17	13.616	1801	1807	1818	rBV	954572	1151965	39.32%	5.233%
18	13.904	1849	1856	1867	rBV	862689	1217450	41.55%	5.530%
19	14.216	1902	1909	1917	rBV	463153	688016	23.48%	3.125%
20	14.463	1945	1951	1967	rBV	180173	495040	16.90%	2.249%
21	14.663	1982	1985	1995	rVB5	11832	20406	0.70%	0.093%
22	15.228	2071	2081	2098	rBV	880844	1635234	55.81%	7.428%
23	15.375	2098	2106	2117	rBV	393689	593378	20.25%	2.696%
24	15.457	2117	2120	2129	rVB3	8737	16354	0.56%	0.074%
25	17.022	2378	2386	2395	rBV	587098	968695	33.06%	4.400%
26	17.128	2397	2404	2420	rVV	1469798	1956976	66.79%	8.890%
27	17.239	2420	2423	2430	rVB9	4074	7080	0.24%	0.032%
28	19.045	2725	2730	2733	rBV2	21307	29836	1.02%	0.136%
29	19.122	2739	2743	2747	rVB	14393	21540	0.74%	0.098%
30	19.498	2801	2807	2818	rBV	1833881	2502083	85.40%	11.366%
31	21.445	3132	3138	3149	rVB2	704764	1258910	42.97%	5.719%
32	24.451	3639	3649	3661	rVB	1147985	2929913	100.00%	13.310%
33	24.668	3677	3686	3698	rVB	495960	1324600	45.21%	6.017%




Sum of corrected areas: 22013568

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022967.D
Acq On : 09 Nov 2024 15:14
Operator : RC/JU
Sample : P4746-22
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

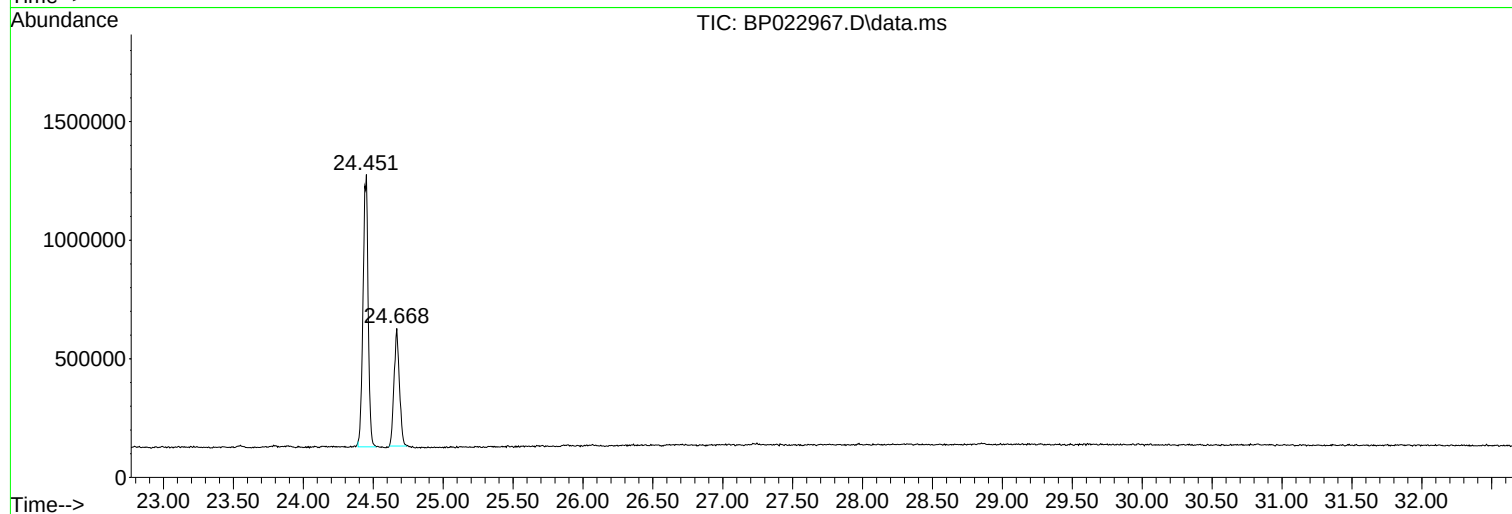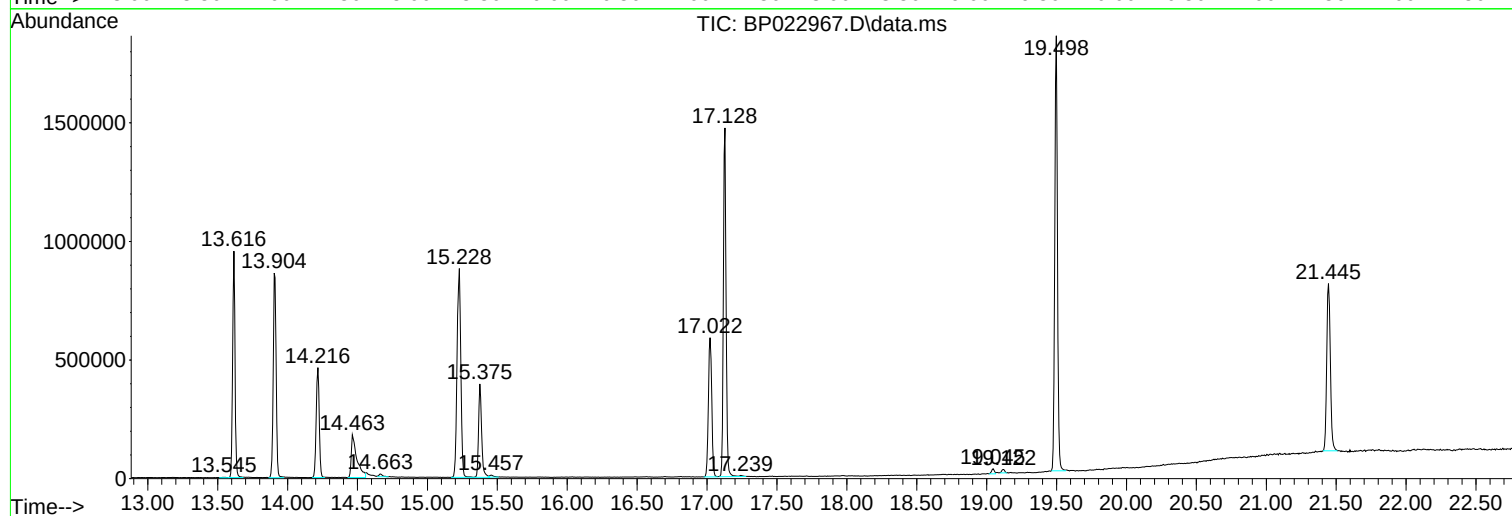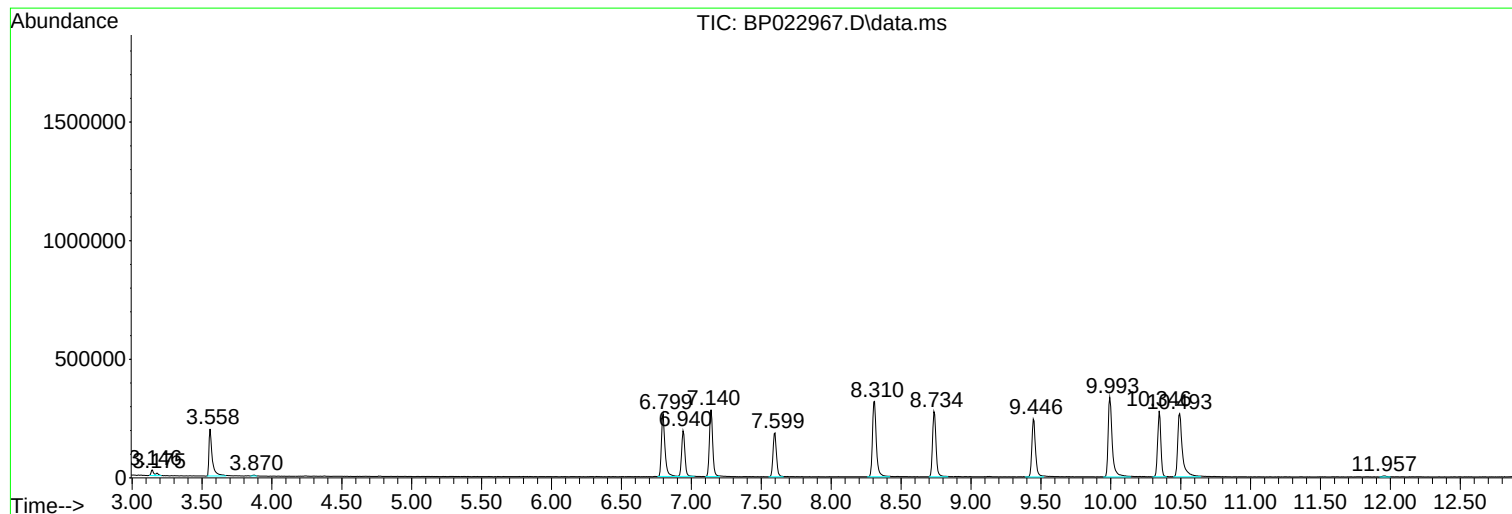

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022967.D
Acq On : 09 Nov 2024 15:14
Operator : RC/JU
Sample : P4746-22
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022967.D
Acq On : 09 Nov 2024 15:14
Operator : RC/JU
Sample : P4746-22
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP03

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc