

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022969.D
 Acq On : 09 Nov 2024 16:35
 Operator : RC/JU
 Sample : P4744-22
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	16	21	24	rBV	22231	29608	1.09%	0.149%
2	3.140	24	26	30	rVB	11268	13102	0.48%	0.066%
3	3.564	94	98	114	rBV	52885	98722	3.63%	0.498%
4	3.870	146	150	155	rVB4	4067	6489	0.24%	0.033%
5	4.381	233	237	243	rVB4	8578	12673	0.47%	0.064%
6	6.734	635	637	642	rVV4	2274	2893	0.11%	0.015%
7	6.805	642	649	666	rVV	50596	111562	4.11%	0.563%
8	6.940	666	672	688	rVB	168620	269317	9.91%	1.359%
9	7.140	699	706	723	rBV	196963	342923	12.62%	1.731%
10	7.593	776	783	794	rBV	207126	354579	13.05%	1.789%
11	8.305	897	904	921	rBV2	160325	327075	12.04%	1.651%
12	8.740	971	978	997	rBV	223898	396676	14.60%	2.002%
13	8.887	997	1003	1004	rBV6	1952	2936	0.11%	0.015%
14	9.128	1041	1044	1049	rVB5	3537	4790	0.18%	0.024%
15	9.452	1090	1099	1110	rBV	191205	355747	13.09%	1.795%
16	9.987	1183	1190	1215	rBV	266808	537977	19.80%	2.715%
17	10.346	1243	1251	1260	rBV	284797	488654	17.98%	2.466%
18	10.493	1268	1276	1298	rBV	262751	490349	18.04%	2.475%
19	11.604	1461	1465	1470	rVB6	2982	4387	0.16%	0.022%
20	11.951	1519	1524	1531	rBV5	4421	8589	0.32%	0.043%
21	13.098	1712	1719	1722	rBV7	1771	3301	0.12%	0.017%
22	13.628	1801	1809	1819	rBV	638384	966314	35.56%	4.877%
23	13.898	1844	1855	1867	rBV2	523478	988712	36.38%	4.990%
24	14.210	1899	1908	1918	rBV	429278	766382	28.20%	3.868%
25	14.498	1949	1957	1960	rBV3	23902	44816	1.65%	0.226%
26	14.622	1976	1978	1987	rVB10	2824	4318	0.16%	0.022%
27	15.216	2073	2079	2094	rBV	1081957	1421979	52.33%	7.176%
28	15.381	2100	2107	2119	rBV	310335	521027	19.17%	2.629%
29	15.475	2120	2123	2128	rVB5	7099	10457	0.38%	0.053%
30	15.604	2138	2145	2150	rBV	45191	65097	2.40%	0.329%
31	15.816	2176	2181	2185	rBV7	1647	3329	0.12%	0.017%
32	16.022	2210	2216	2223	rBV7	1792	4527	0.17%	0.023%
33	16.145	2232	2237	2239	rBV5	4055	5752	0.21%	0.029%
34	16.181	2239	2243	2247	rVB2	11738	14004	0.52%	0.071%
35	16.428	2280	2285	2286	rBV5	2044	2801	0.10%	0.014%
36	16.492	2292	2296	2300	rBV7	2563	4489	0.17%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022969.D
 Acq On : 09 Nov 2024 16:35
 Operator : RC/JU
 Sample : P4744-22
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	16.545	2300	2305	2311	rVB8	11530	16980	0.62%	0.086%
38	17.016	2378	2385	2395	rBV	675039	1072614	39.47%	5.413%
39	17.128	2396	2404	2420	rBV2	1033401	1771073	65.17%	8.938%
40	17.528	2467	2472	2478	rBV	29512	45667	1.68%	0.230%
41	17.710	2498	2503	2509	rVB3	28179	42531	1.57%	0.215%
42	17.957	2540	2545	2552	rBV4	26169	42618	1.57%	0.215%
43	18.175	2577	2582	2592	rVB2	31125	48400	1.78%	0.244%
44	18.257	2593	2596	2601	rBV6	3478	6236	0.23%	0.031%
45	18.822	2689	2692	2698	rBV8	5635	11439	0.42%	0.058%
46	19.051	2727	2731	2736	rBV3	19050	29080	1.07%	0.147%
47	19.128	2740	2744	2748	rVV	18840	30297	1.11%	0.153%
48	19.163	2748	2750	2758	rVB9	7552	15247	0.56%	0.077%
49	19.286	2768	2771	2780	rVB9	11802	16528	0.61%	0.083%
50	19.504	2802	2808	2816	rBV	1904812	2307171	84.90%	11.644%
51	21.451	3133	3139	3151	rBV2	930828	1460838	53.76%	7.372%
52	24.445	3639	3648	3665	rVB	1057066	2717490	100.00%	13.714%
53	24.674	3678	3687	3699	rVB	539835	1494475	54.99%	7.542%




Sum of corrected areas: 19815037

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022969.D
Acq On : 09 Nov 2024 16:35
Operator : RC/JU
Sample : P4744-22
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP75

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

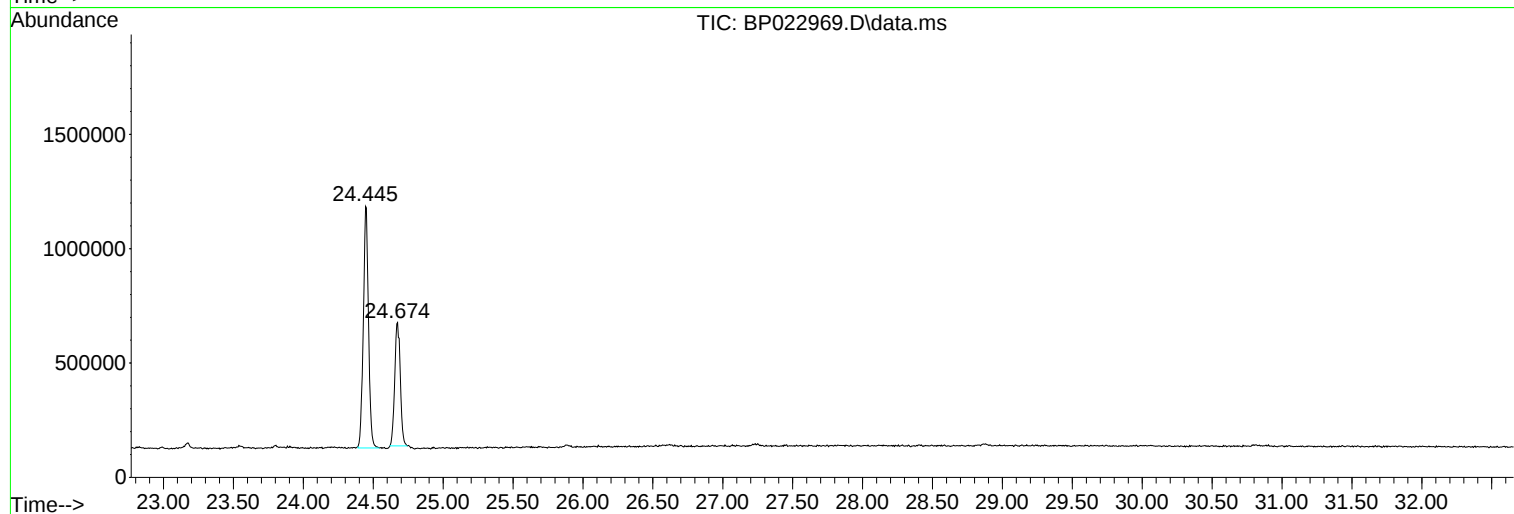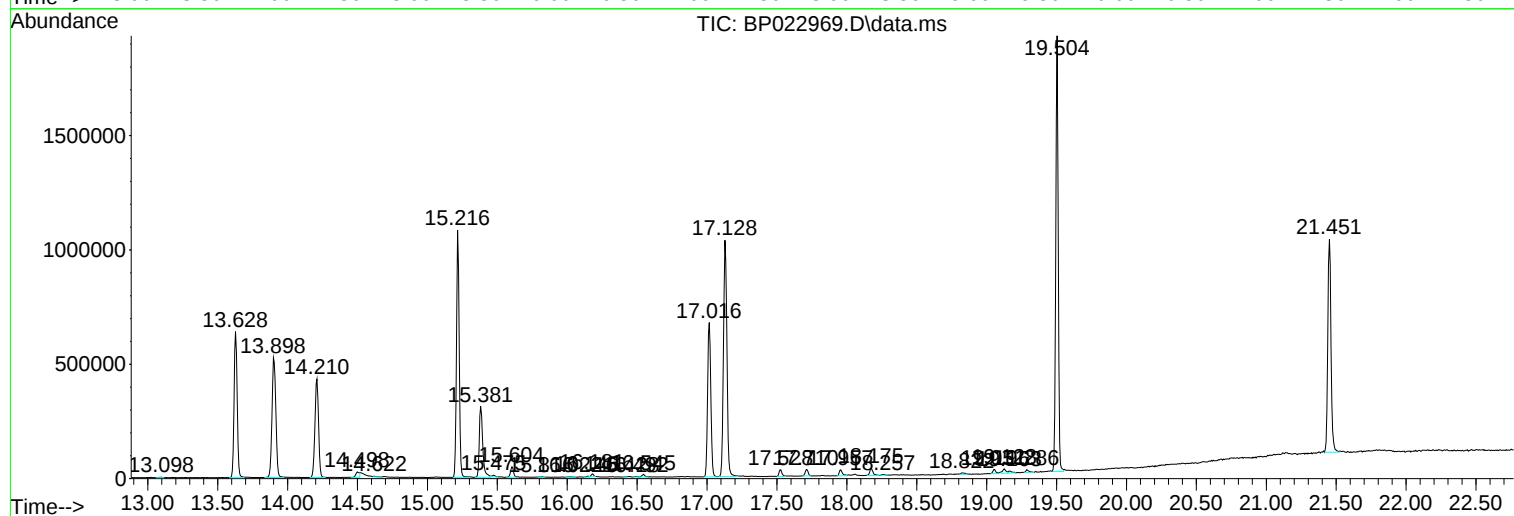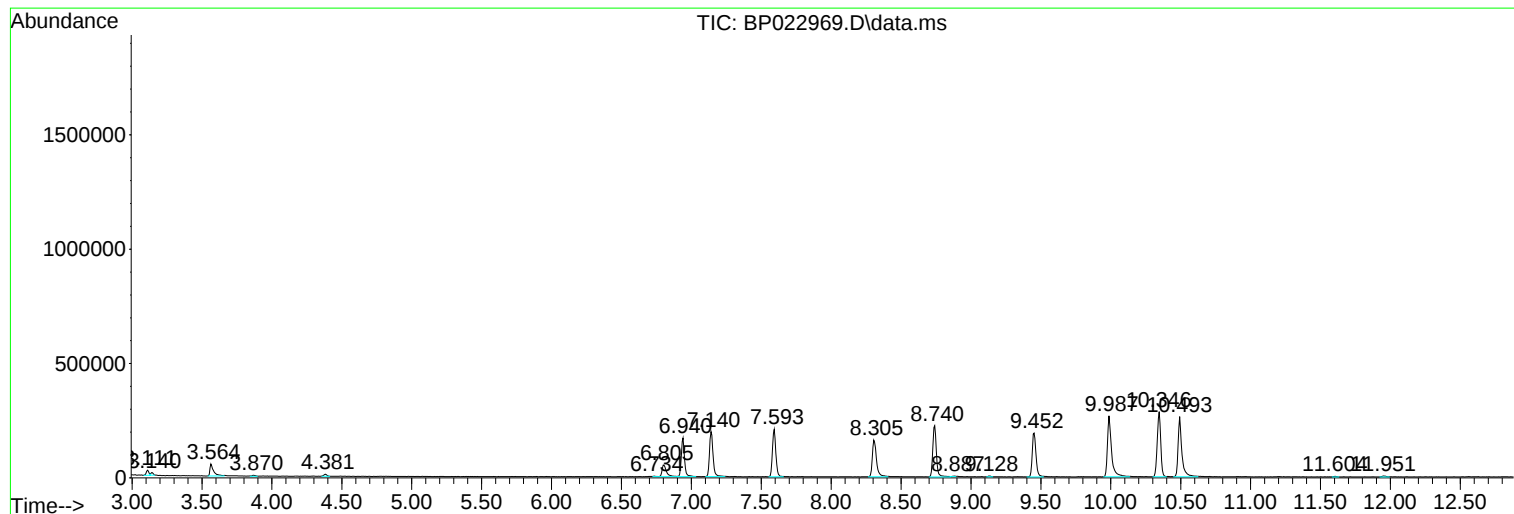

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022969.D
Acq On : 09 Nov 2024 16:35
Operator : RC/JU
Sample : P4744-22
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP75

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022969.D
Acq On : 09 Nov 2024 16:35
Operator : RC/JU
Sample : P4744-22
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP75

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------