

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022971.D
 Acq On : 09 Nov 2024 17:56
 Operator : RC/JU
 Sample : P4746-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	17	21	25	rBV	32730	44733	1.48%	0.202%
2	3.146	25	27	34	rVB	12227	13973	0.46%	0.063%
3	3.569	95	99	113	rBV	39357	71321	2.36%	0.322%
4	3.869	146	150	155	rBV4	3661	4876	0.16%	0.022%
5	6.805	643	649	666	rBB	55116	111778	3.70%	0.504%
6	6.946	666	673	687	rBV	182304	306236	10.14%	1.381%
7	7.140	700	706	726	rBV	223002	388743	12.88%	1.753%
8	7.593	776	783	795	rBV	245881	406005	13.45%	1.831%
9	8.304	894	904	923	rBV	186758	352993	11.69%	1.592%
10	8.734	970	977	995	rBV	252384	458384	15.18%	2.068%
11	8.875	997	1001	1011	rVB9	4083	10249	0.34%	0.046%
12	9.128	1039	1044	1050	rVB2	7220	11369	0.38%	0.051%
13	9.446	1089	1098	1116	rBV	235702	417237	13.82%	1.882%
14	9.987	1183	1190	1213	rBV	299717	611263	20.25%	2.757%
15	10.340	1242	1250	1262	rBV	322364	544188	18.03%	2.455%
16	10.487	1269	1275	1293	rBV	230027	472698	15.66%	2.132%
17	11.598	1459	1464	1470	rVB6	3045	6095	0.20%	0.027%
18	11.951	1517	1524	1529	rBV5	3763	7671	0.25%	0.035%
19	13.104	1715	1720	1726	rVB4	3741	5831	0.19%	0.026%
20	13.534	1786	1793	1799	rBV10	2074	5283	0.18%	0.024%
21	13.604	1799	1805	1817	rVV	717381	1111161	36.81%	5.012%
22	13.898	1849	1855	1871	rVB	795942	1107243	36.68%	4.994%
23	14.216	1902	1909	1920	rBV	662699	850089	28.16%	3.834%
24	14.504	1950	1958	1959	rBV3	26324	39314	1.30%	0.177%
25	14.675	1985	1987	1993	rVB7	2552	3689	0.12%	0.017%
26	15.057	2049	2052	2059	rVB7	2363	3280	0.11%	0.015%
27	15.234	2074	2082	2095	rBV	1029372	1577864	52.27%	7.117%
28	15.369	2099	2105	2117	rVV	351886	581253	19.25%	2.622%
29	15.469	2120	2122	2130	rVB5	6157	10823	0.36%	0.049%
30	15.604	2137	2145	2159	rVB	52843	73001	2.42%	0.329%
31	16.175	2234	2242	2249	rBV2	12127	23108	0.77%	0.104%
32	17.022	2379	2386	2394	rBV	797332	1183515	39.20%	5.338%
33	17.116	2395	2402	2413	rVV	1488912	1969976	65.26%	8.886%
34	17.451	2454	2459	2461	rBV5	2212	4140	0.14%	0.019%
35	17.510	2465	2469	2473	rBV2	14708	21936	0.73%	0.099%
36	17.710	2499	2503	2510	rBV6	13900	20000	0.66%	0.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022971.D
 Acq On : 09 Nov 2024 17:56
 Operator : RC/JU
 Sample : P4746-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	17.822	2518	2522	2525	rBV6	2598	3246	0.11%	0.015%
38	17.951	2539	2544	2554	rBV3	17454	32846	1.09%	0.148%
39	18.027	2554	2557	2560	rBV	3860	5155	0.17%	0.023%
40	18.163	2574	2580	2603	rBV	220086	401671	13.31%	1.812%
41	18.822	2688	2692	2698	rVB5	8551	13251	0.44%	0.060%
42	19.045	2724	2730	2734	rBV	18515	31845	1.05%	0.144%
43	19.127	2740	2744	2747	rBV	19365	28662	0.95%	0.129%
44	19.163	2748	2750	2758	rVB9	12713	17020	0.56%	0.077%
45	19.292	2768	2772	2776	rBV6	9834	13419	0.44%	0.061%
46	19.504	2801	2808	2816	rBV	1641777	2516653	83.37%	11.351%
47	21.451	3132	3139	3151	rBV	891075	1607759	53.26%	7.252%
48	24.462	3641	3651	3666	rVB	1205398	3018835	100.00%	13.616%
49	24.674	3678	3687	3700	rBV	563887	1648808	54.62%	7.437%




Sum of corrected areas: 22170488

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022971.D
Acq On : 09 Nov 2024 17:56
Operator : RC/JU
Sample : P4746-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

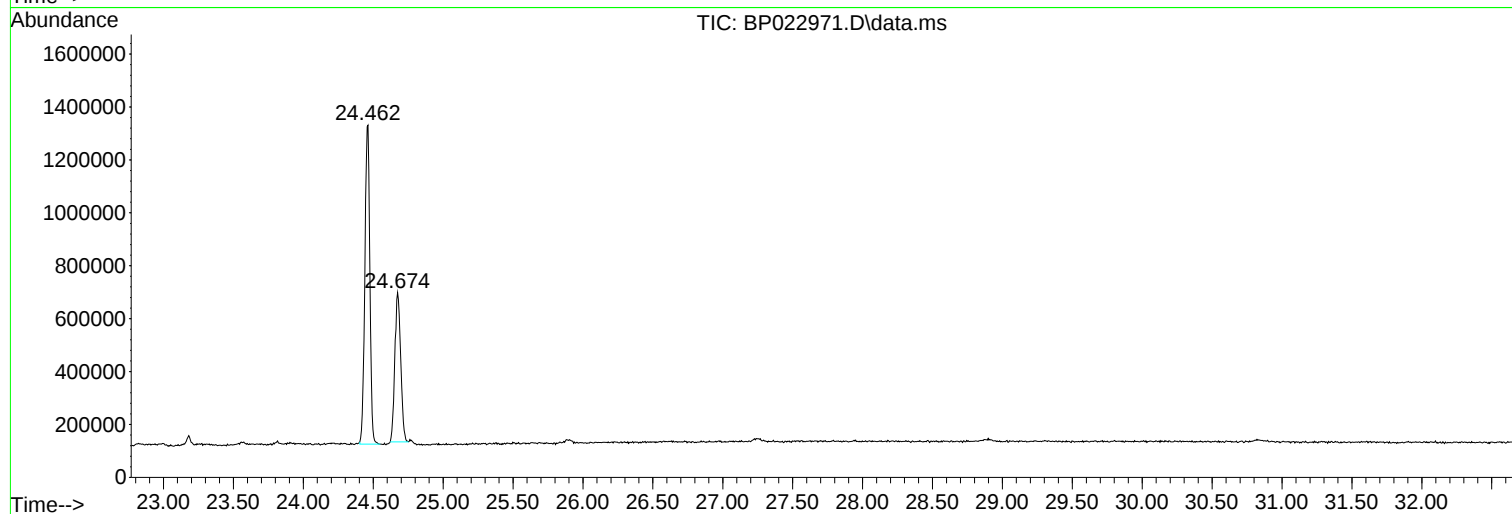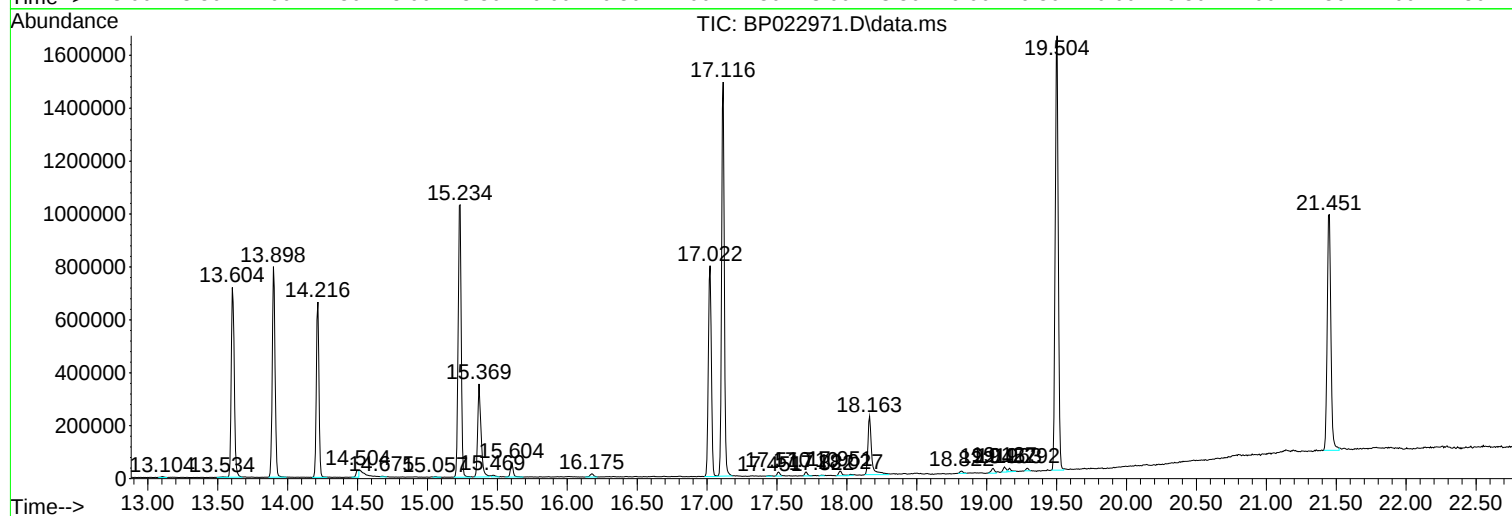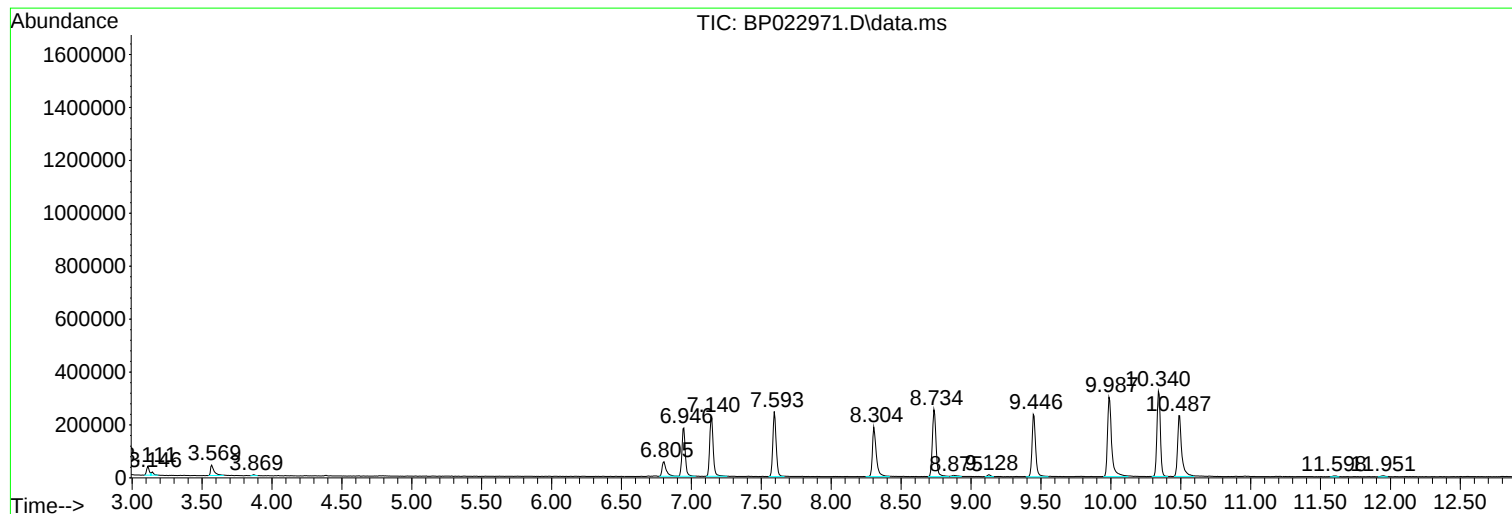

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022971.D
Acq On : 09 Nov 2024 17:56
Operator : RC/JU
Sample : P4746-02
Misc :
ALS Vial : 56 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
GCP77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 3,5-di-tert-Butyl-4-hydroxy... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
18.163	6.79 ng/ul	401671	Phenanthrene-d10	17.022	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	3,5-di-tert-Butyl-4-hydroxypheny...	278	C17H26O3	020170-32-5	97
2	Lycopodan-5-one, 12-hydroxy-15-m...	263	C16H25NO2	021061-90-5	91
3	4,6-Dinitro-1,1,3,3,5-pentamethy...	278	C14H18N2O4	000116-66-5	72
4	Cyanic acid, (1-methylethylidene...	278	C17H14N2O2	001156-51-0	68
5	3,5-di-tert-Butyl-4-hydroxypheny...	278	C17H26O3	020170-32-5	64

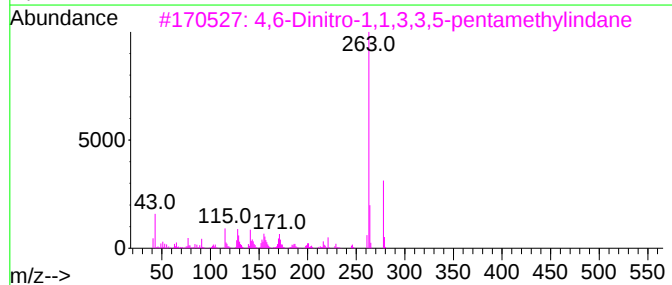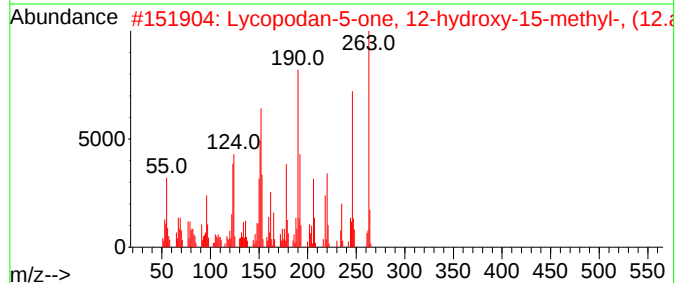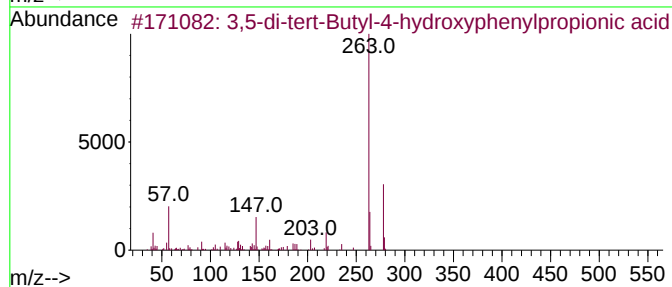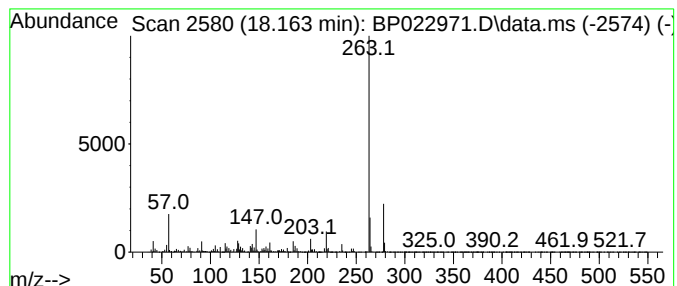

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022971.D
Acq On : 09 Nov 2024 17:56
Operator : RC/JU
Sample : P4746-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
3,5-di-tert-But...	18.163	6.8	ng/u1	401671	4	17.022	1183520	20.0