

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022976.D
 Acq On : 09 Nov 2024 21:18
 Operator : RC/JU
 Sample : P4746-21
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	23	26	29	rBV	12410	15233	0.54%	0.073%
2	3.181	29	33	39	rVB	26292	34576	1.22%	0.165%
3	3.564	95	98	110	rBV	47023	83185	2.93%	0.396%
4	3.863	144	149	154	rBV	7537	10523	0.37%	0.050%
5	4.040	171	179	187	rVB	28777	50627	1.78%	0.241%
6	4.787	299	306	311	rBV3	2653	4831	0.17%	0.023%
7	5.205	370	377	386	rVB2	9492	20422	0.72%	0.097%
8	6.734	631	637	642	rBV4	2036	4344	0.15%	0.021%
9	6.799	642	648	664	rVV2	71165	145724	5.14%	0.694%
10	6.934	664	671	685	rVV	180507	303014	10.68%	1.443%
11	7.140	698	706	723	rVV	232021	391378	13.80%	1.863%
12	7.587	776	782	795	rBV	222730	375985	13.25%	1.790%
13	8.299	896	903	922	rBV	200529	388483	13.70%	1.850%
14	8.734	970	977	991	rBV	245495	432373	15.24%	2.059%
15	9.134	1037	1045	1050	rBV2	14623	22566	0.80%	0.107%
16	9.440	1090	1097	1113	rBV2	203892	401526	14.16%	1.912%
17	9.646	1127	1132	1138	rVB9	2117	4803	0.17%	0.023%
18	9.987	1183	1190	1216	rBV	293505	596720	21.04%	2.841%
19	10.340	1243	1250	1263	rVB	310225	511186	18.02%	2.434%
20	10.487	1266	1275	1295	rBV	246032	504513	17.79%	2.402%
21	10.898	1335	1345	1349	rBV5	4697	11966	0.42%	0.057%
22	10.951	1349	1354	1362	rVB3	5401	12003	0.42%	0.057%
23	11.028	1362	1367	1369	rBV5	1552	2838	0.10%	0.014%
24	11.128	1378	1384	1389	rVB6	2846	4476	0.16%	0.021%
25	11.598	1454	1464	1470	rBV2	35257	62161	2.19%	0.296%
26	11.657	1470	1474	1481	rVB7	3707	6441	0.23%	0.031%
27	11.957	1519	1525	1533	rBV4	4395	8343	0.29%	0.040%
28	12.134	1552	1555	1561	rVB8	2945	4634	0.16%	0.022%
29	12.728	1650	1656	1663	rBV2	13312	22231	0.78%	0.106%
30	12.798	1663	1668	1674	rVB8	1651	3364	0.12%	0.016%
31	13.104	1713	1720	1726	rBV7	5769	9937	0.35%	0.047%
32	13.616	1800	1807	1822	rBV	640078	1057562	37.28%	5.035%
33	13.886	1847	1853	1868	rBV	725180	1074339	37.87%	5.115%
34	14.198	1896	1906	1914	rBV	619250	801751	28.26%	3.817%
35	14.486	1949	1955	1969	rBV2	39750	126420	4.46%	0.602%
36	14.681	1986	1988	1993	rVB5	3509	4352	0.15%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022976.D
 Acq On : 09 Nov 2024 21:18
 Operator : RC/JU
 Sample : P4746-21
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	14.981	2035	2039	2042	rBV3	3805	5665	0.20%	0.027%
38	15.022	2042	2046	2050	rVV	9832	13653	0.48%	0.065%
39	15.051	2050	2051	2057	rVB4	3046	3121	0.11%	0.015%
40	15.222	2074	2080	2093	rBV	1086378	1513697	53.36%	7.207%
41	15.369	2098	2105	2119	rBV	312282	536763	18.92%	2.556%
42	16.604	2311	2315	2319	rVB4	4526	6235	0.22%	0.030%
43	16.686	2325	2329	2334	rVB8	2013	3046	0.11%	0.015%
44	17.016	2379	2385	2393	rBV	921116	1114374	39.29%	5.306%
45	17.110	2395	2401	2414	rVV	1166596	1783534	62.88%	8.491%
46	17.316	2433	2436	2440	rVB5	2847	3814	0.13%	0.018%
47	17.910	2531	2537	2541	rBV6	7898	12462	0.44%	0.059%
48	17.963	2541	2546	2552	rVB4	20296	31626	1.11%	0.151%
49	18.022	2552	2556	2560	rBV3	4177	6288	0.22%	0.030%
50	18.574	2647	2650	2656	rVB8	3282	3823	0.13%	0.018%
51	18.763	2677	2682	2683	rBV5	2830	4242	0.15%	0.020%
52	19.051	2727	2731	2735	rBV3	16498	21585	0.76%	0.103%
53	19.092	2736	2738	2740	rVV2	3513	3694	0.13%	0.018%
54	19.127	2740	2744	2746	rVV	18683	23414	0.83%	0.111%
55	19.163	2746	2750	2761	rVB2	64615	88761	3.13%	0.423%
56	19.286	2768	2771	2778	rBV9	10749	14721	0.52%	0.070%
57	19.504	2802	2808	2819	rBV	1817127	2398587	84.56%	11.420%
58	21.451	3133	3139	3150	rVB2	919613	1497577	52.80%	7.130%
59	24.457	3640	3650	3665	rVB	1135985	2836571	100.00%	13.505%
60	24.686	3679	3689	3699	rBV	524325	1562020	55.07%	7.437%




Sum of corrected areas: 21004103

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022976.D
Acq On : 09 Nov 2024 21:18
Operator : RC/JU
Sample : P4746-21
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP94

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

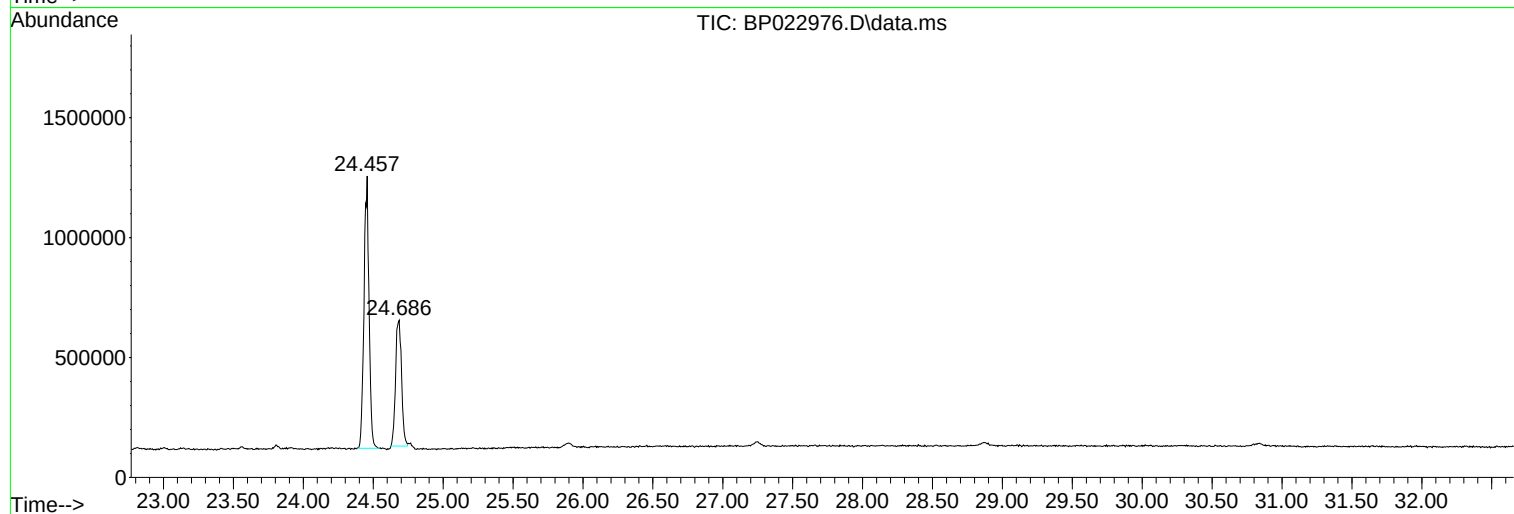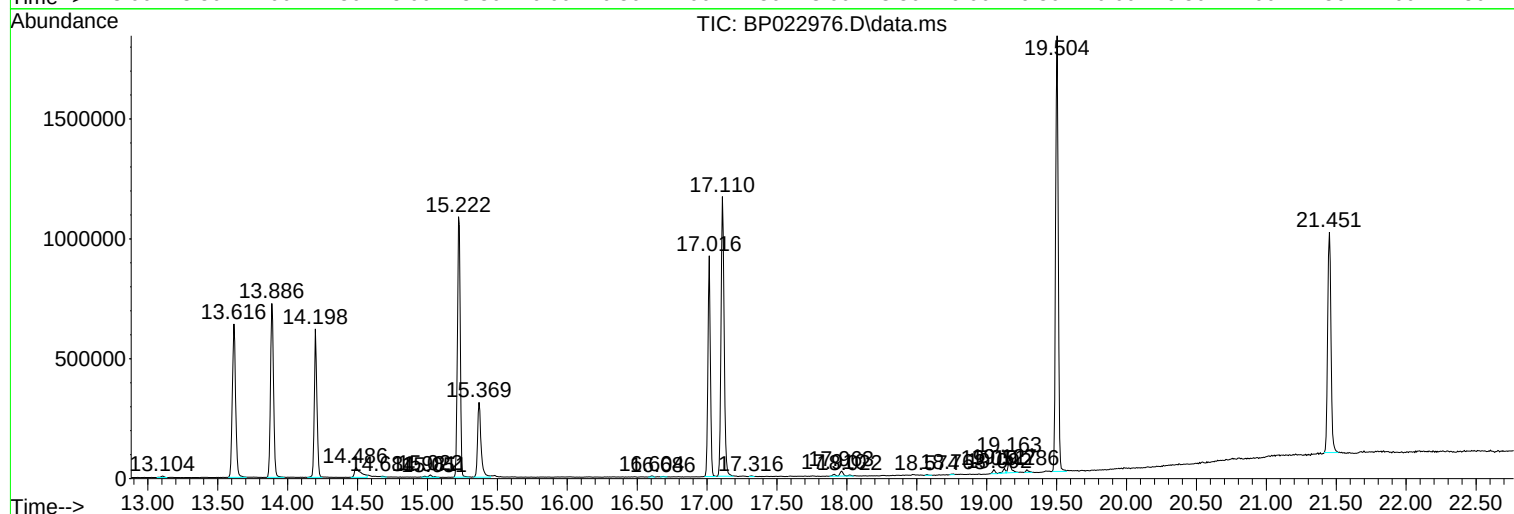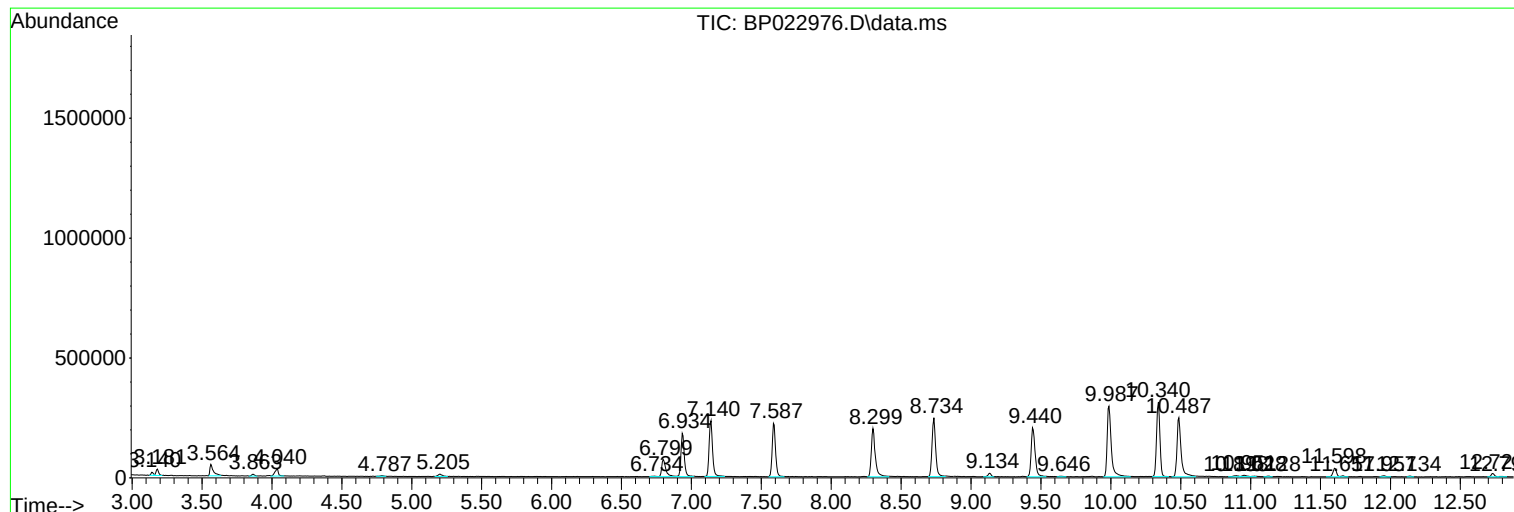

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022976.D
Acq On : 09 Nov 2024 21:18
Operator : RC/JU
Sample : P4746-21
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP94

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022976.D
Acq On : 09 Nov 2024 21:18
Operator : RC/JU
Sample : P4746-21
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP94

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc