

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022985.D
 Acq On : 10 Nov 2024 04:07
 Operator : RC/JU
 Sample : P4746-16
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP022985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	16	21	23	rBV5	5241	7958	0.27%	0.037%
2	3.140	23	26	33	rVB	14667	19668	0.67%	0.092%
3	3.564	95	98	113	rBV	29040	57186	1.95%	0.266%
4	3.864	145	149	151	rBV3	2935	3444	0.12%	0.016%
5	4.364	231	234	242	rVB2	5416	8476	0.29%	0.039%
6	4.611	272	276	280	rBV7	2019	3560	0.12%	0.017%
7	4.975	332	338	340	rBV7	1477	3081	0.11%	0.014%
8	6.793	640	647	662	rVV	130162	246037	8.40%	1.146%
9	6.928	664	670	682	rVB	214388	330828	11.30%	1.540%
10	7.134	694	705	715	rBV	260864	455730	15.56%	2.122%
11	7.587	774	782	793	rBV	248603	371294	12.68%	1.729%
12	8.293	896	902	916	rBV	316408	535621	18.29%	2.494%
13	8.728	968	976	988	rBV	294435	489301	16.71%	2.278%
14	8.869	993	1000	1004	rBV10	1747	3053	0.10%	0.014%
15	9.110	1036	1041	1048	rVB6	2249	4232	0.14%	0.020%
16	9.440	1090	1097	1115	rBV	255211	447207	15.27%	2.082%
17	9.575	1115	1120	1127	rBV3	5549	11513	0.39%	0.054%
18	9.981	1182	1189	1213	rBV	315754	680239	23.23%	3.167%
19	10.146	1213	1217	1227	rVV4	7289	17055	0.58%	0.079%
20	10.334	1241	1249	1259	rBV	318699	507152	17.32%	2.361%
21	10.487	1268	1275	1294	rBV	104700	230720	7.88%	1.074%
22	10.787	1319	1326	1328	rBV6	4018	8080	0.28%	0.038%
23	11.934	1517	1521	1531	rVB5	4708	10484	0.36%	0.049%
24	13.410	1763	1772	1773	rBV4	5822	9266	0.32%	0.043%
25	13.434	1774	1776	1782	rVV7	5176	10918	0.37%	0.051%
26	13.481	1782	1784	1789	rVB6	2148	3209	0.11%	0.015%
27	13.610	1799	1806	1816	rBV	864951	1113534	38.02%	5.185%
28	13.898	1849	1855	1865	rBV	860947	1162026	39.67%	5.411%
29	14.216	1902	1909	1918	rVV	547183	777908	26.56%	3.622%
30	14.498	1948	1957	1973	rBV5	48112	186433	6.37%	0.868%
31	14.663	1981	1985	1991	rVB8	6101	9507	0.32%	0.044%
32	15.022	2039	2046	2048	rBV8	1477	3180	0.11%	0.015%
33	15.222	2068	2080	2089	rBV	961915	1609897	54.97%	7.496%
34	15.363	2097	2104	2116	rBV	367702	575281	19.64%	2.679%
35	15.445	2116	2118	2128	rVB5	5923	11755	0.40%	0.055%
36	16.475	2289	2293	2299	rVB7	2641	4072	0.14%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
 Data File : BP022985.D
 Acq On : 10 Nov 2024 04:07
 Operator : RC/JU
 Sample : P4746-16
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCP89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	17.010	2376	2384	2394	rBV	695274	1068548	36.48%	4.975%
38	17.116	2395	2402	2414	rVV	1356229	1896319	64.75%	8.829%
39	17.704	2498	2502	2506	rBV4	2860	3613	0.12%	0.017%
40	17.945	2539	2543	2552	rVB7	10442	16562	0.57%	0.077%
41	18.157	2574	2579	2586	rBV2	16899	27623	0.94%	0.129%
42	19.033	2724	2728	2733	rBV3	19173	25534	0.87%	0.119%
43	19.116	2738	2742	2747	rBV	14099	22080	0.75%	0.103%
44	19.292	2768	2772	2778	rBV8	7199	12745	0.44%	0.059%
45	19.486	2799	2805	2819	rBV	1520249	2437448	83.22%	11.349%
46	21.445	3132	3138	3148	rBV2	822802	1462488	49.93%	6.810%
47	24.451	3639	3649	3659	rVB	1061007	2928886	100.00%	13.637%
48	24.668	3677	3686	3702	rVB	627413	1646353	56.21%	7.666%




Sum of corrected areas: 21477104

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022985.D
Acq On : 10 Nov 2024 04:07
Operator : RC/JU
Sample : P4746-16
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

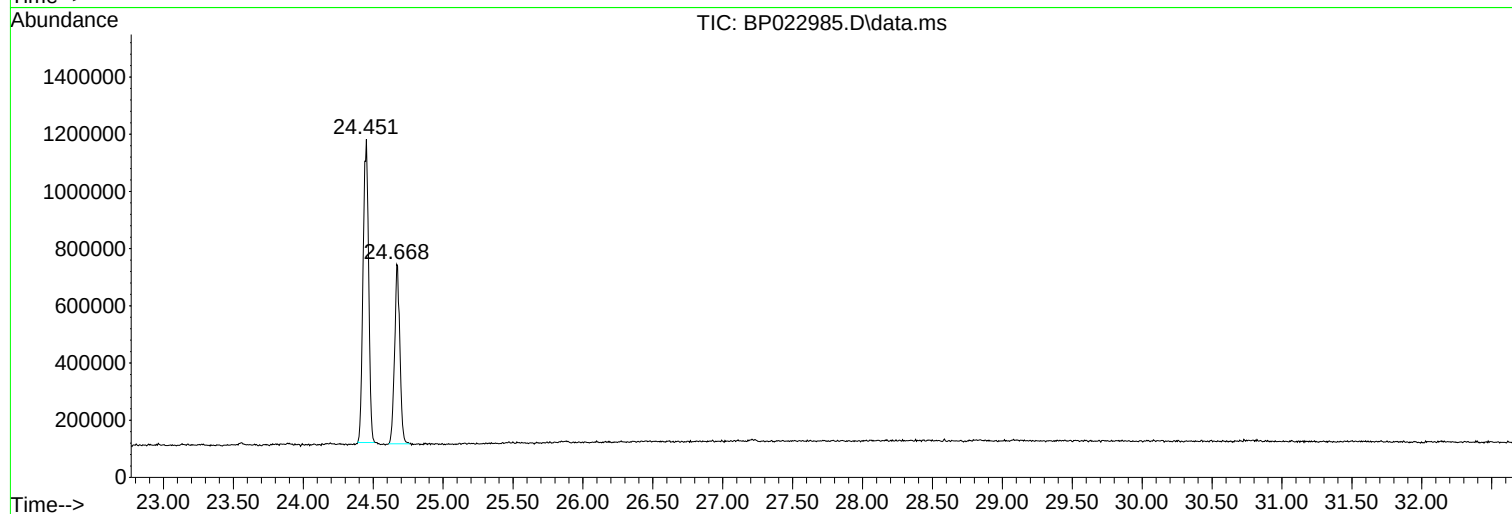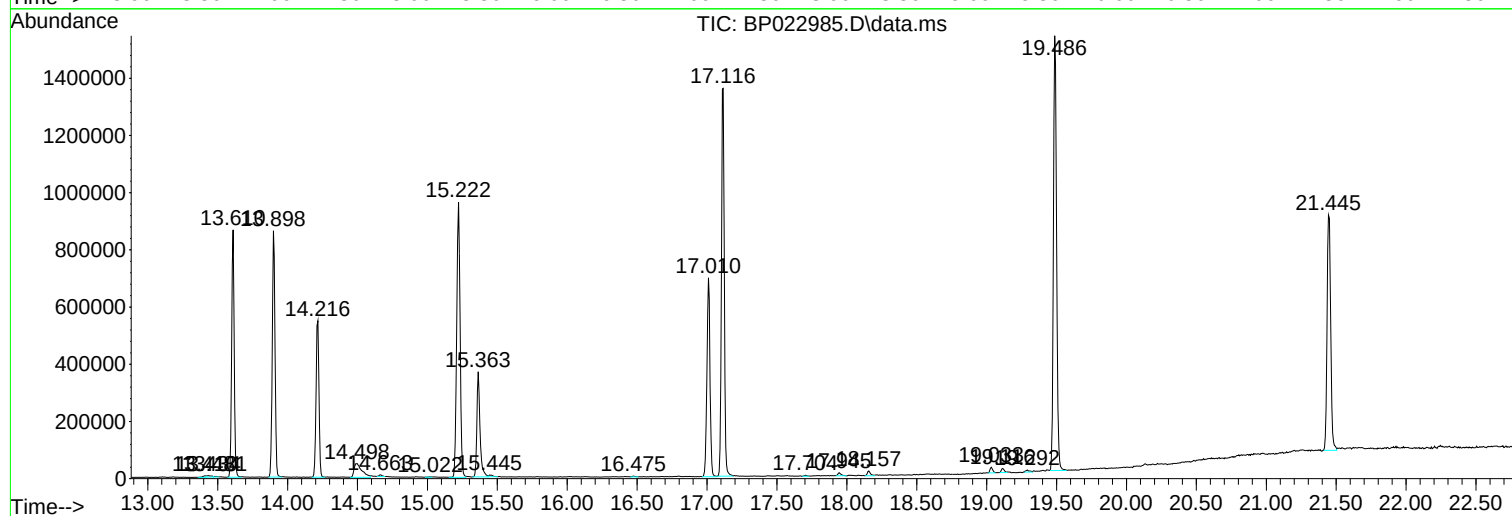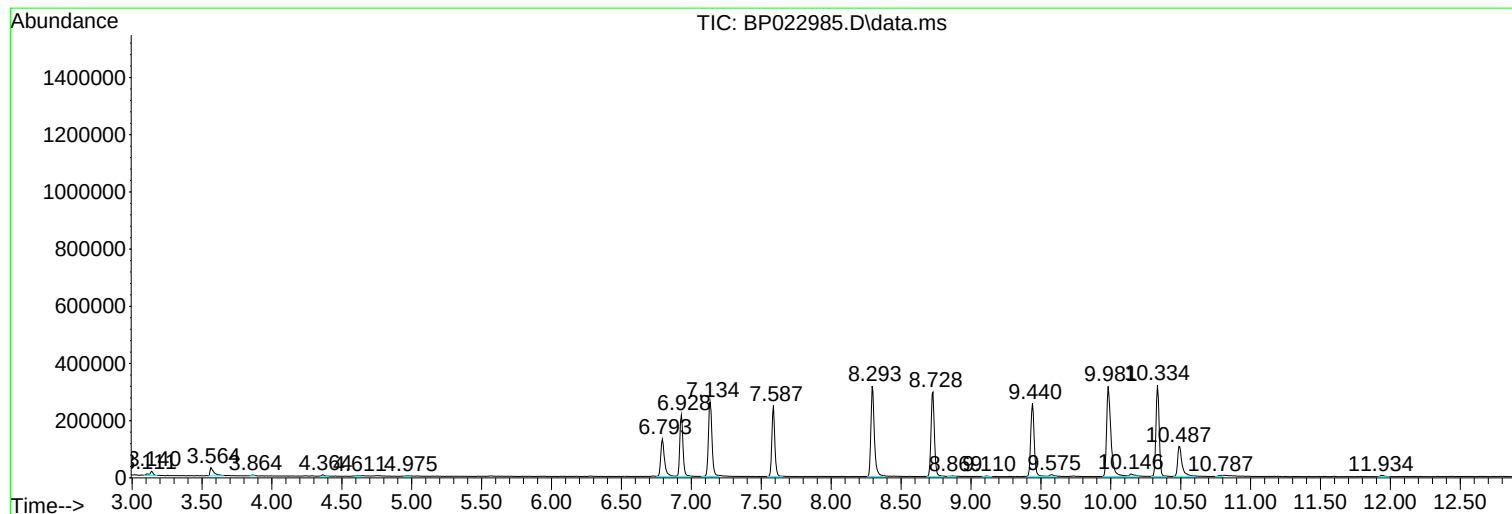

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022985.D
Acq On : 10 Nov 2024 04:07
Operator : RC/JU
Sample : P4746-16
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110924\
Data File : BP022985.D
Acq On : 10 Nov 2024 04:07
Operator : RC/JU
Sample : P4746-16
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCP89

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc