

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018030.D
 Acq On : 10 Nov 2023 17:45
 Operator : MA/JU
 Sample : SST02054
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST020619

Quant Time: Nov 10 21:23:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:21:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	64556	20.000	ng/ul	0.00
20) Naphthalene-d8	10.675	136	278257	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.527	164	186760	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	425916	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	403331	20.000	ng/ul	0.00
88) Perylene-d12	23.939	264	434157	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	13265	7.249	ng/uL	0.00
4) Pyridine-d5	3.663	84	87746	18.389	ng/ul	0.00
7) Phenol-d5	7.016	99	109860	17.627	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.198	67	68946	18.824	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	89234	18.080	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	92565	18.125	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	45469	18.137	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	52694	18.689	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.298	165	92977	18.368	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	127299	18.338	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	316448	18.364	ng/ul	0.00
49) Acenaphthylene-d8	14.227	160	341245	18.182	ng/ul	0.00
54) 4-Nitrophenol-d4	14.780	143	42564	16.530	ng/ul	0.00
60) Fluorene-d10	15.527	176	260909	18.339	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	54849	17.814	ng/ul	0.00
73) Anthracene-d10	17.410	188	411962	17.884	ng/ul	0.00
81) Pyrene-d10	19.663	212	484103	17.969	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.774	264	453419	17.961	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.269	88	14207	7.114	ng/uL	100
5) Pyridine	3.687	79	90842	18.447	ng/ul	100
6) Benzaldehyde	7.022	77	75606	22.902	ng/ul	100
8) Phenol	7.046	94	109552	17.819	ng/ul	100
10) Bis(2-Chloroethyl)ether	7.298	93	89214	18.704	ng/ul	100
12) 2-Chlorophenol	7.404	128	89601	18.082	ng/ul	100
13) 2-Methylphenol	8.304	108	83357	17.944	ng/ul	100
14) 2,2'-oxybis(1-Chloropr...	8.363	45	61358	11.265	ng/ul	100
16) Acetophenone	8.710	105	148322	18.271	ng/ul	100
17) N-Nitroso-di-n-propyla...	8.669	70	80602	18.186	ng/ul	100
18) 4-Methylphenol	8.640	108	92129	18.185	ng/ul	100
19) Hexachloroethane	8.904	117	43804	18.476	ng/ul	100
22) Nitrobenzene	9.098	77	124787	18.435	ng/ul	100
23) Isophorone	9.610	82	226780	18.360	ng/ul	100
25) 2-Nitrophenol	9.804	139	54094	18.535	ng/ul	100
26) 2,4-Dimethylphenol	9.845	107	110129	17.739	ng/ul	100
27) Bis(2-Chloroethoxy)met...	10.098	93	123840	18.386	ng/ul	100
29) 2,4-Dichlorophenol	10.322	162	89331	18.481	ng/ul	100
30) Naphthalene	10.722	128	304104	17.971	ng/ul	100
32) 4-Chloroaniline	10.875	127	124299	18.694	ng/ul	100
33) Hexachlorobutadiene	10.939	225	65326	18.409	ng/ul	100
34) Caprolactam	11.722	113	28207	17.345	ng/ul	100
35) 4-Chloro-3-methylphenol	11.986	107	106572	18.534	ng/ul	100
36) 2-Methylnaphthalene	12.339	142	212272	18.272	ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018030.D
 Acq On : 10 Nov 2023 17:45
 Operator : MA/JU
 Sample : SST02054
 Misc :
 ALS Vial : 4 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SST020619


Quant Time: Nov 10 21:23:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:21:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.557	142	217575	18.225	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.692	216	113709	18.023	ng/ul	100
40) Hexachlorocyclopentadiene	12.628	237	48316	15.865	ng/ul	100
41) 2,4,6-Trichlorophenol	12.957	196	74363	17.967	ng/ul	100
42) 2,4,5-Trichlorophenol	13.033	196	78457	18.290	ng/ul	100
43) 1,1'-Biphenyl	13.357	154	287544	18.106	ng/ul	100
44) 2-Chloronaphthalene	13.404	162	225878	17.915	ng/ul	100
45) 2-Nitroaniline	13.657	65	74641	18.345	ng/ul	100
47) Dimethylphthalate	13.998	163	312112	18.464	ng/ul	100
48) 2,6-Dinitrotoluene	14.151	165	61944	18.437	ng/ul	100
50) Acenaphthylene	14.257	152	385233	18.180	ng/ul	100
51) 3-Nitroaniline	14.498	138	58630	18.806	ng/ul	100
52) Acenaphthene	14.592	153	254967	18.146	ng/ul	100
53) 2,4-Dinitrophenol	14.710	184	28675	15.762	ng/ul	100
55) 4-Nitrophenol	14.798	109	60195	17.611	ng/ul	100
56) Dibenzofuran	14.933	168	351135	18.235	ng/ul	100
57) 2,4-Dinitrotoluene	14.945	165	93860	18.698	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.157	232	70884	18.294	ng/ul	100
59) Diethylphthalate	15.351	149	323459	18.316	ng/ul	100
61) Fluorene	15.586	166	296467	18.135	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.580	204	146243	18.255	ng/ul	100
63) 4-Nitroaniline	15.674	138	56605	19.399	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.698	198	57197	17.902	ng/ul	100
67) N-Nitrosodiphenylamine	15.810	169	248870	18.220	ng/ul	100
68) 4-Bromophenyl-phenylether	16.486	248	87625	18.254	ng/ul	100
69) Hexachlorobenzene	16.563	284	95249	17.782	ng/ul	100
70) Atrazine	16.769	200	91682	19.242	ng/ul	100
71) Pentachlorophenol	16.939	266	55271	17.092	ng/ul	100
72) Phenanthrene	17.351	178	475990	18.201	ng/ul	100
74) Anthracene	17.445	178	482741	18.089	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.310	216	114802	17.651	ng/ul	100
76) Pentachlorobenzene	14.822	250	112114	17.608	ng/ul	100
77) Carbazole	17.739	167	434626	18.754	ng/ul	100
78) Di-n-butylphthalate	18.245	149	549297	18.681	ng/ul	100
80) Fluoranthene	19.333	202	564927	17.955	ng/ul	100
82) Pyrene	19.692	202	594663	18.037	ng/ul	100
83) Butylbenzylphthalate	20.557	149	256931	18.531	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.362	252	188928	19.606	ng/ul	100
85) Benzo(a)anthracene	21.415	228	589279	18.094	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.298	149	357689	18.711	ng/ul	100
87) Chrysene	21.474	228	545079	17.890	ng/ul	100
89) Di-n-octyl phthalate	22.256	149	603889	18.599	ng/ul	100
90) Benzo(b)fluoranthene	23.162	252	560867	18.152	ng/ul	100
91) Benzo(k)fluoranthene	23.209	252	557187	17.924	ng/ul	100
93) Benzo(a)pyrene	23.827	252	526297	18.037	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.597	276	628671	17.964	ng/ul	100
95) Dibenzo(a,h)anthracene	26.621	278	516804	17.935	ng/ul	100
96) Benzo(g,h,i)perylene	27.433	276	500615	17.885	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 10 21:23:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:21:36 2023
Response via : Initial Calibration




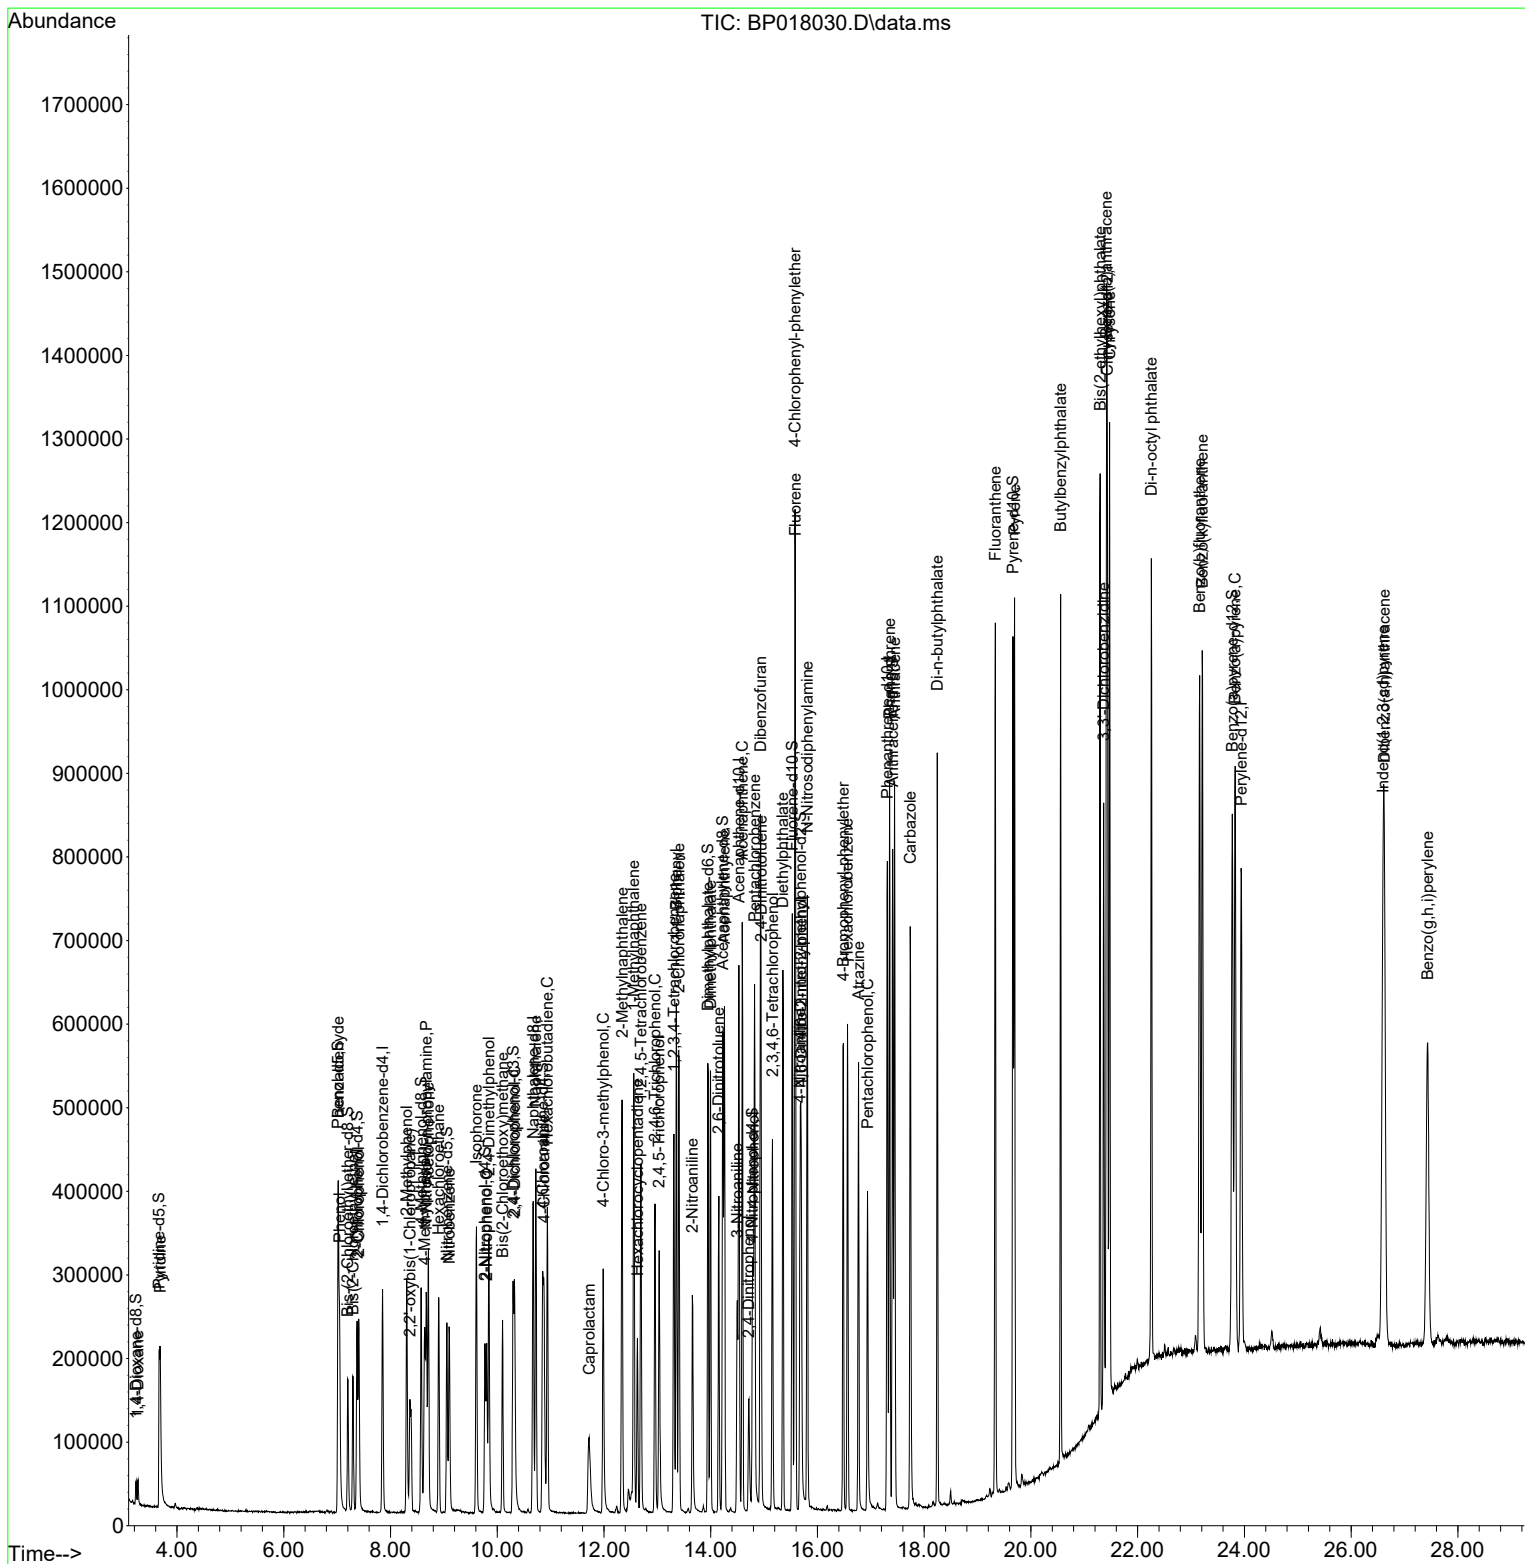


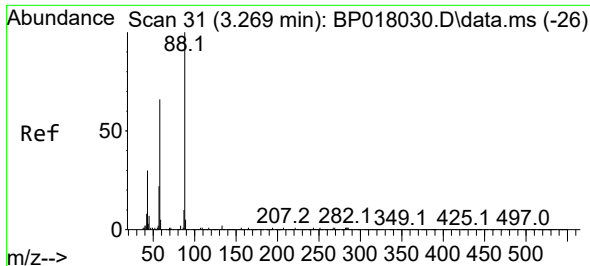

#2
1,4-Dioxane
Concen: 7.114 ng/uL
RT: 3.269 min Scan# 31
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion: 88	Resp: 14207
Ion Ratio	Lower Upper
88	100
43	31.8 25.4 38.2
58	66.6 53.3 79.9

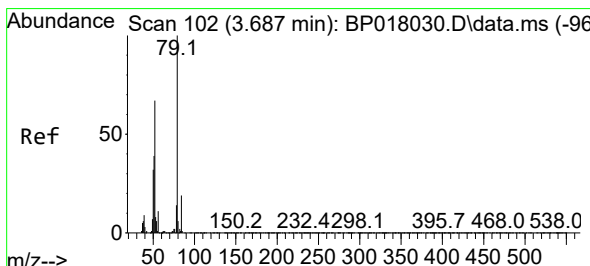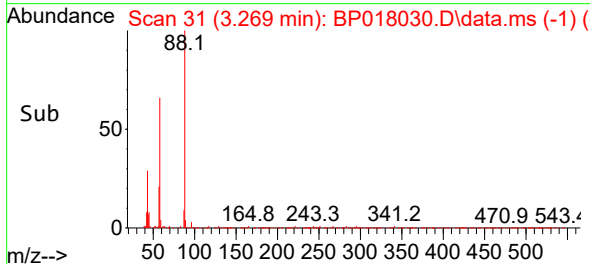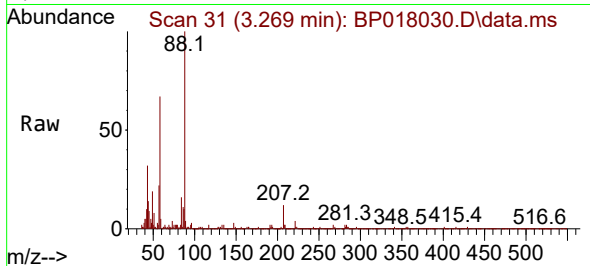

#5
Pyridine
Concen: 18.447 ng/uL
RT: 3.687 min Scan# 102
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion: 79	Resp: 90842
Ion Ratio	Lower Upper
79	100
52	67.4 53.9 80.9
51	40.2 32.2 48.2


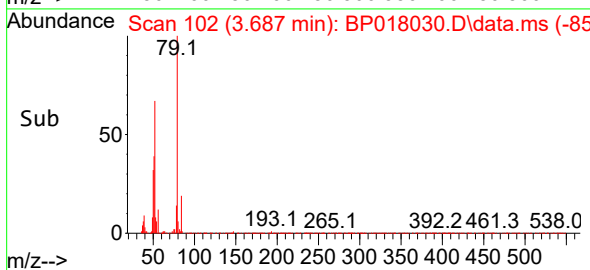

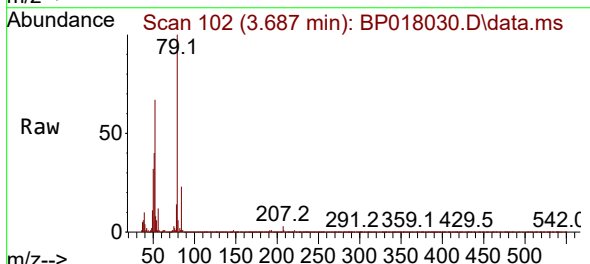




#6
Benzaldehyde
Concen: 22.902 ng/ul
RT: 7.022 min Scan# 669
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion: 77 Resp: 75606
Ion Ratio Lower Upper
77 100
105 90.9 72.7 109.1
106 84.4 67.5 101.3



#8
Phenol
Concen: 17.819 ng/ul
RT: 7.046 min Scan# 673
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion: 94 Resp: 109552
Ion Ratio Lower Upper
94 100
65 35.2 28.2 42.2
66 50.4 40.3 60.5

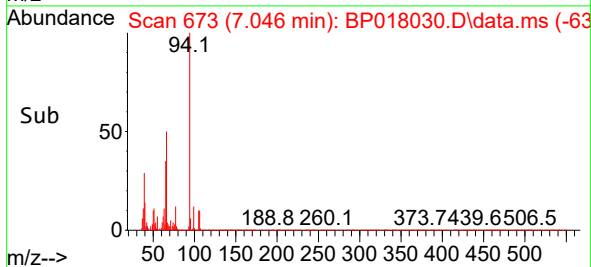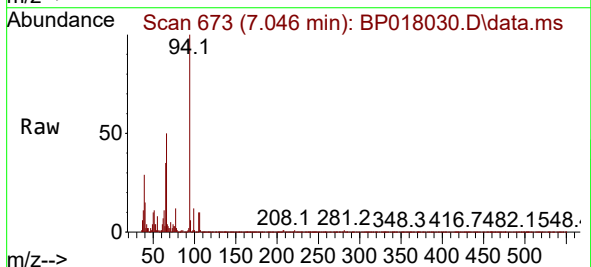







#10
 Bis(2-Chloroethyl)ether
 Concen: 18.704 ng/ul
 RT: 7.298 min Scan# 716
 Delta R.T. 0.000 min
 Lab File: BP018030.D
 Acq: 10 Nov 2023 17:45

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020619

Tgt Ion: 93 Resp: 89214




Ion	Ratio	Lower	Upper
93	100		
63	72.2	57.8	86.6
95	31.9	25.5	38.3

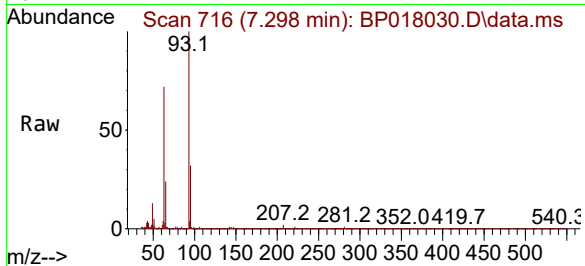


#12
 2-Chlorophenol
 Concen: 18.082 ng/ul
 RT: 7.404 min Scan# 734
 Delta R.T. 0.000 min
 Lab File: BP018030.D
 Acq: 10 Nov 2023 17:45

Tgt Ion:128 Resp: 89601

Ion	Ratio	Lower	Upper
128	100		
64	49.0	39.2	58.8
130	33.3	26.6	40.0

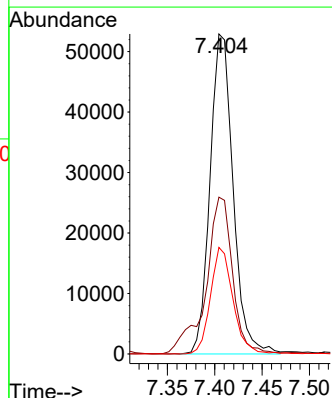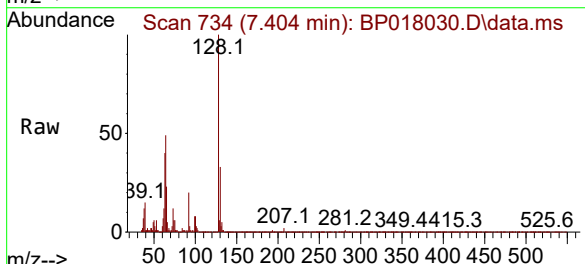



#13

2-Methylphenol

Concen: 17.944 ng/ul

RT: 8.304 min Scan# 887

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :





SSTD020619

Tgt Ion:108 Resp: 83357

Ion Ratio Lower Upper

108 100

107 94.0 75.2 112.8

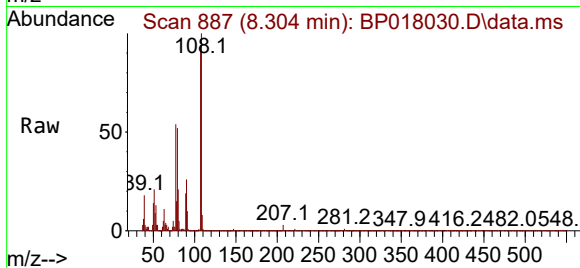

#14

2,2'-oxybis(1-Chloropropane)

Concen: 11.265 ng/ul

RT: 8.363 min Scan# 897

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion: 45 Resp: 61358


Ion Ratio Lower Upper

45 100

77 20.1 16.1 24.1

79 13.9 11.1 16.7



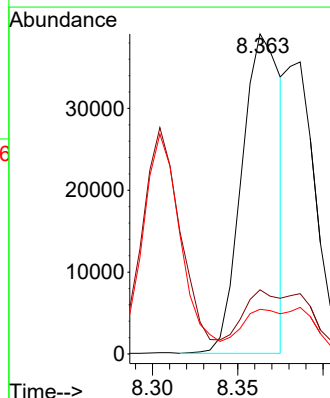
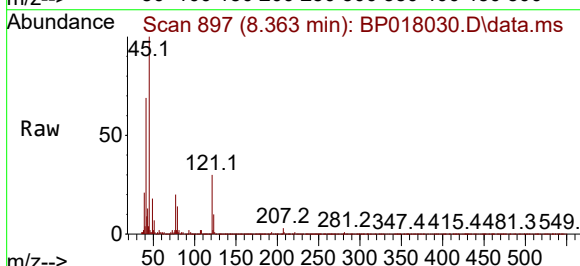




#16
Acetophenone
Concen: 18.271 ng/ul
RT: 8.710 min Scan# 956
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:105 Resp: 148322
Ion Ratio Lower Upper
105 100
77 87.6 70.1 105.1
51 29.2 23.4 35.0



#17
N-Nitroso-di-n-propylamine
Concen: 18.186 ng/ul
RT: 8.669 min Scan# 949
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion: 70 Resp: 80602
Ion Ratio Lower Upper
70 100
42 54.6 43.7 65.5
101 10.3 8.2 12.4
130 19.0 15.2 22.8









#18
4-Methylphenol
Concen: 18.185 ng/ul
RT: 8.640 min Scan# 944
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:108 Resp: 92129
Ion Ratio Lower Upper
108 100
107 110.3 88.2 132.4



#19
Hexachloroethane
Concen: 18.476 ng/ul
RT: 8.904 min Scan# 989
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:117 Resp: 43804
Ion Ratio Lower Upper
117 100
201 106.0 84.8 127.2
199 61.2 49.0 73.4



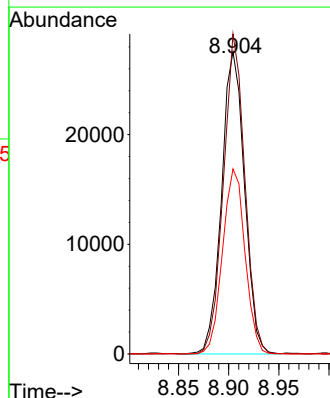





#22
Nitrobenzene
Concen: 18.435 ng/ul
RT: 9.098 min Scan# 1109
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion: 77 Resp: 124787
Ion Ratio Lower Upper
77 100
123 34.8 27.8 41.8
65 14.4 11.5 17.3



#23
Isophorone
Concen: 18.360 ng/ul
RT: 9.610 min Scan# 1109
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion: 82 Resp: 226780
Ion Ratio Lower Upper
82 100
95 8.2 6.6 9.8
138 16.4 13.1 19.7



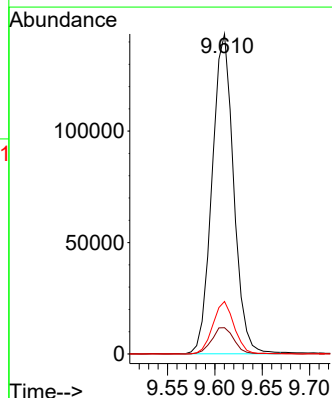





#25
2-Nitrophenol
Concen: 18.535 ng/ul
RT: 9.804 min Scan# 1142
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:	139	Resp:	54094
Ion Ratio	Lower	Upper	
139	100		
65	64.2	51.4	77.0
109	41.4	33.1	49.7



#26
2,4-Dimethylphenol
Concen: 17.739 ng/ul
RT: 9.845 min Scan# 1149
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:	107	Resp:	110129
Ion Ratio	Lower	Upper	
107	100		
121	47.3	37.8	56.8
122	77.6	62.1	93.1



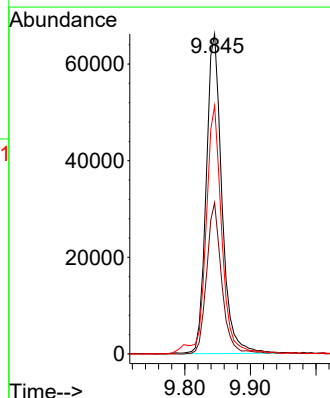





#27
 Bis(2-Chloroethoxy)methane
 Concen: 18.386 ng/ul
 RT: 10.098 min Scan# 1192
 Delta R.T. 0.000 min
 Lab File: BP018030.D
 Acq: 10 Nov 2023 17:45




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020619


Tgt Ion: 93 Resp: 123840
 Ion Ratio Lower Upper
 93 100
 95 32.7 26.2 39.2
 123 10.7 8.6 12.8

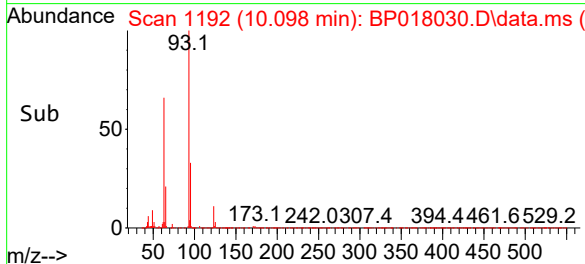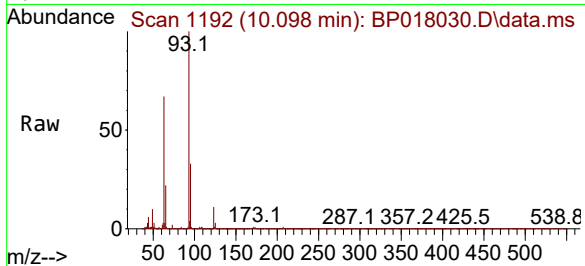

#29
 2,4-Dichlorophenol
 Concen: 18.481 ng/ul
 RT: 10.322 min Scan# 1230
 Delta R.T. 0.000 min
 Lab File: BP018030.D
 Acq: 10 Nov 2023 17:45

Tgt Ion: 162 Resp: 89331
 Ion Ratio Lower Upper
 162 100
 164 64.7 51.8 77.6
 98 35.9 28.7 43.1


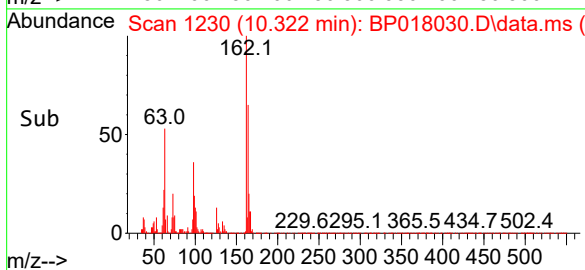

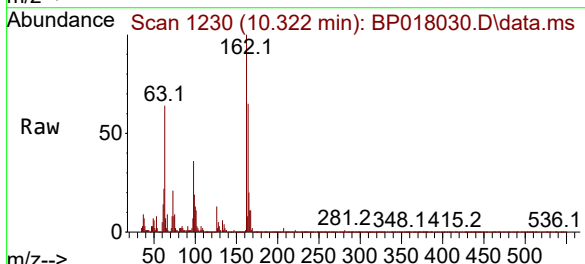




#30
Naphthalene
Concen: 17.971 ng/ul
RT: 10.722 min Scan# 1298
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:128 Resp: 304104
Ion Ratio Lower Upper
128 100
129 11.2 9.0 13.4
127 12.9 10.3 15.5

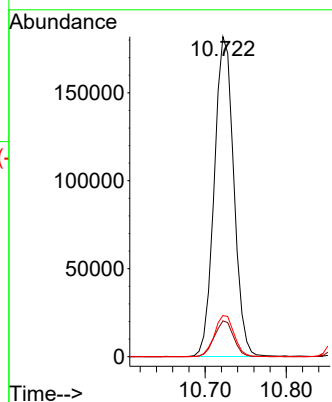

#32
4-Chloroaniline
Concen: 18.694 ng/ul
RT: 10.875 min Scan# 1324
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:127 Resp: 124299
Ion Ratio Lower Upper
127 100
129 32.6 26.1 39.1





#33

Hexachlorobutadiene

Concen: 18.409 ng/ul

RT: 10.939 min Scan# 11

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:225 Resp: 65326

Ion Ratio Lower Upper

225 100

223 65.6 52.5 78.7

227 64.9 51.9 77.9

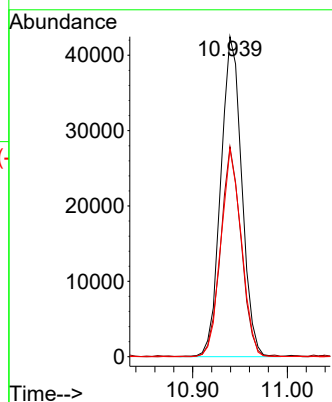

#34

Caprolactam

Concen: 17.345 ng/ul

RT: 11.722 min Scan# 1468

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:113 Resp: 28207


Ion Ratio Lower Upper

113 100

55 147.9 118.3 177.5

56 119.5 95.6 143.4









#35
4-Chloro-3-methylphenol
Concen: 18.534 ng/ul
RT: 11.986 min Scan# 1513
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:107 Resp: 106572
Ion Ratio Lower Upper
107 100
144 23.9 19.1 28.7
142 68.5 54.8 82.2

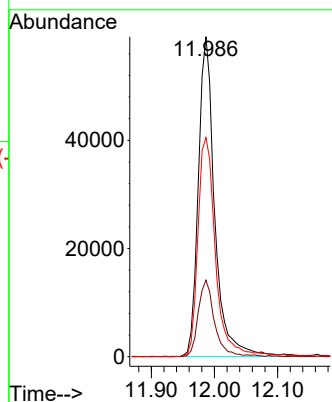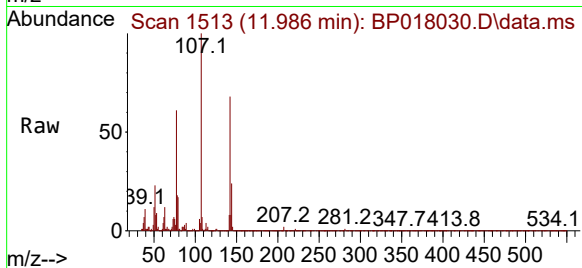

#36
2-Methylnaphthalene
Concen: 18.272 ng/ul
RT: 12.339 min Scan# 1573
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:142 Resp: 212272
Ion Ratio Lower Upper
142 100
141 89.6 71.7 107.5

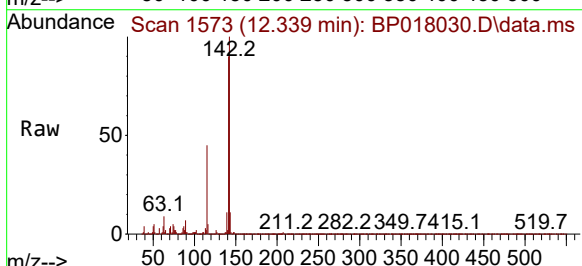



#37

1-Methylnaphthalene

Concen: 18.225 ng/ul

RT: 12.557 min Scan# 1610

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:142 Resp: 217575

Ion Ratio Lower Upper

142 100

141 91.0 72.8 109.2

116 5.0 4.0 6.0

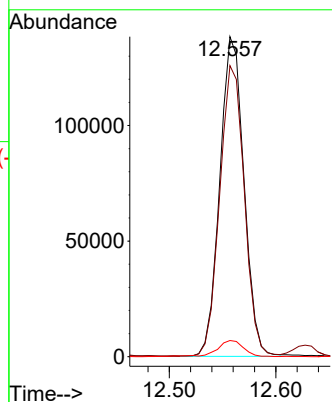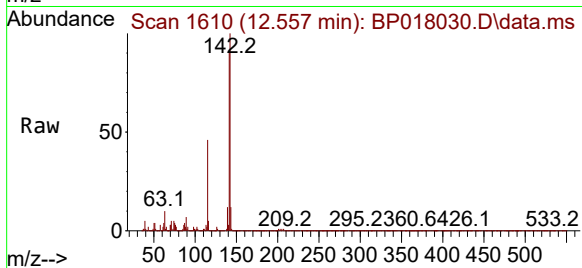

#39

1,2,4,5-Tetrachlorobenzene

Concen: 18.023 ng/ul

RT: 12.692 min Scan# 1633

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Tgt Ion:216 Resp: 113709




Ion Ratio Lower Upper


216 100

214 81.0 64.8 97.2

179 22.9 18.3 27.5

108 19.6 15.7 23.5




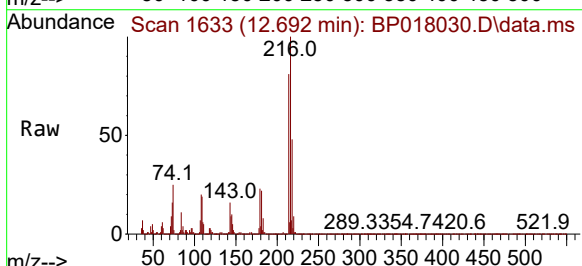




#40
Hexachlorocyclopentadiene
Concen: 15.865 ng/ul
RT: 12.628 min Scan# 1622
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:237 Resp: 48316
Ion Ratio Lower Upper
237 100
235 62.4 49.9 74.9
272 11.1 8.9 13.3



#41
2,4,6-Trichlorophenol
Concen: 17.967 ng/ul
RT: 12.957 min Scan# 1678
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:196 Resp: 74363
Ion Ratio Lower Upper
196 100
198 98.6 78.9 118.3
200 32.3 25.8 38.8





#42

2,4,5-Trichlorophenol

Concen: 18.290 ng/ul

RT: 13.033 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:196 Resp: 78457

Ion Ratio Lower Upper

196 100

198 98.6 78.9 118.3

200 33.3 26.6 40.0

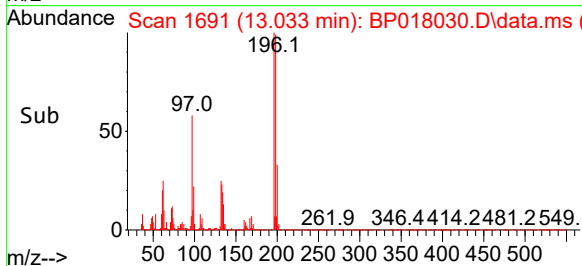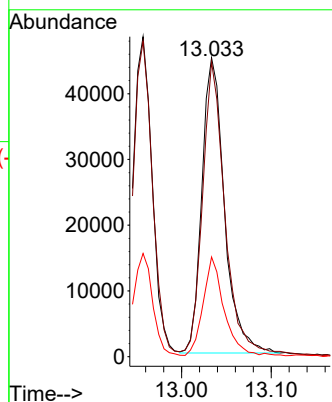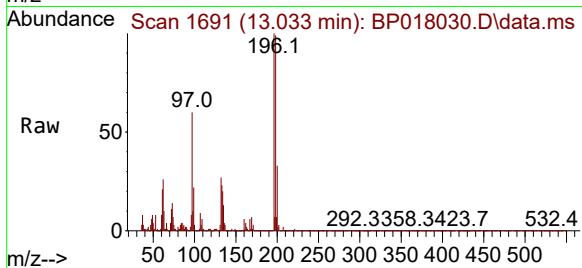

#43

1,1'-Biphenyl

Concen: 18.106 ng/ul

RT: 13.357 min Scan# 1746

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:154 Resp: 287544


Ion Ratio Lower Upper

154 100

153 40.5 32.4 48.6

76 12.3 9.8 14.8

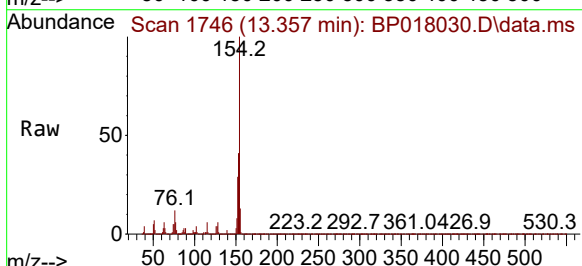




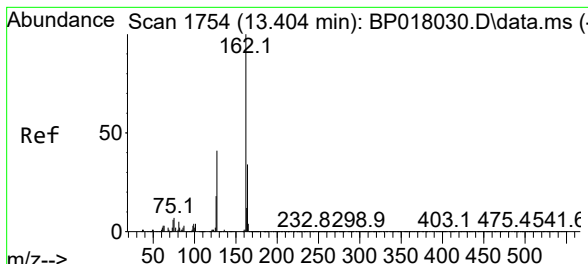


#44
 2-Chloronaphthalene
 Concen: 17.915 ng/ul
 RT: 13.404 min Scan# 1754
 Delta R.T. 0.000 min
 Lab File: BP018030.D
 Acq: 10 Nov 2023 17:45

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020619

Tgt Ion: 162 Resp: 225878




Ion	Ratio	Lower	Upper
162	100		
164	33.6	26.9	40.3
127	44.3	35.4	53.2

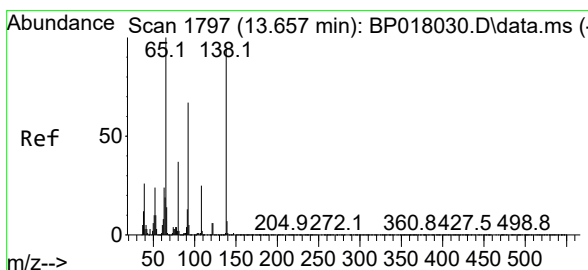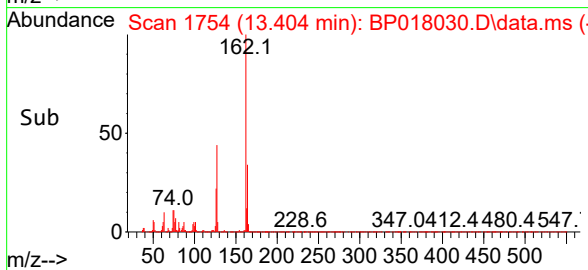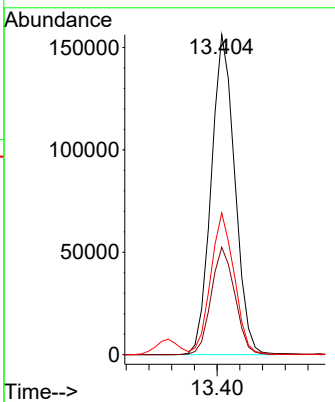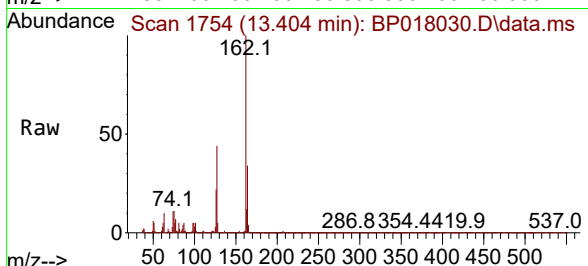


#45
 2-Nitroaniline
 Concen: 18.345 ng/ul
 RT: 13.657 min Scan# 1797
 Delta R.T. 0.000 min
 Lab File: BP018030.D
 Acq: 10 Nov 2023 17:45

Tgt Ion: 65 Resp: 74641

Ion	Ratio	Lower	Upper
65	100		
92	67.2	53.8	80.6
138	93.9	75.1	112.7


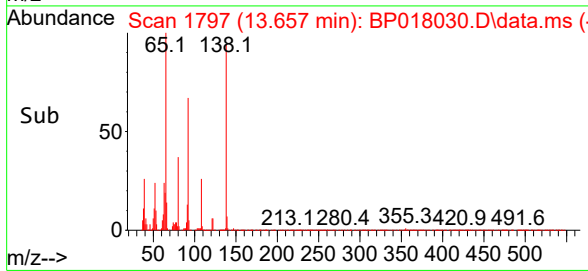
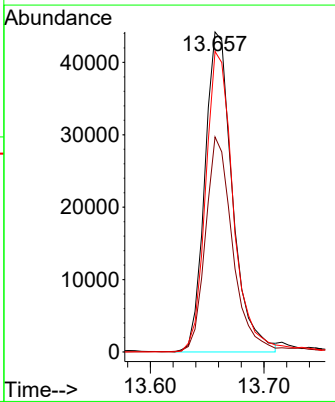
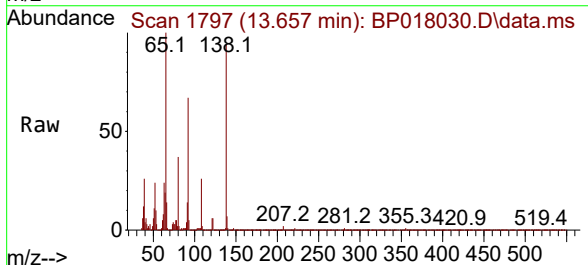




#47
Dimethylphthalate
Concen: 18.464 ng/ul
RT: 13.998 min Scan# 1855
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:163 Resp: 312112
Ion Ratio Lower Upper
163 100
194 4.4 3.5 5.3
164 10.0 8.0 12.0

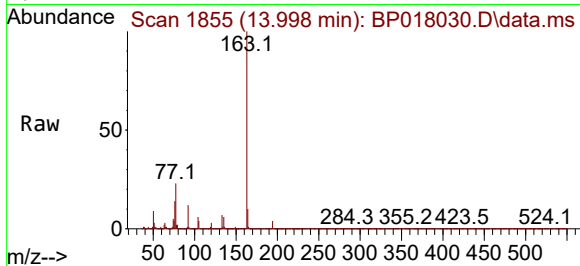

#48
2,6-Dinitrotoluene
Concen: 18.437 ng/ul
RT: 14.151 min Scan# 1881
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:165 Resp: 61944
Ion Ratio Lower Upper
165 100
89 74.2 59.4 89.0
121 22.8 18.2 27.4




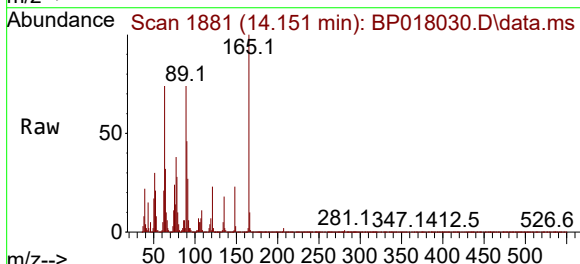




#50
Acenaphthylene
Concen: 18.180 ng/ul
RT: 14.257 min Scan# 1899
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:152 Resp: 385233
Ion Ratio Lower Upper
152 100
151 20.2 16.2 24.2
153 13.0 10.4 15.6



#51
3-Nitroaniline
Concen: 18.806 ng/ul
RT: 14.498 min Scan# 1940
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:138 Resp: 58630
Ion Ratio Lower Upper
138 100
108 10.4 8.3 12.5
92 123.7 99.0 148.4





#52

Acenaphthene

Concen: 18.146 ng/ul

RT: 14.592 min Scan# 1956

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:153 Resp: 254967

Ion Ratio Lower Upper

153 100

152 48.8 39.0 58.6

154 88.7 71.0 106.4



#53

2,4-Dinitrophenol

Concen: 15.762 ng/ul

RT: 14.710 min Scan# 1976

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:184 Resp: 28675


Ion Ratio Lower Upper

184 100

63 84.6 67.7 101.5

154 75.3 60.2 90.4









#55
4-Nitrophenol
Concen: 17.611 ng/ul
RT: 14.798 min Scan# 1991
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:	109	Resp:	60195
Ion Ratio	Lower	Upper	
109	100		
139	93.6	74.9	112.3
65	117.2	93.8	140.6

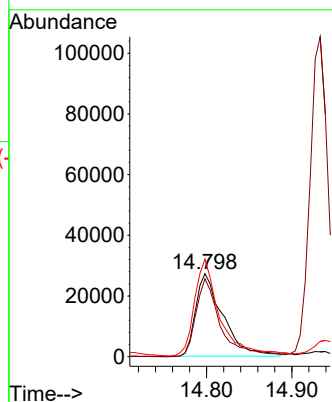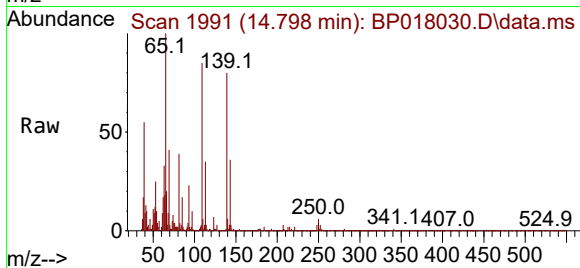

#56
Dibenzofuran
Concen: 18.235 ng/ul
RT: 14.933 min Scan# 2014
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:	168	Resp:	351135
Ion Ratio	Lower	Upper	
168	100		
139	42.5	34.0	51.0




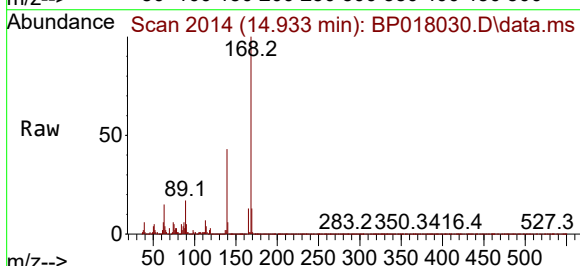




#57
2,4-Dinitrotoluene
Concen: 18.698 ng/ul
RT: 14.945 min Scan# 2016
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:165 Resp: 93860
Ion Ratio Lower Upper
165 100
63 60.7 48.6 72.8
182 2.6 2.1 3.1

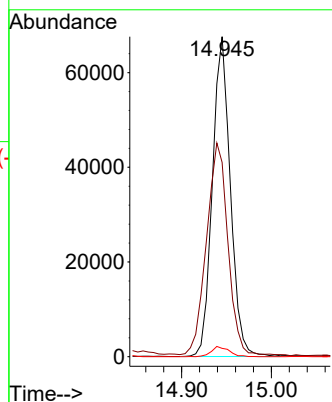

#58
2,3,4,6-Tetrachlorophenol
Concen: 18.294 ng/ul
RT: 15.157 min Scan# 2052
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:232 Resp: 70884
Ion Ratio Lower Upper
232 100
131 55.1 44.1 66.1
130 3.1 2.5 3.7
166 34.9 27.9 41.9


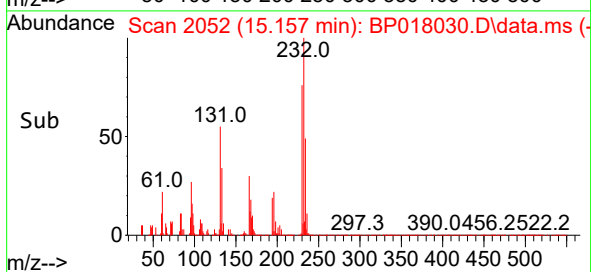






#59
Diethylphthalate
Concen: 18.316 ng/ul
RT: 15.351 min Scan# 2085
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:149 Resp: 323459
Ion Ratio Lower Upper
149 100
177 20.4 16.3 24.5
150 12.5 10.0 15.0



#61
Fluorene
Concen: 18.135 ng/ul
RT: 15.586 min Scan# 2125
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:166 Resp: 296467
Ion Ratio Lower Upper
166 100
165 98.8 79.0 118.6
167 13.3 10.6 16.0









#62
4-Chlorophenyl-phenylether
Concen: 18.255 ng/ul
RT: 15.580 min Scan# 2124
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:204 Resp: 146243
Ion Ratio Lower Upper
204 100
206 32.7 26.2 39.2
141 70.0 56.0 84.0



#63
4-Nitroaniline
Concen: 19.399 ng/ul
RT: 15.674 min Scan# 2140
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:138 Resp: 56605
Ion Ratio Lower Upper
138 100
92 58.3 46.6 70.0
108 130.9 104.7 157.1




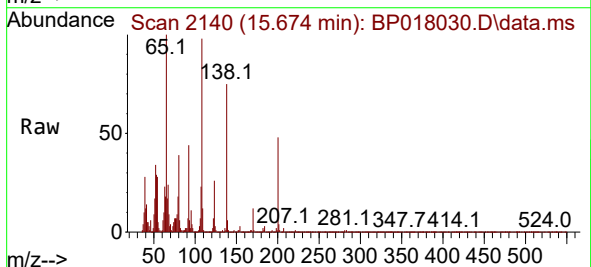




#66
 4,6-Dinitro-2-methylphenol
 Concen: 17.902 ng/ul
 RT: 15.698 min Scan# 2144
 Delta R.T. 0.000 min
 Lab File: BP018030.D
 Acq: 10 Nov 2023 17:45




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020619


Tgt Ion:198 Resp: 57197
 Ion Ratio Lower Upper
 198 100
 182 4.7 3.8 5.6
 77 34.0 27.2 40.8



#67
 N-Nitrosodiphenylamine
 Concen: 18.220 ng/ul
 RT: 15.810 min Scan# 2163
 Delta R.T. 0.000 min
 Lab File: BP018030.D
 Acq: 10 Nov 2023 17:45

Tgt Ion:169 Resp: 248870
 Ion Ratio Lower Upper
 169 100
 168 67.3 53.8 80.8
 167 37.2 29.8 44.6









#68
4-Bromophenyl-phenylether
Concen: 18.254 ng/ul
RT: 16.486 min Scan# 2278
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:248 Resp: 87625
Ion Ratio Lower Upper
248 100
250 90.9 72.7 109.1
141 88.0 70.4 105.6

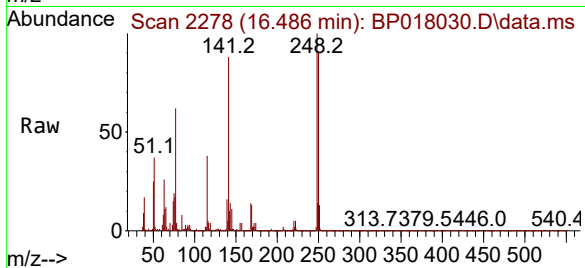

#69
Hexachlorobenzene
Concen: 17.782 ng/ul
RT: 16.563 min Scan# 2291
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:284 Resp: 95249
Ion Ratio Lower Upper
284 100
142 48.6 38.9 58.3
249 35.8 28.6 43.0

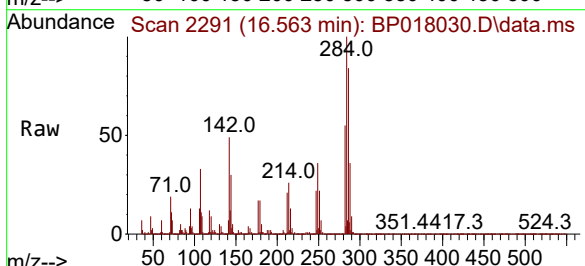



#70

Atrazine

Concen: 19.242 ng/ul

RT: 16.769 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:200 Resp: 91682

Ion Ratio Lower Upper

200 100

173 25.2 20.2 30.2

215 47.3 37.8 56.8

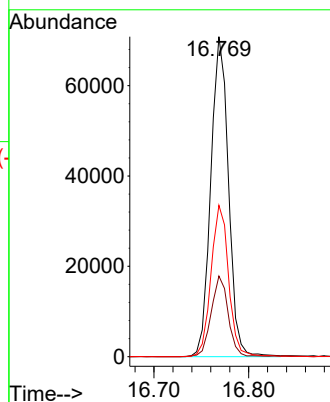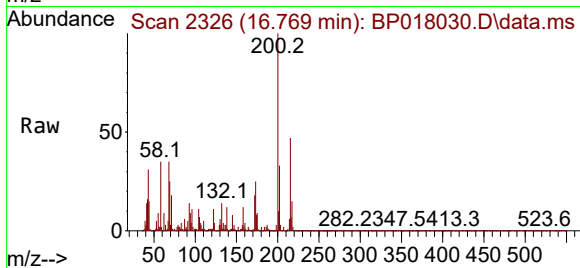

#71

Pentachlorophenol

Concen: 17.092 ng/ul

RT: 16.939 min Scan# 2355

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:266 Resp: 55271


Ion Ratio Lower Upper

266 100

264 63.4 50.7 76.1

268 65.5 52.4 78.6

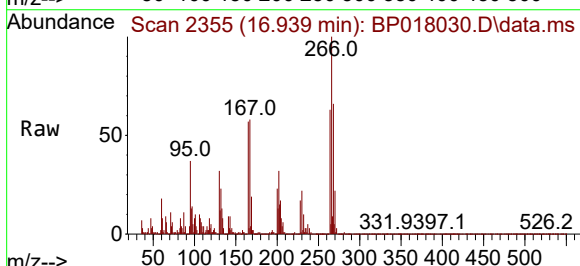



#72

Phenanthrene

Concen: 18.201 ng/ul

RT: 17.351 min Scan# 2425

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:178 Resp: 475990

Ion Ratio Lower Upper

178 100

179 15.0 12.0 18.0

176 19.4 15.5 23.3

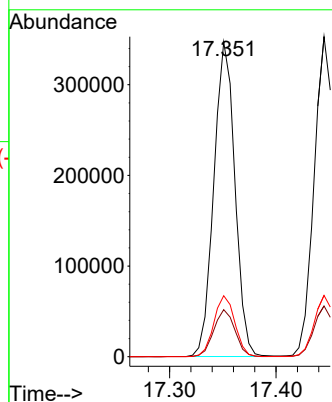

#74

Anthracene

Concen: 18.089 ng/ul

RT: 17.445 min Scan# 2441

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:178 Resp: 482741


Ion Ratio Lower Upper

178 100

179 15.8 12.6 19.0

176 19.2 15.4 23.0





#75

1,2,3,4-Tetrachlorobenzene

Concen: 17.651 ng/uL

RT: 13.310 min Scan# 1738

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:216 Resp: 114802

Ion Ratio Lower Upper

216 100

214 80.0 64.0 96.0

218 48.7 39.0 58.4

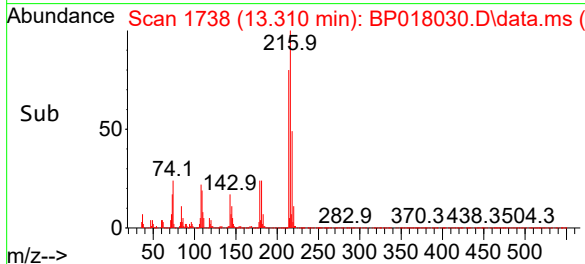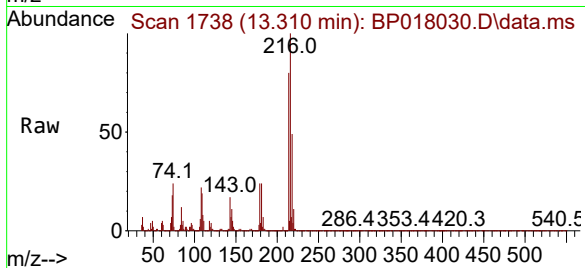

#76

Pentachlorobenzene

Concen: 17.608 ng/uL

RT: 14.822 min Scan# 1995

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:250 Resp: 112114


Ion Ratio Lower Upper

250 100

248 65.9 52.7 79.1

252 65.4 52.3 78.5

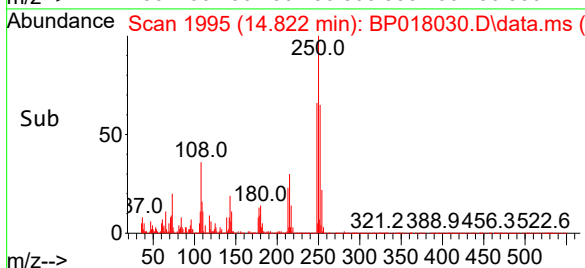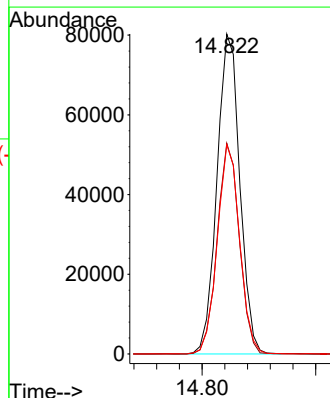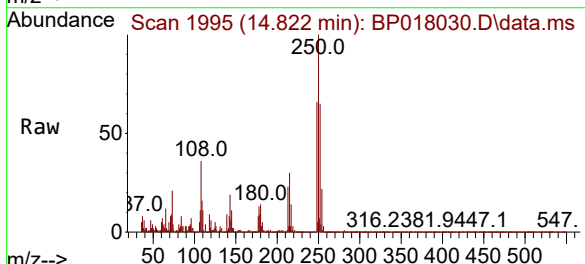



#77

Carbazole

Concen: 18.754 ng/ul

RT: 17.739 min Scan# 2491

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:167 Resp: 434626

Ion Ratio Lower Upper

167 100

166 22.0 17.6 26.4

139 14.2 11.4 17.0

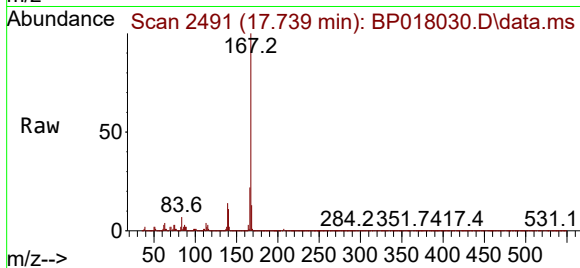

#78

Di-n-butylphthalate

Concen: 18.681 ng/ul

RT: 18.245 min Scan# 2577

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:149 Resp: 549297


Ion Ratio Lower Upper

149 100

150 8.4 6.7 10.1

104 6.4 5.1 7.7

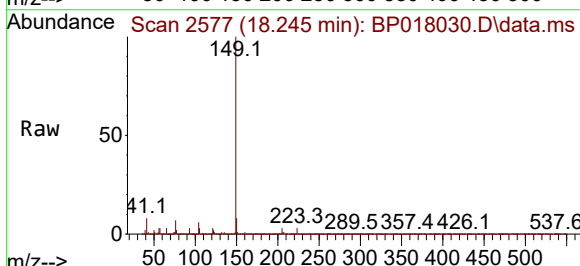



#80

Fluoranthene

Concen: 17.955 ng/ul

RT: 19.333 min Scan# 2762

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:202 Resp: 564927

Ion Ratio Lower Upper

202 100

101 9.0 7.2 10.8

100 7.2 5.8 8.6

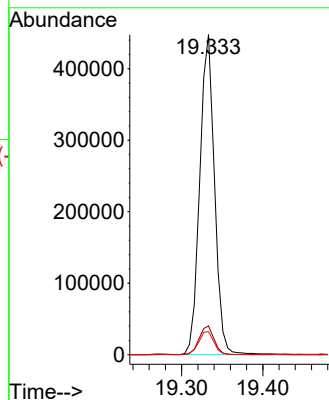

#82

Pyrene

Concen: 18.037 ng/ul

RT: 19.692 min Scan# 2823

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:202 Resp: 594663


Ion Ratio Lower Upper

202 100

101 10.4 8.3 12.5

100 9.3 7.4 11.2

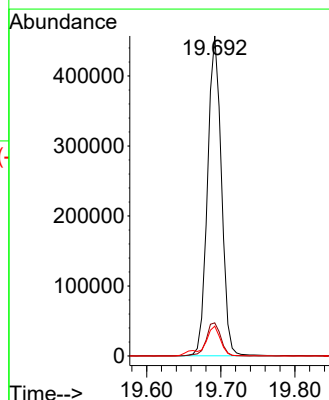



#83

Butylbenzylphthalate

Concen: 18.531 ng/ul

RT: 20.557 min Scan# 2970

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:149 Resp: 256931

Ion Ratio Lower Upper

149 100

91 74.5 59.6 89.4

206 17.9 14.3 21.5

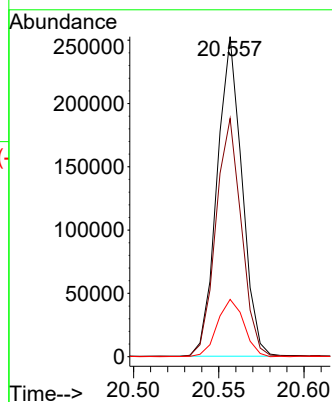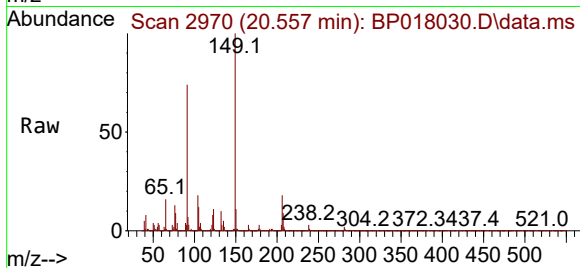

#84

3,3'-Dichlorobenzidine

Concen: 19.606 ng/ul

RT: 21.362 min Scan# 3107

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:252 Resp: 188928


Ion Ratio Lower Upper

252 100

254 61.1 48.9 73.3

126 11.7 9.4 14.0

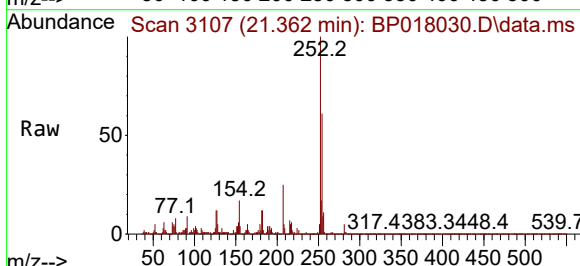



#85

Benzo(a)anthracene

Concen: 18.094 ng/ul

RT: 21.415 min Scan# 3116

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:228 Resp: 589279

Ion Ratio Lower Upper

228 100

229 19.2 15.4 23.0

226 26.7 21.4 32.0

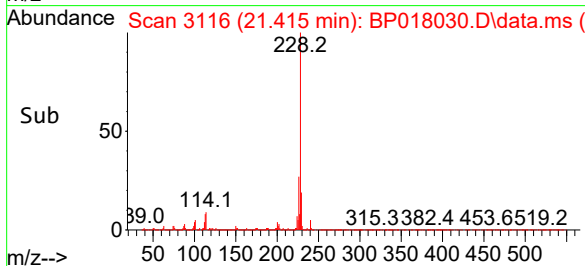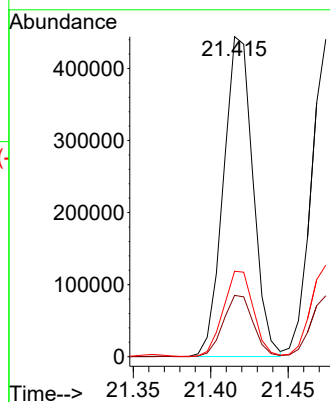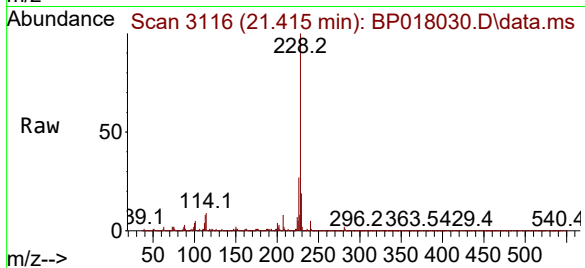

#86

Bis(2-ethylhexyl)phthalate

Concen: 18.711 ng/ul

RT: 21.298 min Scan# 3096

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:149 Resp: 357689


Ion Ratio Lower Upper

149 100

167 26.2 21.0 31.4

279 4.0 3.2 4.8

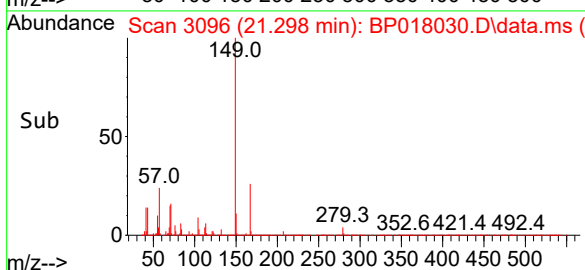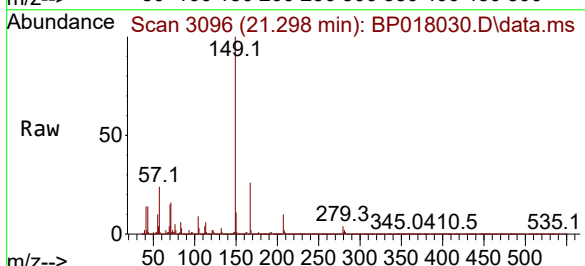



#87

Chrysene

Concen: 17.890 ng/ul

RT: 21.474 min Scan# 3126

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:228 Resp: 545079

Ion Ratio Lower Upper

228 100

226 28.9 23.1 34.7

229 19.2 15.4 23.0

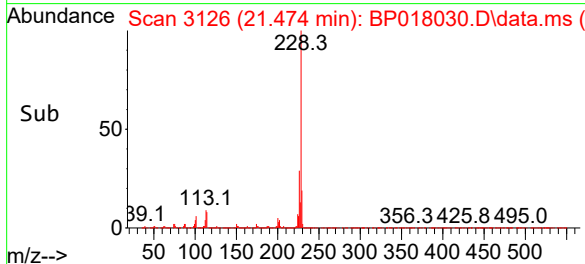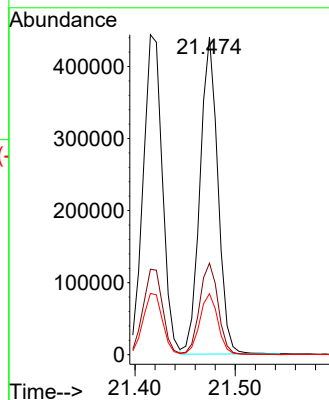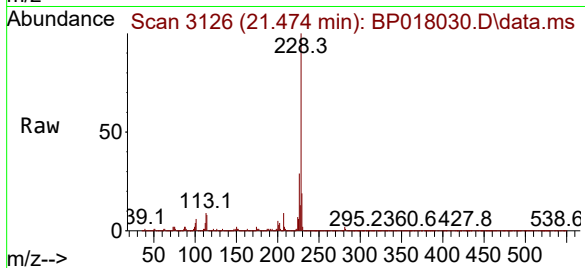

#89

Di-n-octyl phthalate

Concen: 18.599 ng/ul




RT: 22.256 min Scan# 3259


Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Tgt Ion:149 Resp: 603889


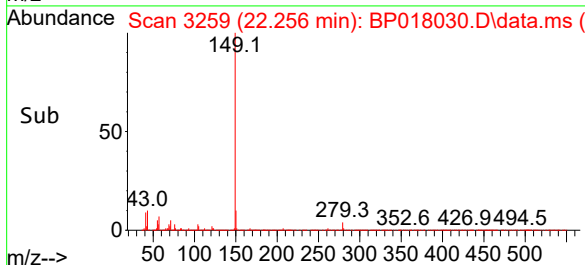
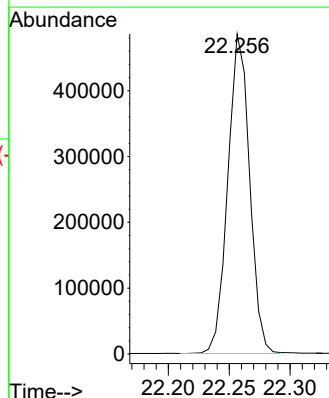
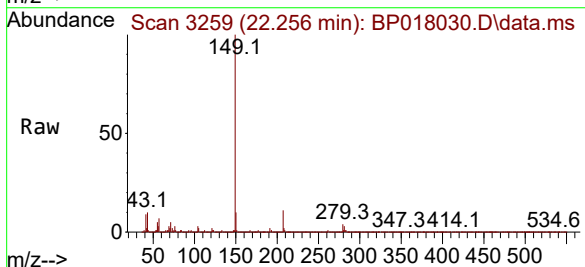




#90
Benzo(b)fluoranthene
Concen: 18.152 ng/ul
RT: 23.162 min Scan# 3413
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:252 Resp: 560867
Ion Ratio Lower Upper
252 100
253 21.2 17.0 25.4
125 8.8 7.0 10.6



#91
Benzo(k)fluoranthene
Concen: 17.924 ng/ul
RT: 23.209 min Scan# 3421
Delta R.T. 0.000 min
Lab File: BP018030.D
Acq: 10 Nov 2023 17:45

Tgt Ion:252 Resp: 557187
Ion Ratio Lower Upper
252 100
253 22.0 17.6 26.4
125 8.5 6.8 10.2





#93

Benzo(a)pyrene

Concen: 18.037 ng/ul

RT: 23.827 min Scan# 3526

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:252 Resp: 526297

Ion Ratio Lower Upper

252 100

253 21.7 17.4 26.0

125 9.1 7.3 10.9



#94

Indeno(1,2,3-cd)pyrene

Concen: 17.964 ng/ul

RT: 26.597 min Scan# 3997

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45




Tgt Ion:276 Resp: 628671


Ion Ratio Lower Upper

276 100

138 19.5 15.6 23.4

277 24.1 19.3 28.9

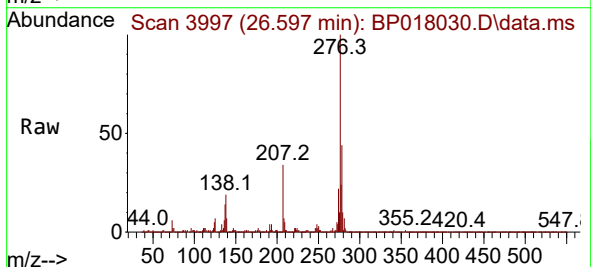



#95

Dibenzo(a,h)anthracene

Concen: 17.935 ng/ul

RT: 26.621 min Scan# 4001

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:278 Resp: 516804

Ion Ratio Lower Upper

278 100

139 13.9 11.1 16.7

279 23.7 19.0 28.4



#96

Benzo(g,h,i)perylene

Concen: 17.885 ng/ul

RT: 27.433 min Scan# 4139

Delta R.T. 0.000 min

Lab File: BP018030.D

Acq: 10 Nov 2023 17:45

Tgt Ion:276 Resp: 500615

Ion Ratio Lower Upper

276 100

138 17.2 13.8 20.6

277 25.2 20.2 30.2

