




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018039.D
 Acq On : 10 Nov 2023 23:24
 Operator : MA/JU
 Sample : PB156652BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK652

Manual IntegrationsAPPROVED

Quant Time: Nov 11 00:42:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2023
 Supervised By :mohammad ahmed 11/15/2023

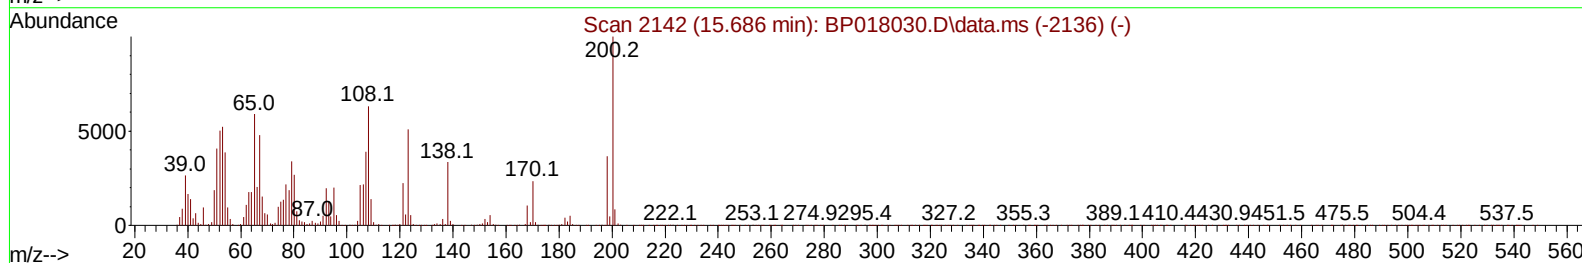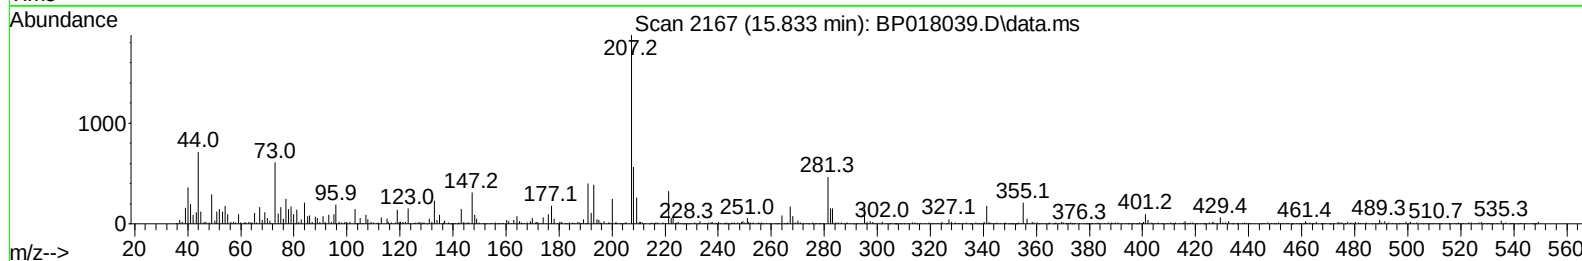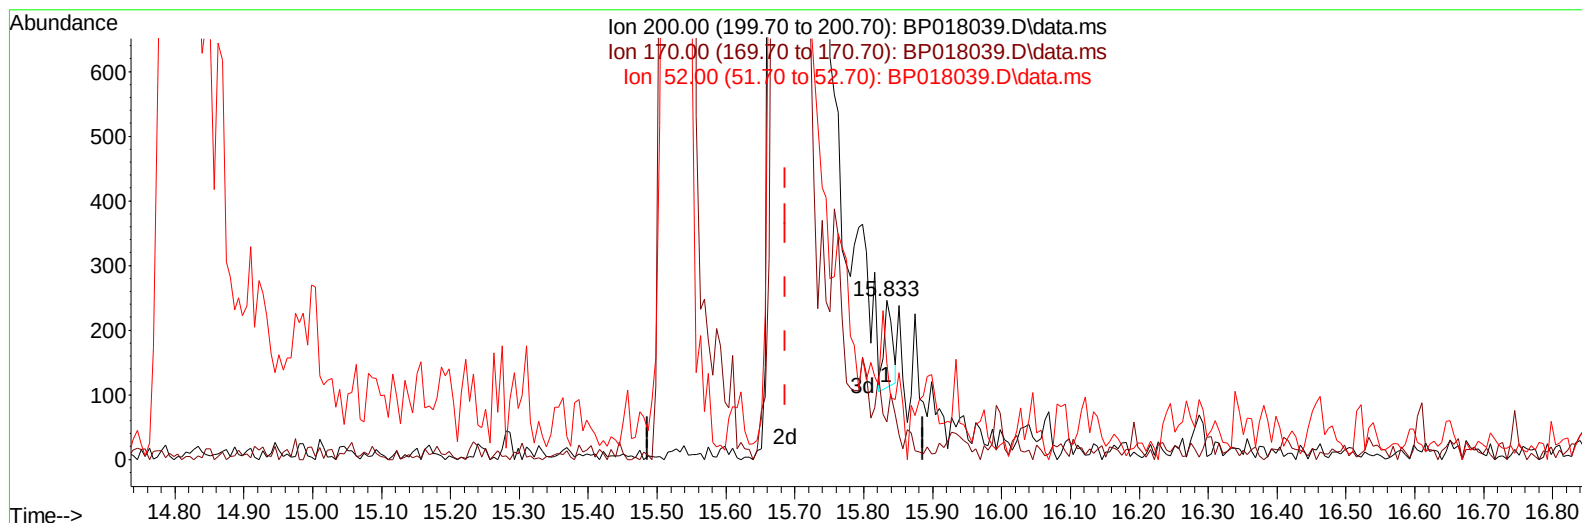

TIC: BP018039.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.833min (+ 0.147) 0.05 ng/u1

response 112

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.60	23.58
52.00	52.00	60.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018039.D
 Acq On : 10 Nov 2023 23:24
 Operator : MA/JU
 Sample : PB156652BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK652

Manual IntegrationsAPPROVED

Quant Time: Nov 11 00:42:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2023
 Supervised By :mohammad ahmed 11/15/2023

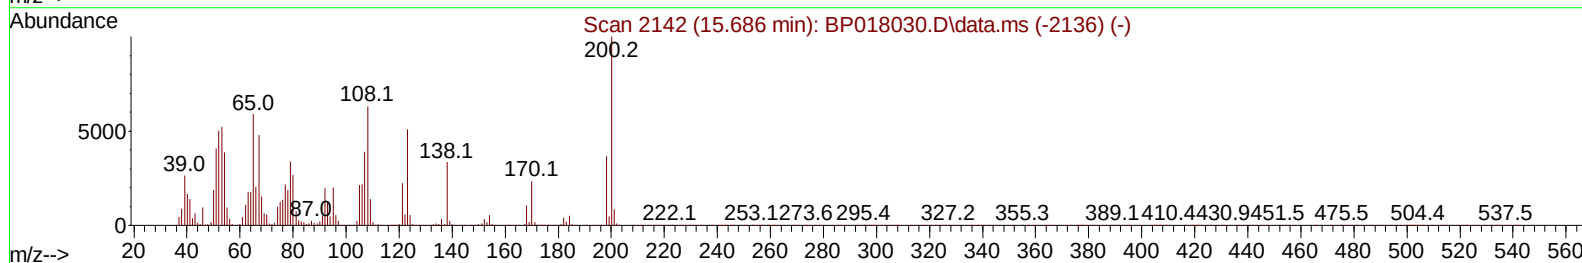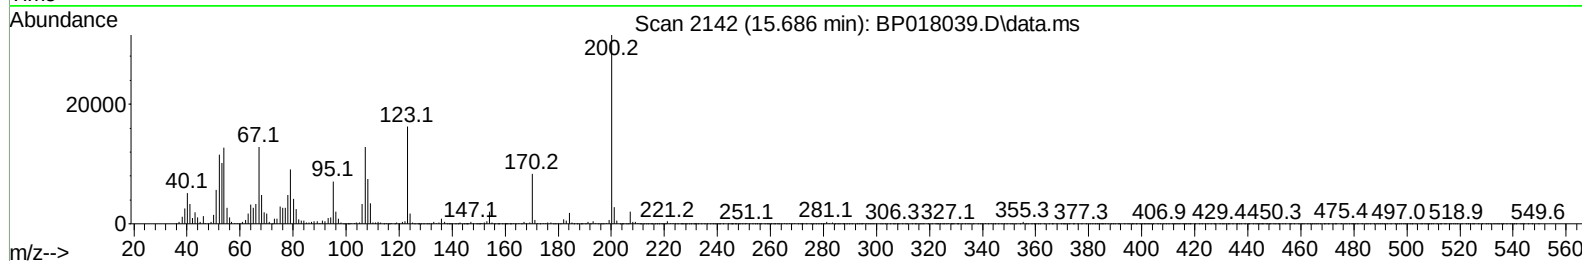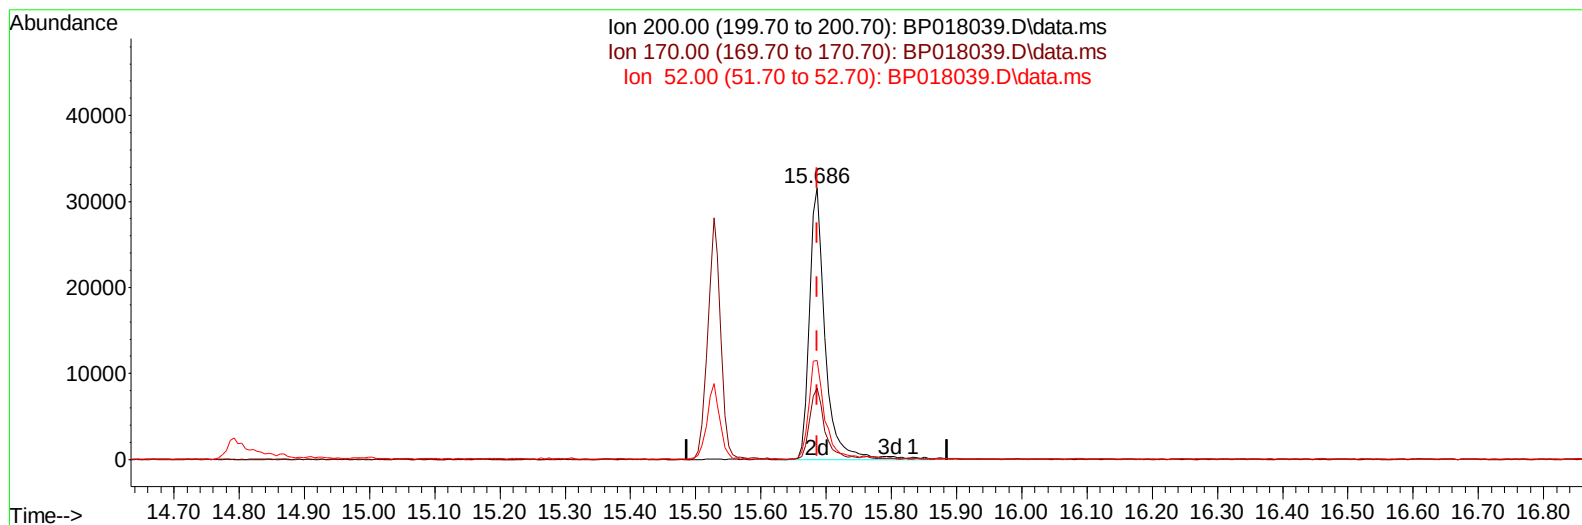

TIC: BP018039.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.686min (+ 0.000) 24.53 ng/ul m

response 53006

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.60	26.38
52.00	52.00	36.47#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018039.D
 Acq On : 10 Nov 2023 23:24
 Operator : MA/JU
 Sample : PB156652BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK652

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2023
 Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 11 00:44:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	53748	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	218349	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.528	164	134887	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	298857	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	274923	20.000	ng/ul	0.00
88) Perylene-d12	23.933	264	315128	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	9923	6.513	ng/uL	0.00
4) Pyridine-d5	3.664	84	118946	29.941	ng/ul	0.00
7) Phenol-d5	7.016	99	140372	27.052	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	91840	30.117	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	117312	28.549	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	114306	26.883	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	57208	29.081	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	65211	29.260	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.298	165	99439	25.034	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	149476	27.441	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	386240	31.034	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	397668	29.336	ng/ul	0.00
54) 4-Nitrophenol-d4	14.792	143	38993	20.967	ng/ul	0.01
60) Fluorene-d10	15.528	176	305446	29.726	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	53006m	24.534	ng/ul	0.00
73) Anthracene-d10	17.410	188	490866	30.369	ng/ul	0.00
81) Pyrene-d10	19.663	212	587898	32.014	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.768	264	575462	31.405	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018039.D
Acq On : 10 Nov 2023 23:24
Operator : MA/JU
Sample : PB156652BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK652

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2023
Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 11 00:44:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

