




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018046.D
Acq On : 11 Nov 2023 03:22
Operator : MA/JU
Sample : 05057-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49G7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 03:52:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/11/2023
Supervised By :mohammad ahmed 11/15/2023

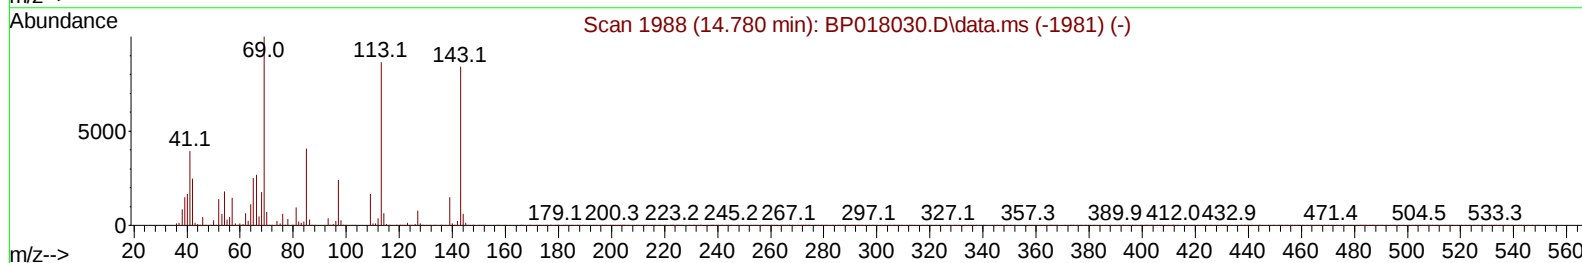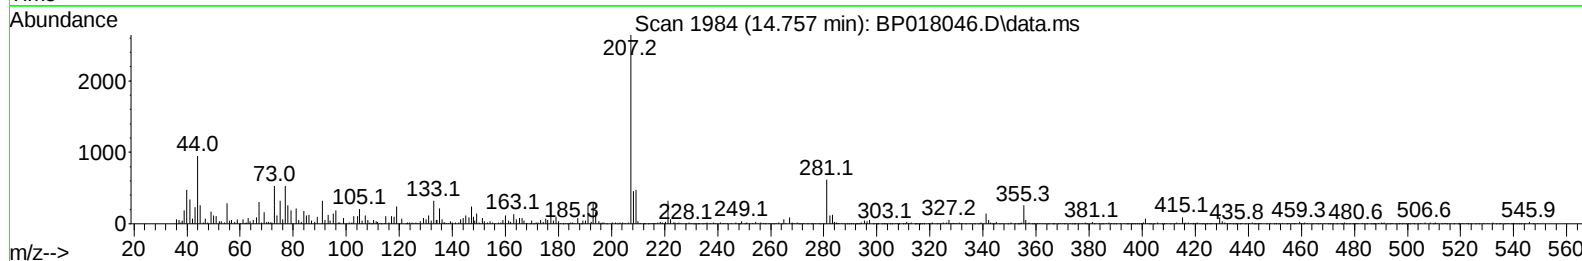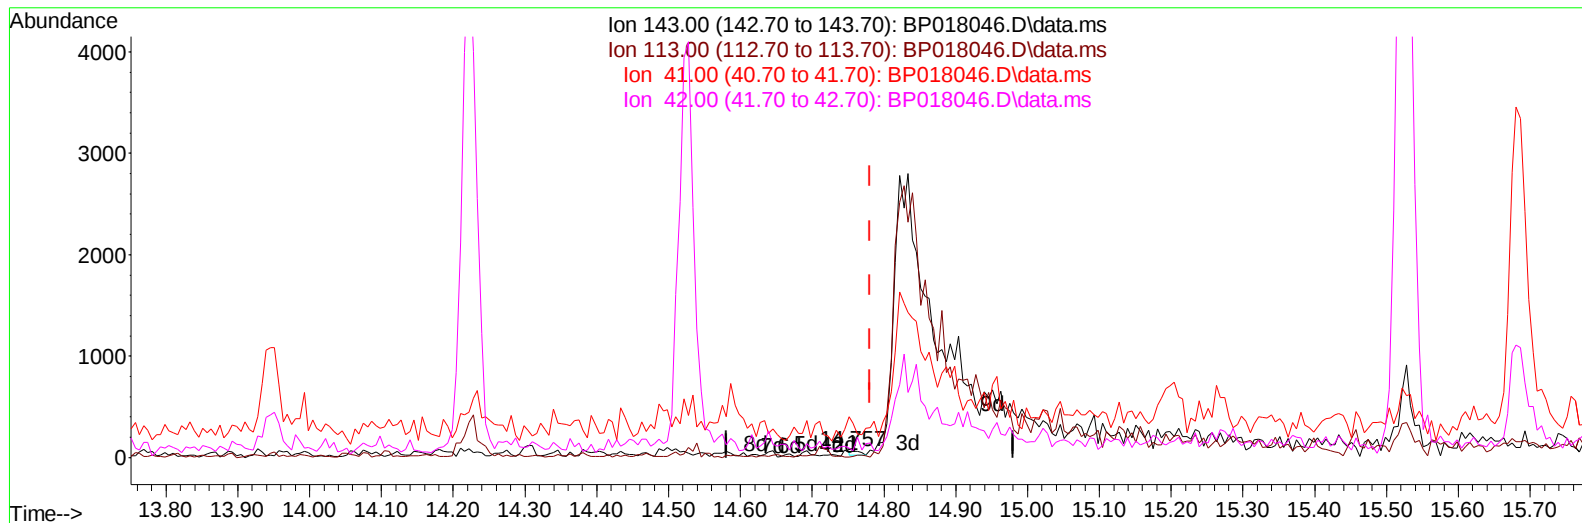

TIC: BP018046.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.023) 0.02 ng/u1

response 33

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	16.13#
41.00	47.70	546.77#
42.00	30.10	109.68#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018046.D
 Acq On : 11 Nov 2023 03:22
 Operator : MA/JU
 Sample : 05057-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49G7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2023
 Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 11 03:52:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	56131	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	224038	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.528	164	140401	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	312551	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	301690	20.000	ng/ul	0.00
88) Perylene-d12	23.933	264	356221	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	5820	3.658	ng/uL	0.00
4) Pyridine-d5	3.675	84	40209	9.692	ng/ul	0.01
7) Phenol-d5	7.028	99	37362	6.895	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.199	67	97663	30.667	ng/ul	0.00
11) 2-Chlorophenol-d4	7.375	132	103776	24.183	ng/ul	0.00
15) 4-Methylphenol-d8	8.581	113	70603	15.900	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	65776	32.587	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	72896	31.878	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.298	165	115691	28.386	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	157754	28.225	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	430113	33.202	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	456201	32.332	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	12259m	6.333	ng/ul	0.05
60) Fluorene-d10	15.528	176	362511	33.894	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	52772	23.356	ng/ul	0.00
73) Anthracene-d10	17.404	188	653530	38.661	ng/ul	0.00
81) Pyrene-d10	19.657	212	800620	39.730	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.768	264	838812	40.496	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018046.D
Acq On : 11 Nov 2023 03:22
Operator : MA/JU
Sample : 05057-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49G7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/11/2023
Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 11 03:52:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

