




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018058.D
 Acq On : 11 Nov 2023 10:43
 Operator : MA/JU
 Sample : PB156765BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK765

Manual IntegrationsAPPROVED

Quant Time: Nov 11 20:27:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2023
 Supervised By :mohammad ahmed 11/15/2023

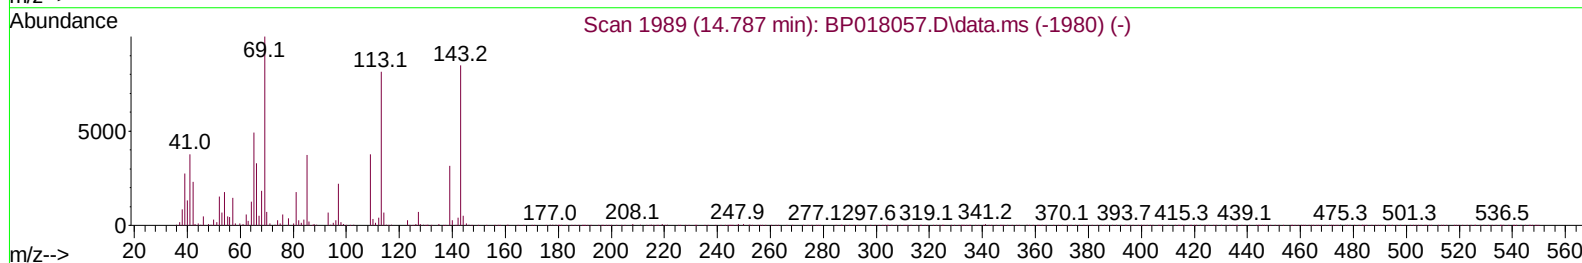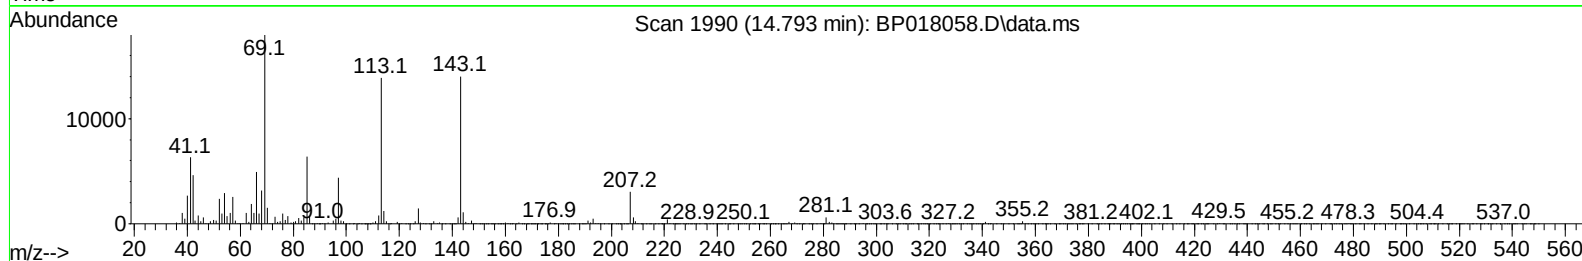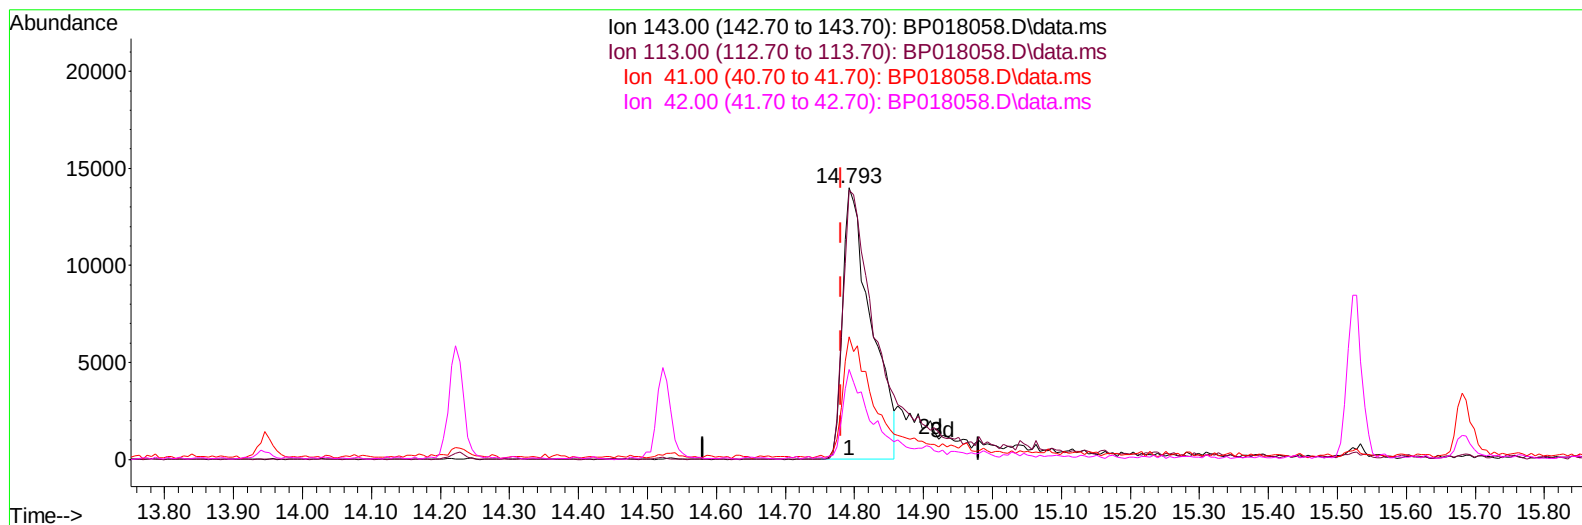

TIC: BP018058.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.793min (+ 0.012) 18.98 ng/ul

response 39857

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	99.11
41.00	47.70	45.19
42.00	30.10	33.08




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018058.D
 Acq On : 11 Nov 2023 10:43
 Operator : MA/JU
 Sample : PB156765BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK765

Manual IntegrationsAPPROVED

Quant Time: Nov 11 20:27:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2023
 Supervised By :mohammad ahmed 11/15/2023

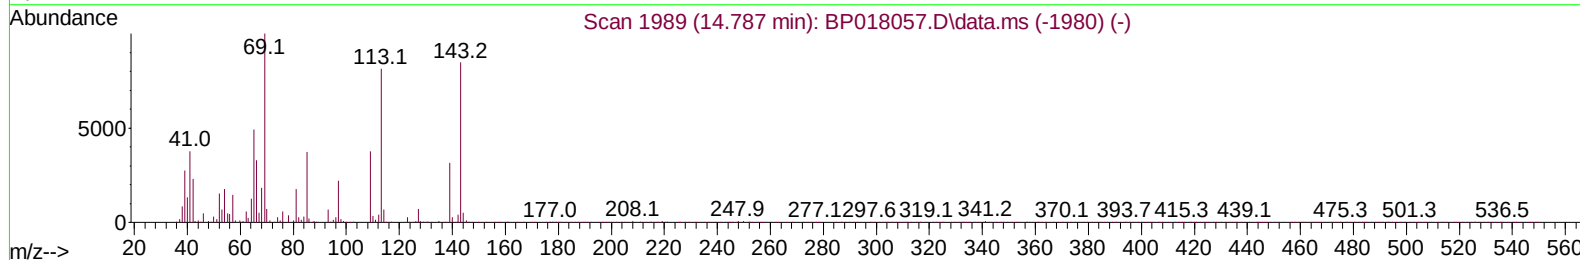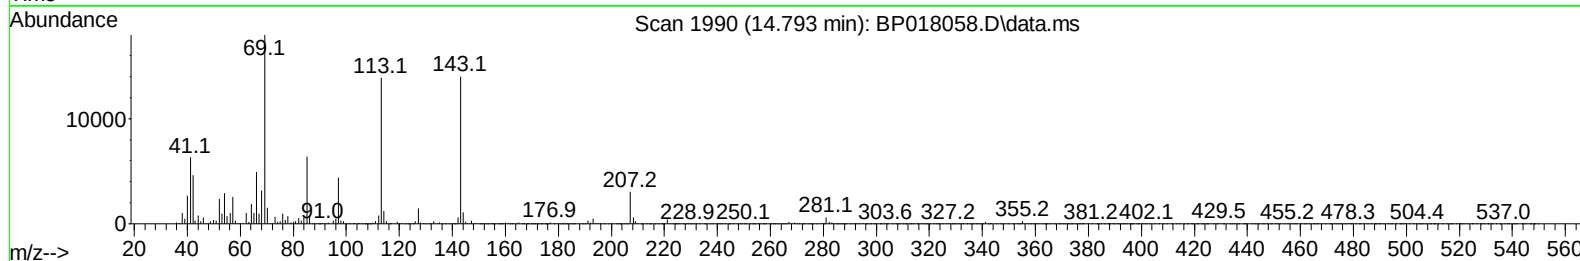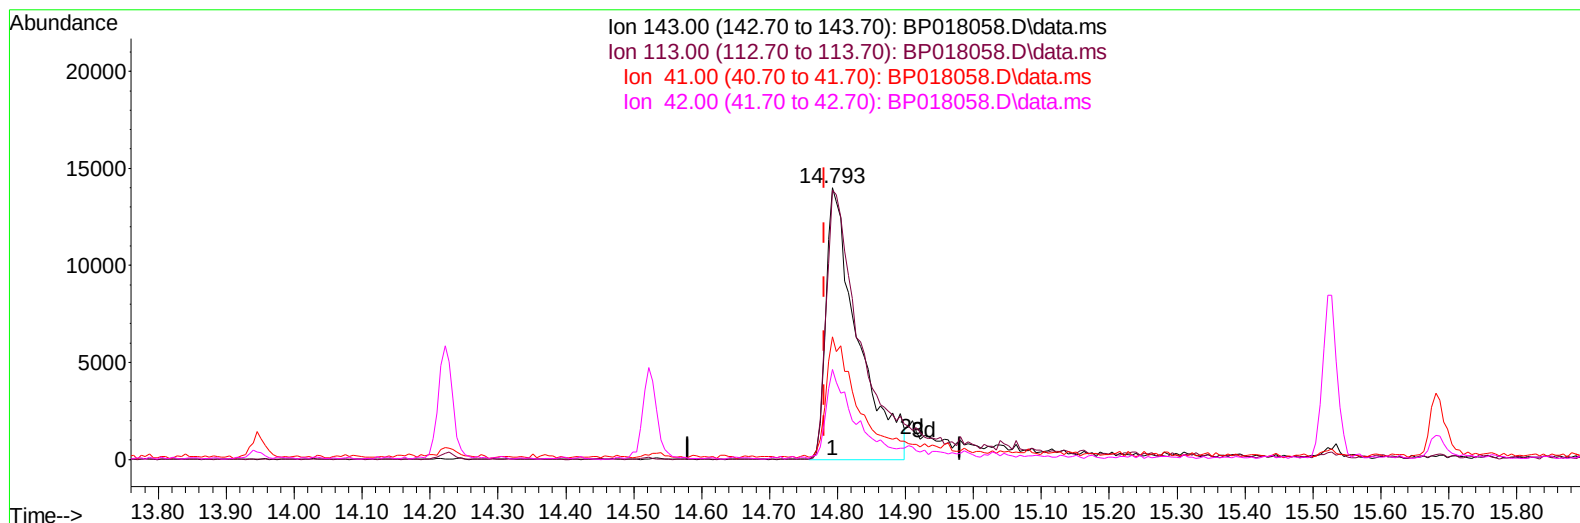

TIC: BP018058.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.793min (+ 0.012) 21.61 ng/ul m

response 45380

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	99.11
41.00	47.70	45.19
42.00	30.10	33.08

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018058.D
 Acq On : 11 Nov 2023 10:43
 Operator : MA/JU
 Sample : PB156765BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK765

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2023
 Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 11 20:28:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	66375	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	263342	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	152328	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	302201	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	259959	20.000	ng/ul	0.00
88) Perylene-d12	23.933	264	316780	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	12503	6.645	ng/uL	0.00
4) Pyridine-d5	3.664	84	153815	31.353	ng/ul	0.00
7) Phenol-d5	7.016	99	191154	29.830	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	122438	32.513	ng/ul	0.00
11) 2-Chlorophenol-d4	7.369	132	154976	30.540	ng/ul	0.00
15) 4-Methylphenol-d8	8.569	113	155725	29.656	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	73424	30.947	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	86007	31.998	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	136560	28.505	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131	184544	28.090	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	439391	31.262	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	498570	32.569	ng/ul	0.00
54) 4-Nitrophenol-d4	14.793	143	45380m	21.607	ng/ul	0.01
60) Fluorene-d10	15.528	176	366192	31.558	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	56344	25.790	ng/ul	0.00
73) Anthracene-d10	17.404	188	541445	33.128	ng/ul	0.00
81) Pyrene-d10	19.657	212	592632	34.130	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.769	264	632407	34.333	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018058.D
Acq On : 11 Nov 2023 10:43
Operator : MA/JU
Sample : PB156765BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK765

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2023
Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 11 20:28:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

