




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018066.D
Acq On : 11 Nov 2023 15:13
Operator : MA/JU
Sample : 05105-01
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0004

Manual IntegrationsAPPROVED

Quant Time: Nov 11 21:40:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2023
Supervised By :mohammad ahmed 11/15/2023

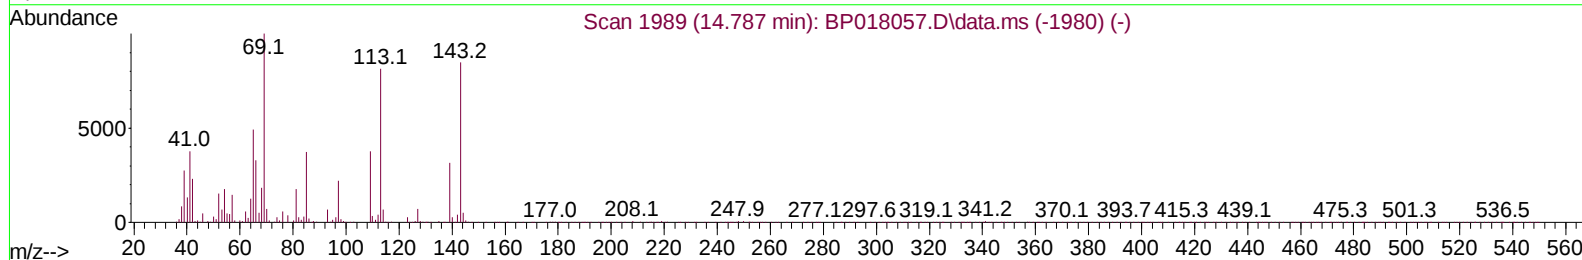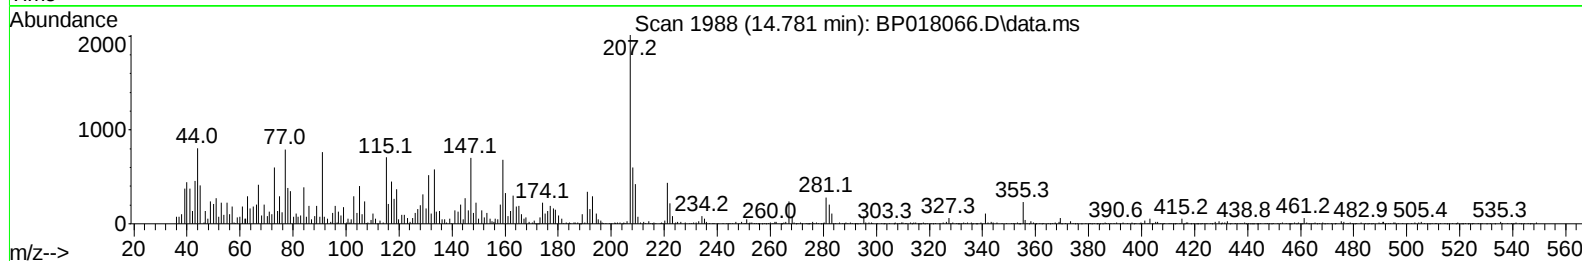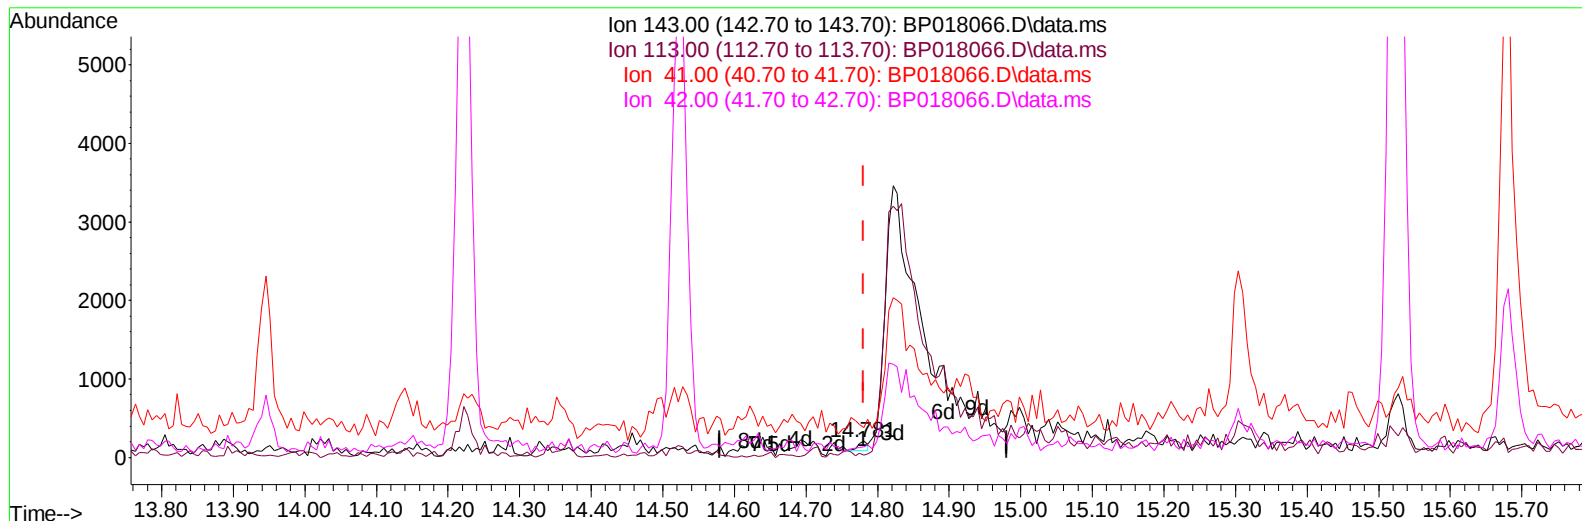

TIC: BP018066.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.781min (+ 0.000) 0.04 ng/u1

response 116

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	15.12#
41.00	47.70	183.90#
42.00	30.10	66.34#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018066.D
 Acq On : 11 Nov 2023 15:13
 Operator : MA/JU
 Sample : 05105-01
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0004

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2023
 Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 11 21:41:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	80966	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	347730	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	224124	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	451931	20.000	ng/ul	0.00
79) Chrysene-d12	21.433	240	343119	20.000	ng/ul	0.00
88) Perylene-d12	23.933	264	387903	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	7080	3.085	ng/uL	0.00
4) Pyridine-d5	3.669	84	51784	8.653	ng/ul	0.00
7) Phenol-d5	7.028	99	48247	6.172	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.199	67	137585	29.951	ng/ul	0.00
11) 2-Chlorophenol-d4	7.369	132	139256	22.497	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	96027	14.992	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	87788	28.022	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	100726	28.380	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.299	165	167790	26.525	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	185387	21.370	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	625919	30.268	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	648476	28.791	ng/ul	0.00
54) 4-Nitrophenol-d4	14.822	143	10690m	3.459	ng/ul	0.04
60) Fluorene-d10	15.528	176	505393	29.602	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	89484	27.389	ng/ul	0.00
73) Anthracene-d10	17.404	188	809397	33.115	ng/ul	0.00
81) Pyrene-d10	19.657	212	901083	39.316	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.768	264	810435	35.931	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018066.D
Acq On : 11 Nov 2023 15:13
Operator : MA/JU
Sample : 05105-01
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0004

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2023
Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 11 21:41:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

