




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018072.D
 Acq On : 11 Nov 2023 18:36
 Operator : MA/JU
 Sample : 05044-14
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEH6

Manual IntegrationsAPPROVED

Quant Time: Nov 11 22:02:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2023
 Supervised By :mohammad ahmed 11/15/2023

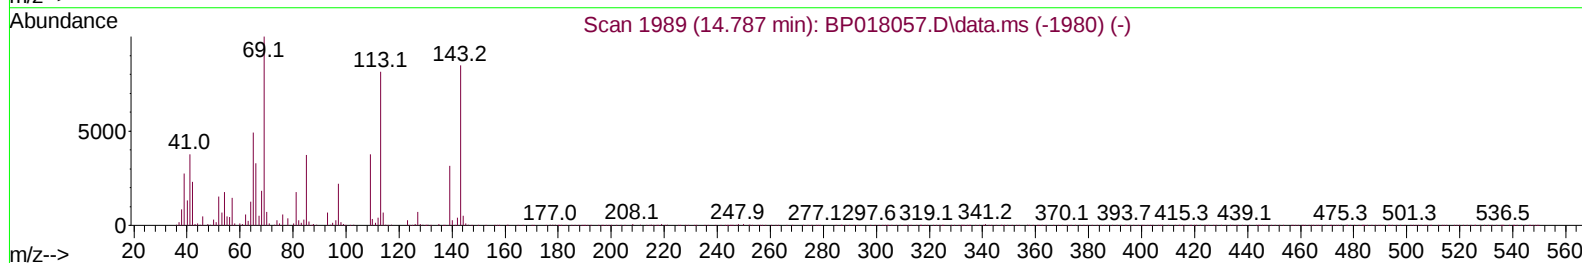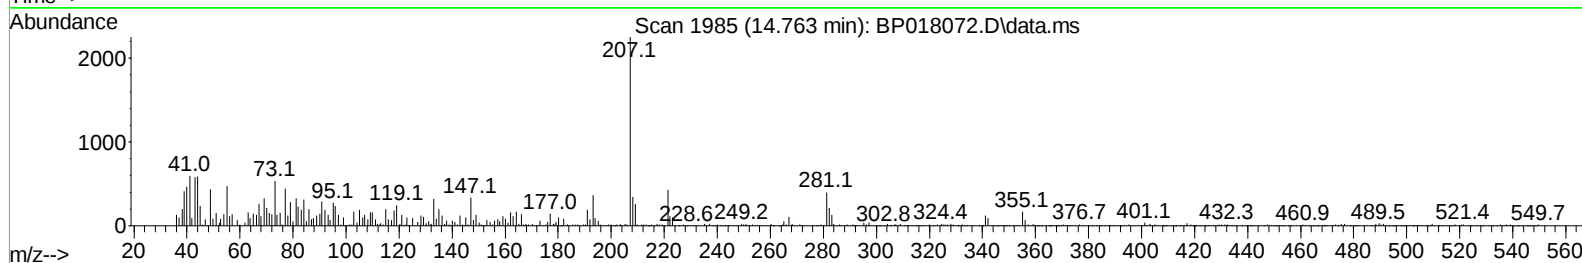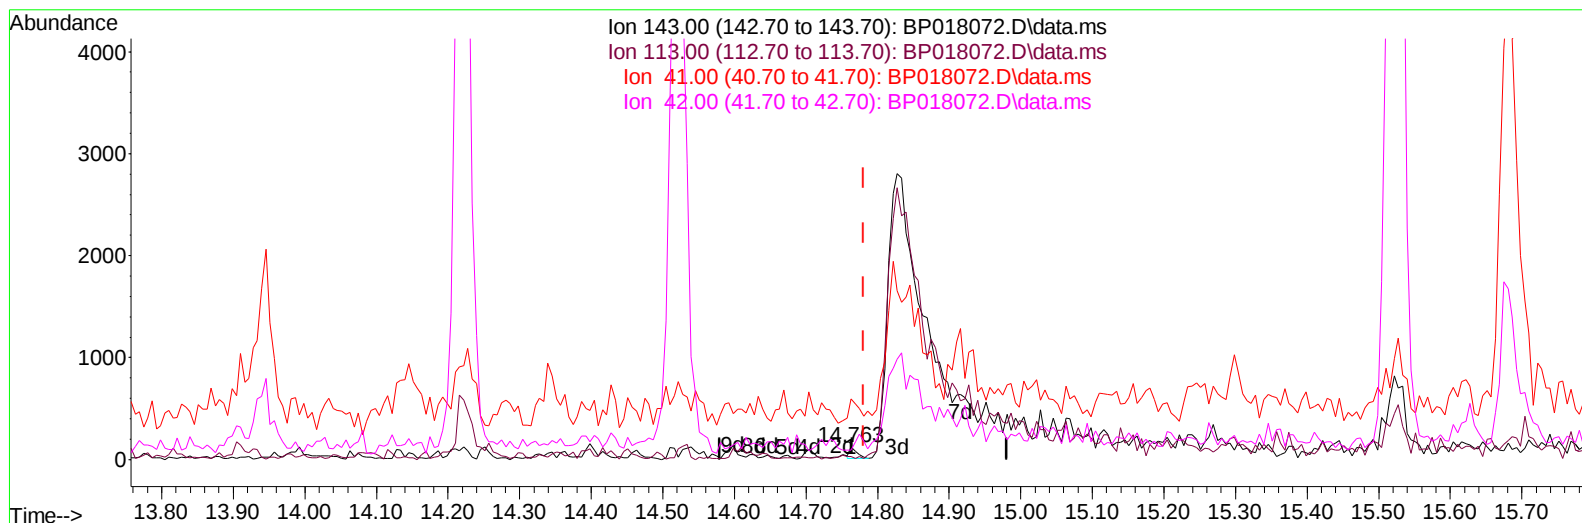

TIC: BP018072.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.763min (-0.017) 0.03 ng/u1

response 83

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	22.13#
41.00	47.70	487.70#
42.00	30.10	77.05#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018072.D
 Acq On : 11 Nov 2023 18:36
 Operator : MA/JU
 Sample : 05044-14
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEH6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2023
 Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 11 22:03:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	85267	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	339441	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.522	164	205347	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	403496	20.000	ng/ul	0.00
79) Chrysene-d12	21.427	240	353220	20.000	ng/ul	0.00
88) Perylene-d12	23.933	264	415338	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	9456	3.912	ng/uL	0.00
4) Pyridine-d5	3.669	84	69686	11.057	ng/ul	0.00
7) Phenol-d5	7.022	99	49673	6.034	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	143178	29.596	ng/ul	0.00
11) 2-Chlorophenol-d4	7.369	132	142112	21.800	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	93397	13.846	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	90264	29.516	ng/ul	0.00
24) 2-Nitrophenol-d4	9.769	143	99091	28.601	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.299	165	163366	26.456	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	181167	21.394	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	595350	31.422	ng/ul	0.00
49) Acenaphthylene-d8	14.222	160	626408	30.354	ng/ul	0.00
54) 4-Nitrophenol-d4	14.828	143	10703m	3.780	ng/ul	0.05
60) Fluorene-d10	15.522	176	488916	31.255	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	68599	23.517	ng/ul	0.00
73) Anthracene-d10	17.404	188	744256	34.105	ng/ul	0.00
81) Pyrene-d10	19.657	212	849227	35.994	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.768	264	875708	36.260	ng/ul	0.00
Target Compounds						Qvalue
34) Caprolactam	11.704	113	14051	7.173	ng/ul	90
59) Diethylphthalate	15.345	149	106270	5.473	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018072.D
Acq On : 11 Nov 2023 18:36
Operator : MA/JU
Sample : 05044-14
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEH6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2023
Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 11 22:03:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

