




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018090.D
Acq On : 12 Nov 2023 05:21
Operator : MA/JU
Sample : 05082-01
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH321

Manual IntegrationsAPPROVED

Quant Time: Nov 12 15:20:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :mohammad ahmed 11/15/2023

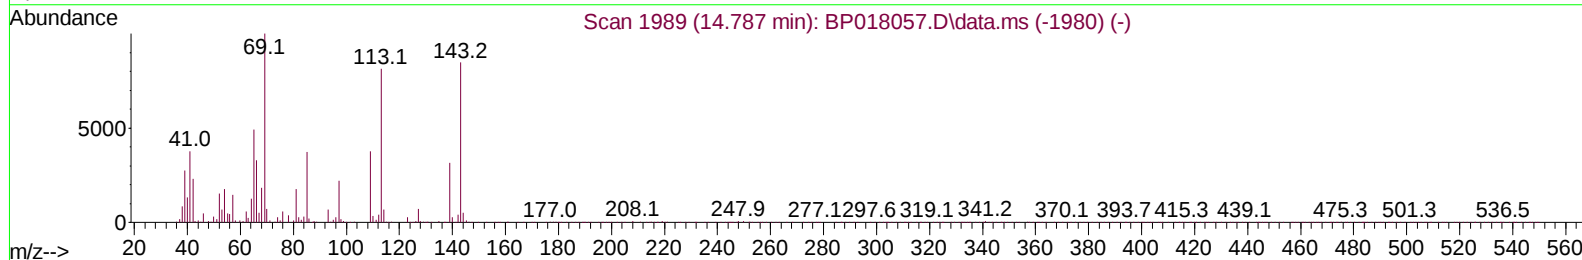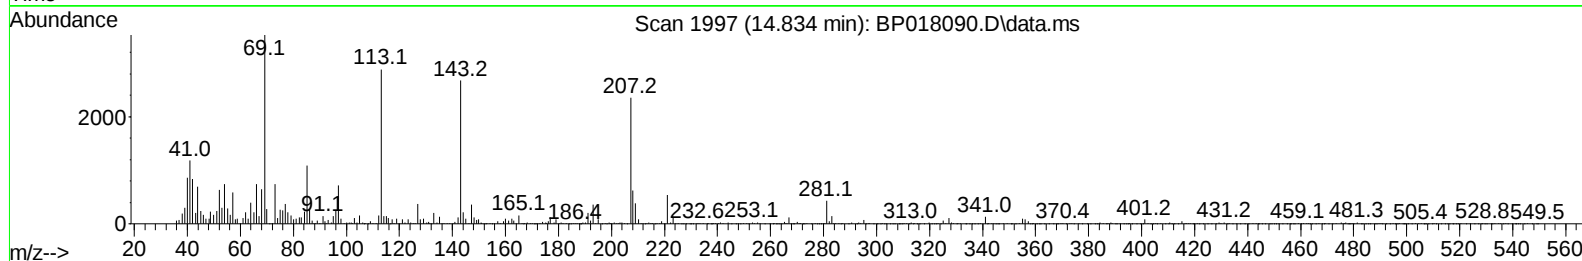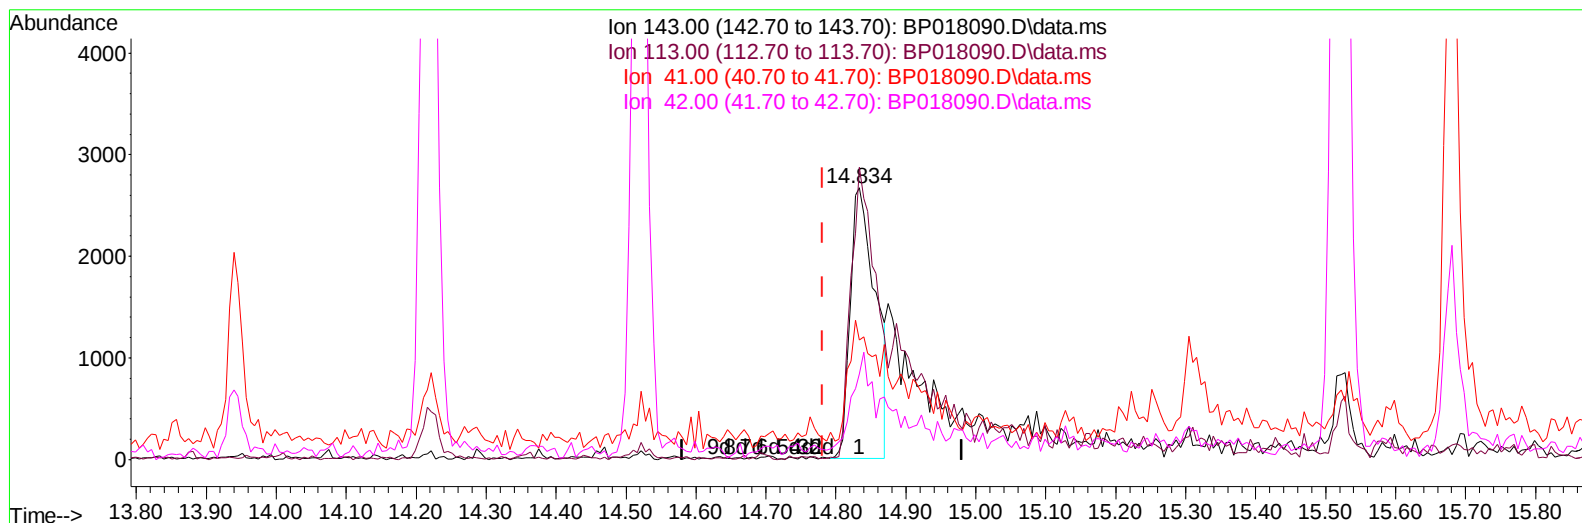

TIC: BP018090.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.834min (+ 0.053) 1.79 ng/u1

response 6619

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	107.74
41.00	47.70	44.03
42.00	30.10	31.43




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018090.D
Acq On : 12 Nov 2023 05:21
Operator : MA/JU
Sample : 05082-01
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH321

Manual IntegrationsAPPROVED

Quant Time: Nov 12 15:20:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :mohammad ahmed 11/15/2023

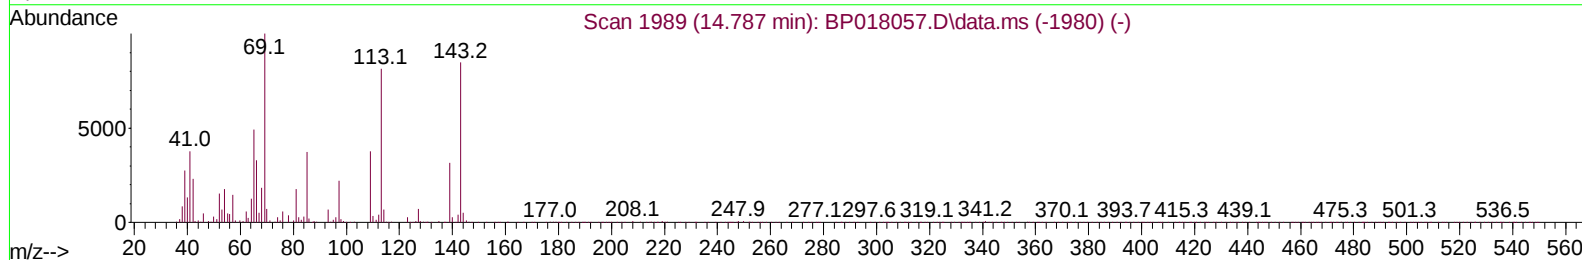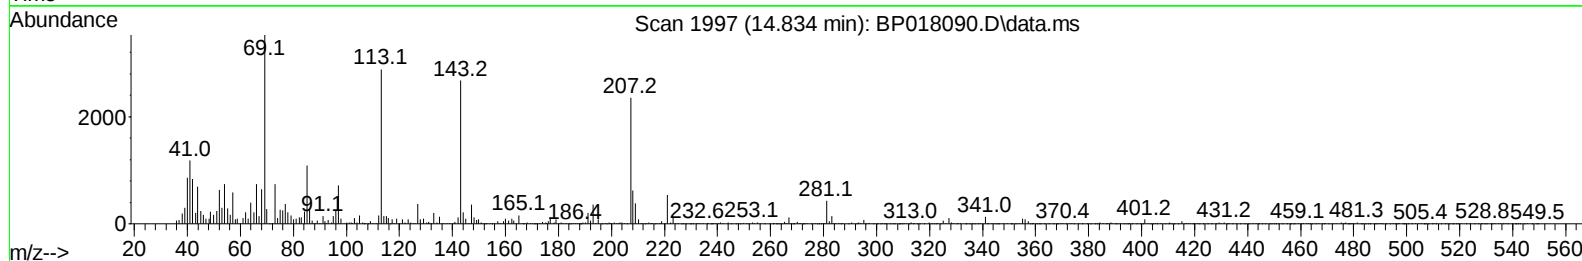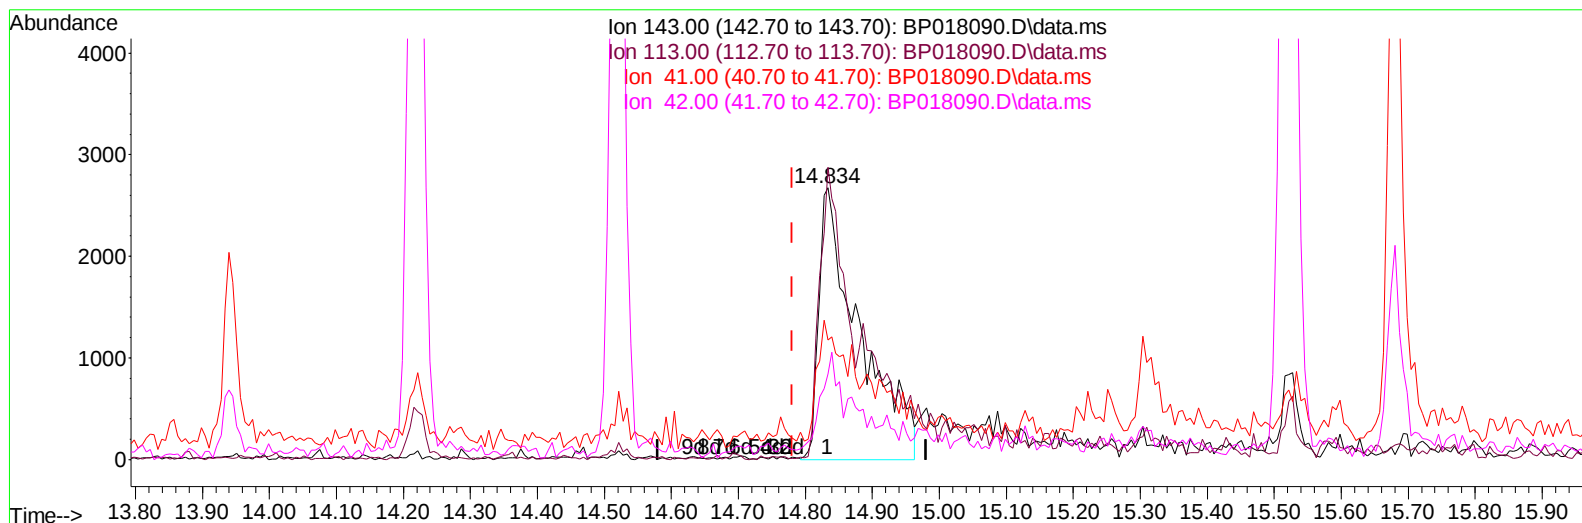

TIC: BP018090.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.834min (+ 0.053) 3.04 ng/ul m

response 11268

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	107.74
41.00	47.70	44.03
42.00	30.10	31.43

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018090.D
 Acq On : 12 Nov 2023 05:21
 Operator : MA/JU
 Sample : 05082-01
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH321

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/13/2023
 Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 12 15:21:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	101436	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	435944	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.522	164	268626	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	514215	20.000	ng/ul	-0.01
79) Chrysene-d12	21.427	240	405244	20.000	ng/ul	0.00
88) Perylene-d12	23.927	264	484284	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	9384	3.263	ng/uL	0.00
4) Pyridine-d5	3.669	84	52060	6.944	ng/ul	0.00
7) Phenol-d5	7.022	99	51980	5.308	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.193	67	166133	28.867	ng/ul	0.00
11) 2-Chlorophenol-d4	7.369	132	160047	20.638	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	107315	13.373	ng/ul	0.00
21) Nitrobenzene-d5	9.052	128	107772	27.440	ng/ul	0.00
24) 2-Nitrophenol-d4	9.763	143	115888	26.044	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	189576	23.904	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	249219	22.915	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	728226	29.381	ng/ul	-0.01
49) Acenaphthylene-d8	14.222	160	762660	28.251	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	11268m	3.042	ng/ul	0.05
60) Fluorene-d10	15.522	176	589736	28.819	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	83552	22.476	ng/ul	0.00
73) Anthracene-d10	17.404	188	944798	33.972	ng/ul	0.00
81) Pyrene-d10	19.657	212	1005776	37.156	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.763	264	1012662	35.961	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018090.D
Acq On : 12 Nov 2023 05:21
Operator : MA/JU
Sample : 05082-01
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH321

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 12 15:21:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

