




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018125.D
 Acq On : 13 Nov 2023 03:21
 Operator : MA/JU
 Sample : 05158-03
 Misc :
 ALS Vial : 106 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH368

Manual IntegrationsAPPROVED

Quant Time: Nov 13 03:55:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2023
 Supervised By :mohammad ahmed 11/15/2023

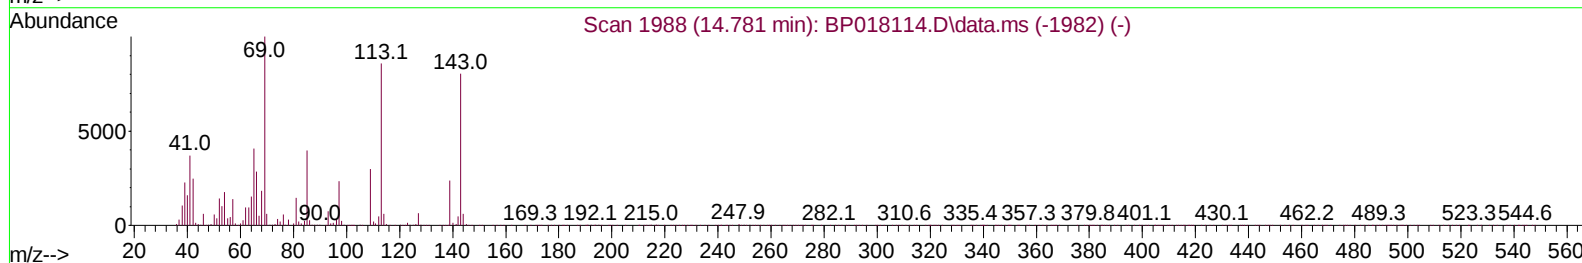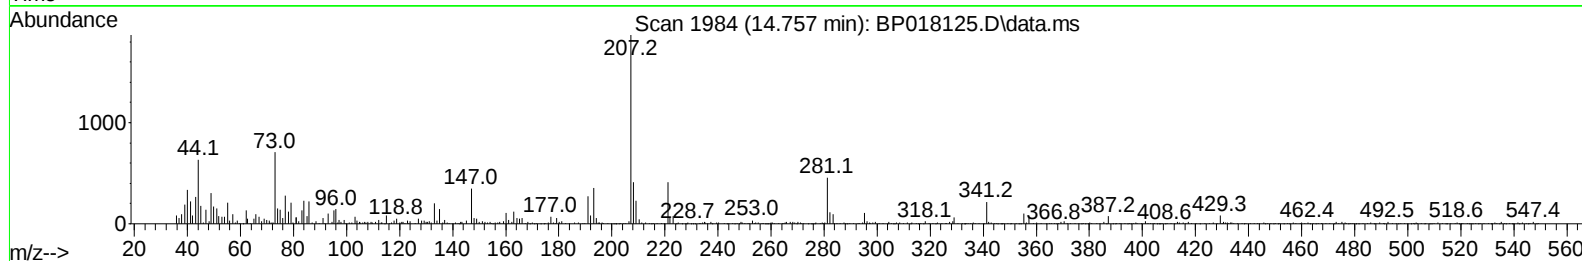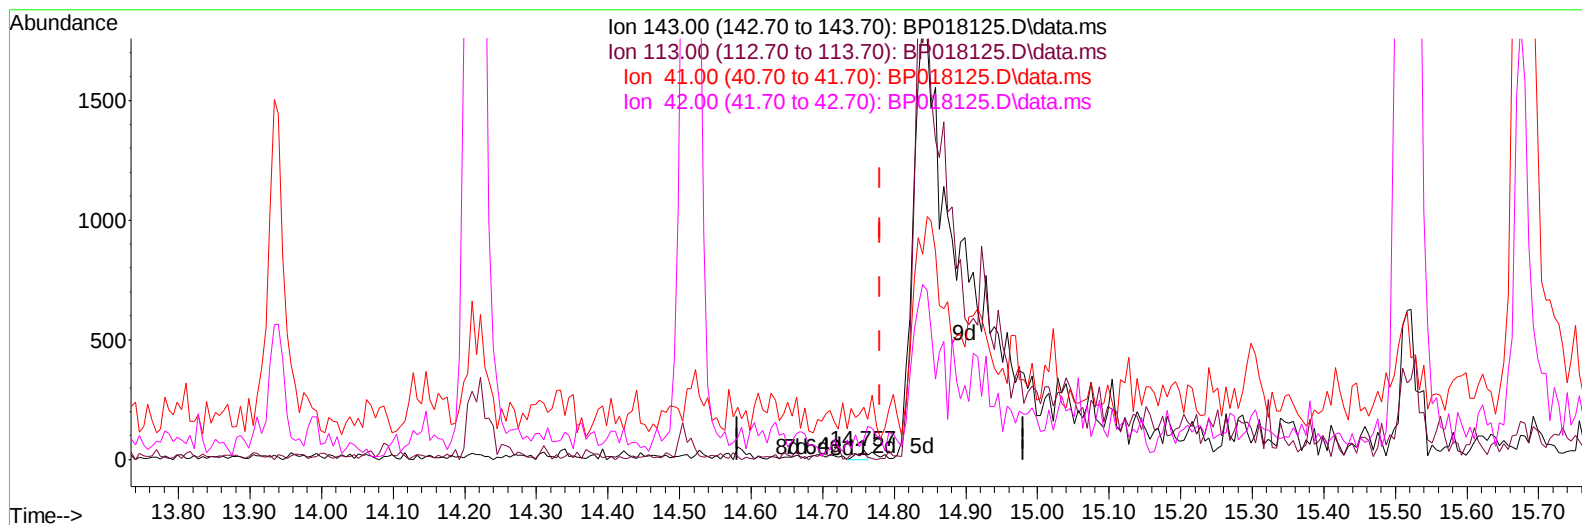

TIC: BP018125.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.757min (-0.023) 0.02 ng/u1

response 36

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	66.67#
41.00	47.70	561.54#
42.00	30.10	217.95#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018125.D
 Acq On : 13 Nov 2023 03:21
 Operator : MA/JU
 Sample : 05158-03
 Misc :
 ALS Vial : 106 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH368

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2023
 Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 13 03:56:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	64822	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.657	136	255544	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.516	164	156302	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.298	188	365720	20.000	ng/ul	-0.01
79) Chrysene-d12	21.427	240	371869	20.000	ng/ul	0.00
88) Perylene-d12	23.927	264	422444	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	6736	3.666	ng/uL	0.00
4) Pyridine-d5	3.675	84	17587	3.671	ng/ul	0.01
7) Phenol-d5	7.022	99	34984	5.590	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	123225	33.506	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.364	132	120073	24.229	ng/ul	-0.01
15) 4-Methylphenol-d8	8.569	113	72484	14.135	ng/ul	0.00
21) Nitrobenzene-d5	9.046	128	76079	33.045	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.763	143	84629	32.446	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	133238	28.661	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131	75697	11.874	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	515320	35.732	ng/ul	-0.01
49) Acenaphthylene-d8	14.216	160	527806	33.602	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.840	143	8396m	3.896	ng/ul	0.06
60) Fluorene-d10	15.516	176	436067	36.624	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.675	200	81307	30.753	ng/ul	-0.01
73) Anthracene-d10	17.398	188	740193	37.422	ng/ul	-0.01
81) Pyrene-d10	19.651	212	952601	38.350	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.757	264	952061	38.759	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018125.D
Acq On : 13 Nov 2023 03:21
Operator : MA/JU
Sample : 05158-03
Misc :
ALS Vial : 106 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH368

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2023
Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 13 03:56:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

