




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018126.D
 Acq On : 13 Nov 2023 03:55
 Operator : MA/JU
 Sample : 05158-04
 Misc :
 ALS Vial : 107 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH371

Manual IntegrationsAPPROVED

Quant Time: Nov 13 04:41:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2023
 Supervised By :mohammad ahmed 11/15/2023

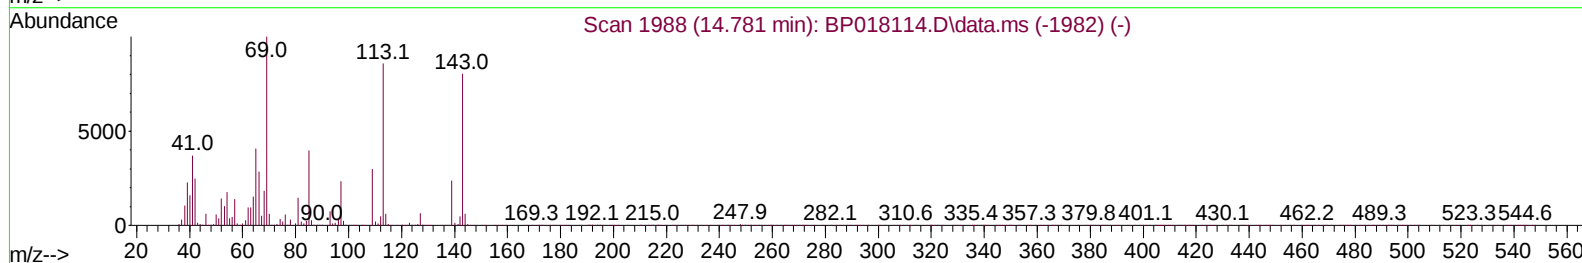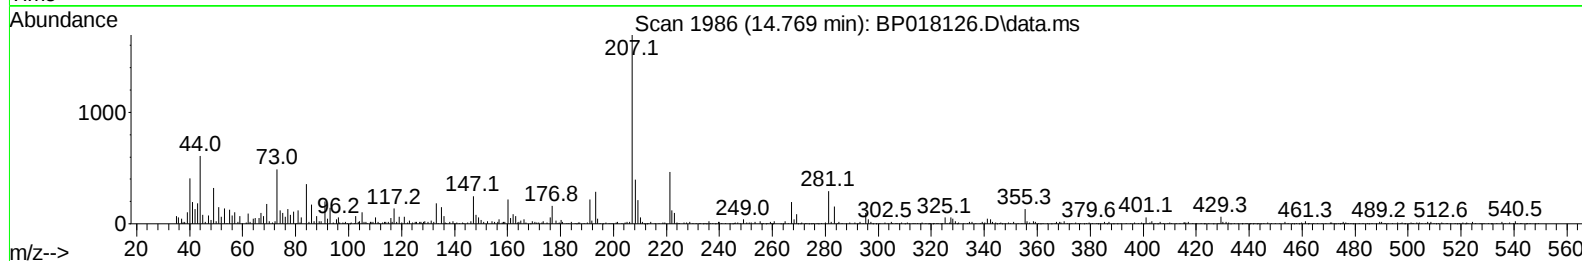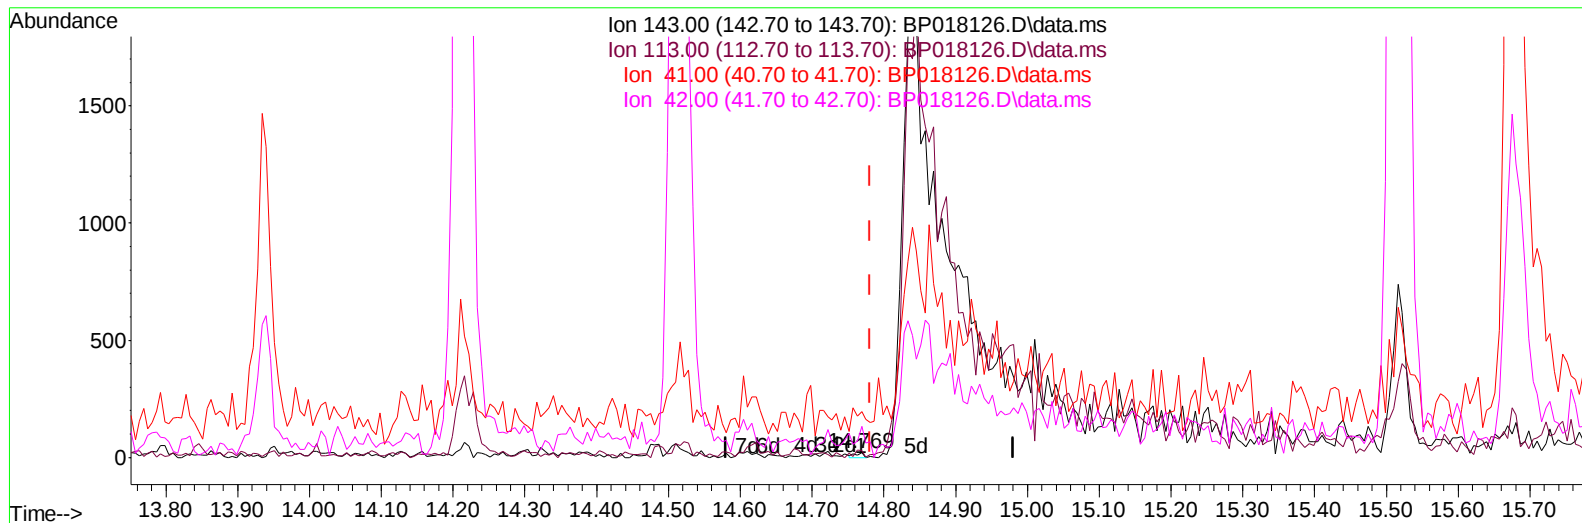

TIC: BP018126.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.769min (-0.011) 0.01 ng/u1

response 16

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	150.00#
41.00	47.70	980.00#
42.00	30.10	670.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018126.D
Acq On : 13 Nov 2023 03:55
Operator : MA/JU
Sample : 05158-04
Misc :
ALS Vial : 107 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH371

Manual IntegrationsAPPROVED

Quant Time: Nov 13 04:41:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2023
Supervised By :mohammad ahmed 11/15/2023

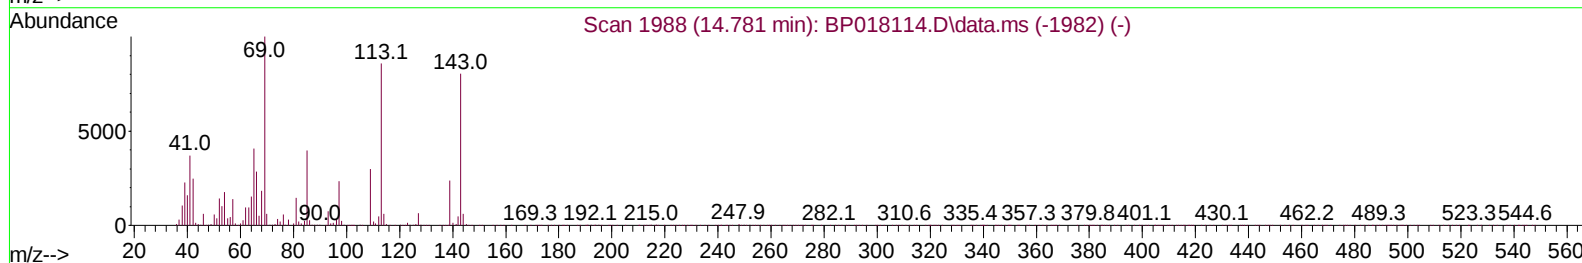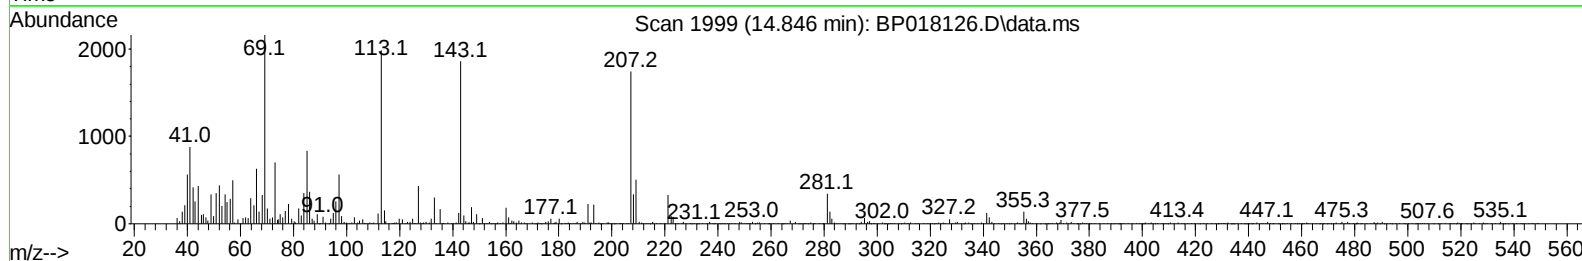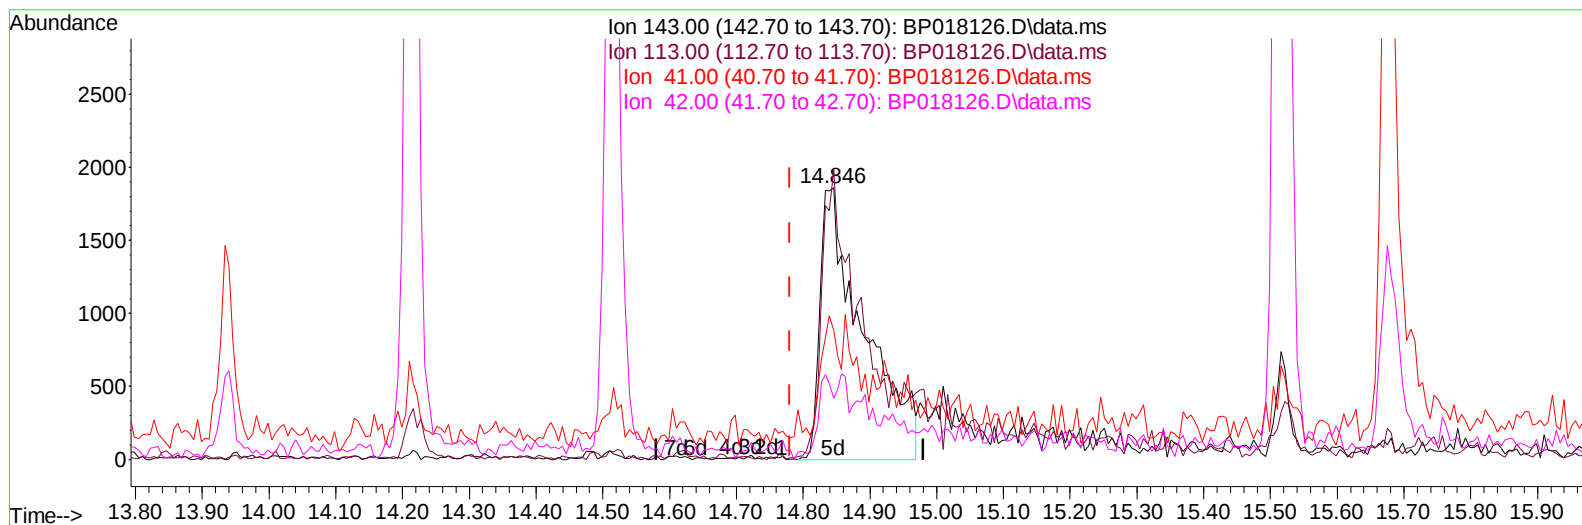

TIC: BP018126.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.846min (+ 0.065) 3.92 ng/ul m

response 8398

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.00	106.67
41.00	47.70	47.44
42.00	30.10	22.54#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018126.D
 Acq On : 13 Nov 2023 03:55
 Operator : MA/JU
 Sample : 05158-04
 Misc :
 ALS Vial : 107 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH371

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2023
 Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 13 04:42:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	63466	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.658	136	254787	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.516	164	155378	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.298	188	370703	20.000	ng/ul	-0.01
79) Chrysene-d12	21.422	240	385407	20.000	ng/ul	-0.01
88) Perylene-d12	23.927	264	444225	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	6038	3.356	ng/uL	0.00
4) Pyridine-d5	3.670	84	42450	9.049	ng/ul	0.00
7) Phenol-d5	7.022	99	33392	5.450	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.193	67	105688	29.351	ng/ul	0.00
11) 2-Chlorophenol-d4	7.364	132	104057	21.446	ng/ul	-0.01
15) 4-Methylphenol-d8	8.569	113	67456	13.435	ng/ul	0.00
21) Nitrobenzene-d5	9.046	128	66478	28.960	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.763	143	71969	27.674	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	116116	25.052	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	147737	23.243	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	463657	32.341	ng/ul	-0.01
49) Acenaphthylene-d8	14.216	160	468327	29.992	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.846	143	8398m	3.920	ng/ul	0.07
60) Fluorene-d10	15.516	176	385664	32.583	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.822	200	266	0.099	ng/ul	0.14
73) Anthracene-d10	17.398	188	694439	34.637	ng/ul	-0.01
81) Pyrene-d10	19.651	212	884765	34.368	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.757	264	909411	35.207	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018126.D
Acq On : 13 Nov 2023 03:55
Operator : MA/JU
Sample : 05158-04
Misc :
ALS Vial : 107 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH371

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2023
Supervised By :mohammad ahmed 11/15/2023

Quant Time: Nov 13 04:42:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

