

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018073.D
 Acq On : 11 Nov 2023 19:10
 Operator : MA/JU
 Sample : 05044-15
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEG1

Quant Time: Nov 11 22:04:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 10 21:55:18 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.845	152	72325	20.000	ng/u1	0.00
20) Naphthalene-d8	10.669	136	277595	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.522	164	163320	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.304	188	345887	20.000	ng/u1	0.00
79) Chrysene-d12	21.427	240	350607	20.000	ng/u1	0.00
88) Perylene-d12	23.933	264	409006	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	9613	4.689	ng/uL	0.00
4) Pyridine-d5	3.669	84	68037	12.727	ng/u1	0.00
7) Phenol-d5	7.028	99	45914	6.576	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.198	67	129800	31.632	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	131577	23.796	ng/u1	0.00
15) 4-Methylphenol-d8	8.575	113	82737	14.460	ng/u1	0.00
21) Nitrobenzene-d5	9.057	128	79972	31.976	ng/u1	0.00
24) 2-Nitrophenol-d4	9.769	143	88632	31.281	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.298	165	146298	28.970	ng/u1	0.00
31) 4-Chloroaniline-d4	10.851	131	168776	24.371	ng/u1	0.00
46) Dimethylphthalate-d6	13.945	166	529501	35.138	ng/u1	0.00
49) Acenaphthylene-d8	14.222	160	546665	33.307	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	12099	5.373	ng/u1	0.05
60) Fluorene-d10	15.527	176	435307	34.989	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.680	200	84160	33.657	ng/u1	0.00
73) Anthracene-d10	17.404	188	713157	38.123	ng/u1	0.00
81) Pyrene-d10	19.657	212	884941	37.787	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.768	264	955530	40.178	ng/u1	0.00
Target Compounds						
34) Caprolactam	11.710	113	13689	8.545	ng/u1	94
59) Diethylphthalate	15.351	149	75978	4.920	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018073.D
Acq On : 11 Nov 2023 19:10
Operator : MA/JU
Sample : 05044-15
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEG1

Quant Time: Nov 11 22:04:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 10 21:55:18 2023
Response via : Initial Calibration

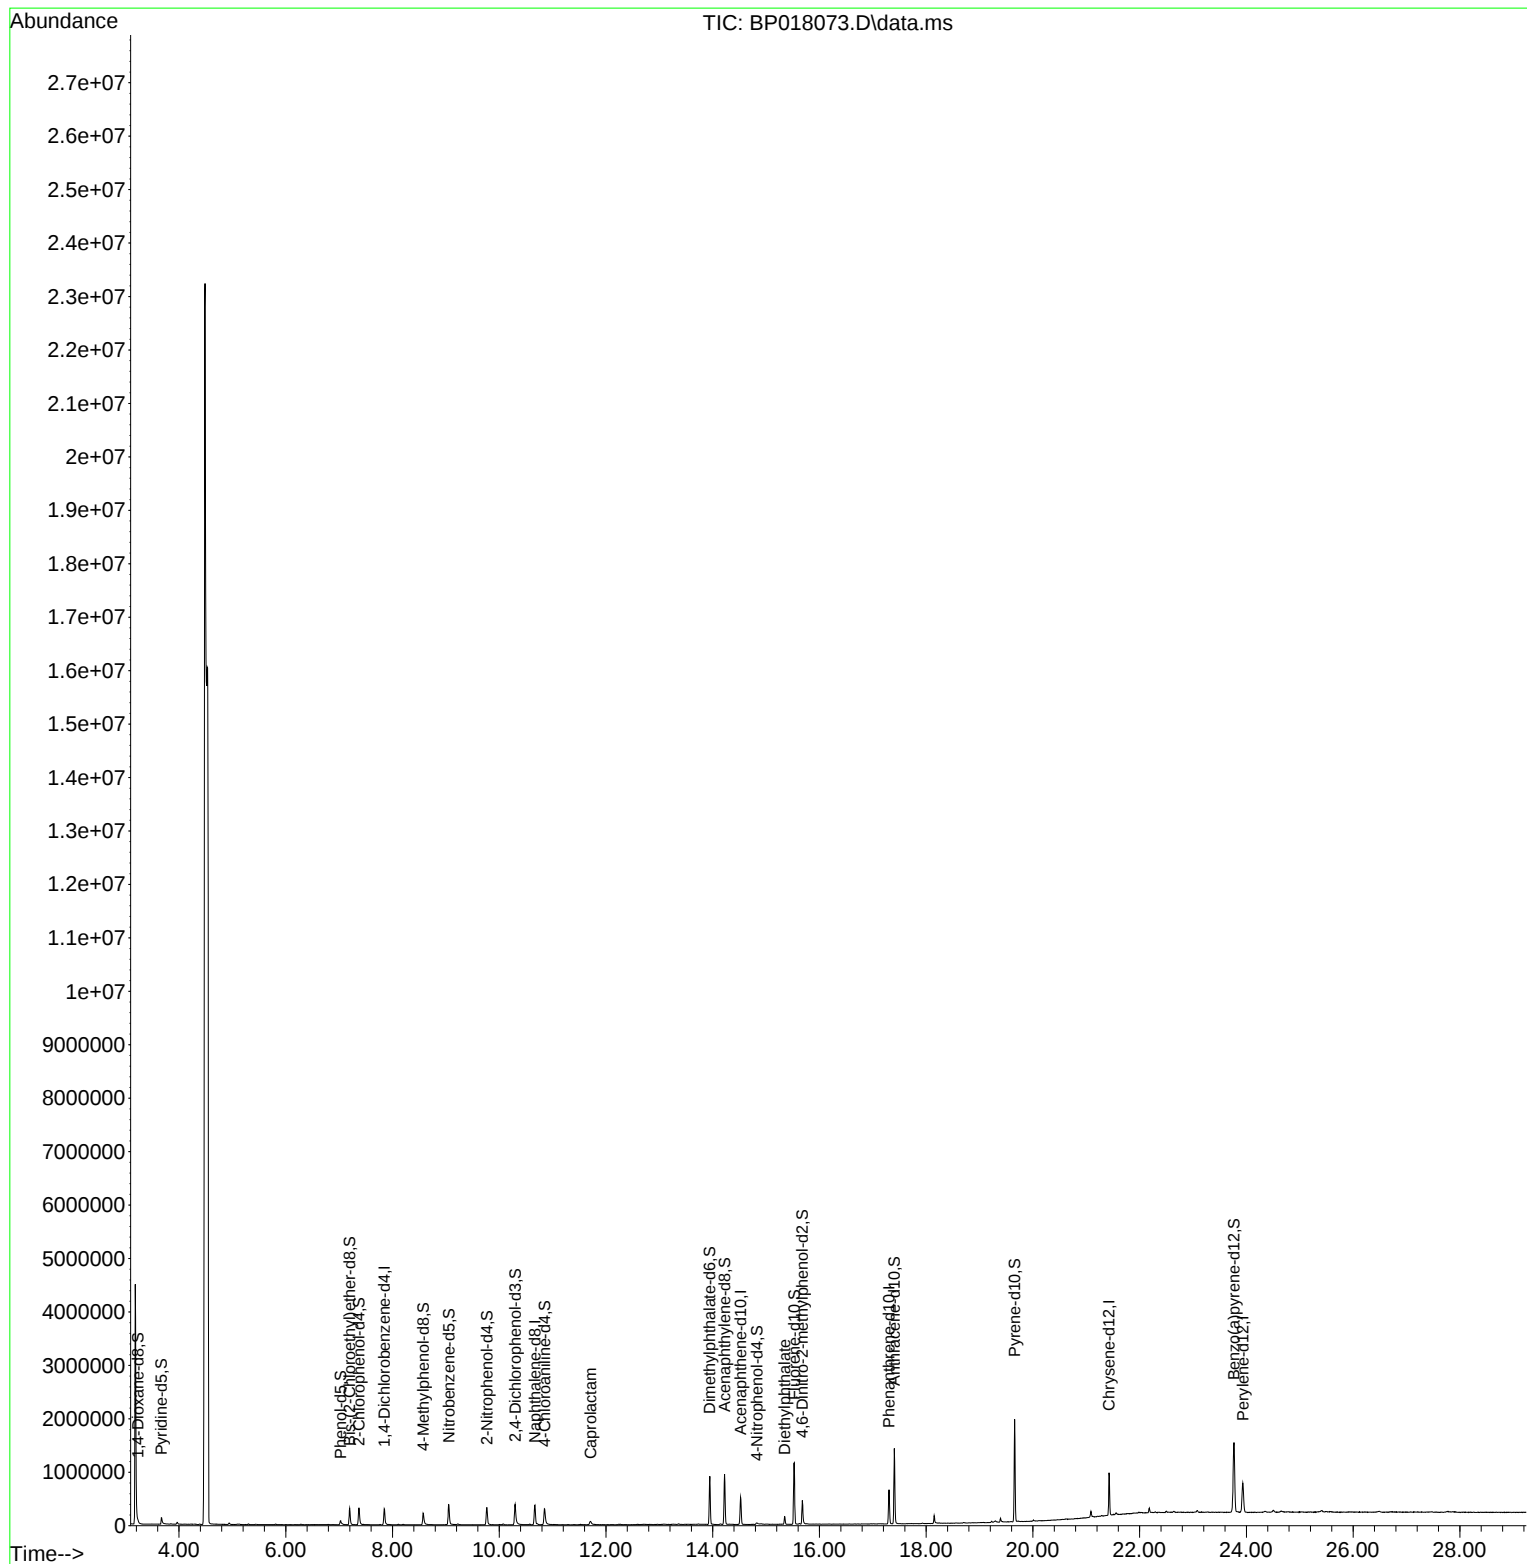

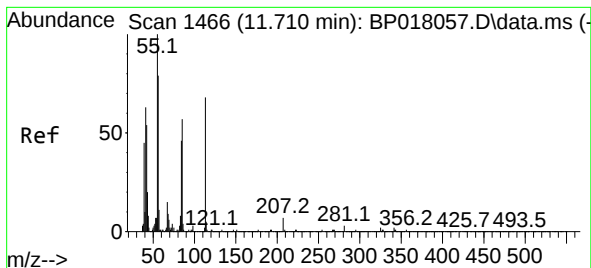

#34

Caprolactam

Concen: 8.545 ng/ul

RT: 11.710 min Scan# 1466

Delta R.T. -0.012 min

Lab File: BP018073.D

Acq: 11 Nov 2023 19:10

Instrument :

BNA_P

ClientSampleId :

BHEG1





Tgt Ion:113 Resp: 13689

Ion Ratio Lower Upper

113 100

55 157.4 118.3 177.5

56 114.4 95.6 143.4

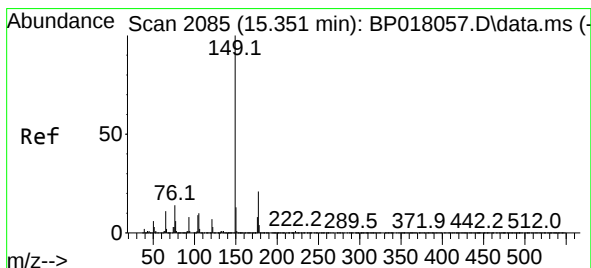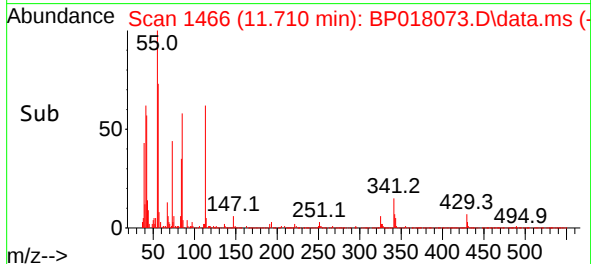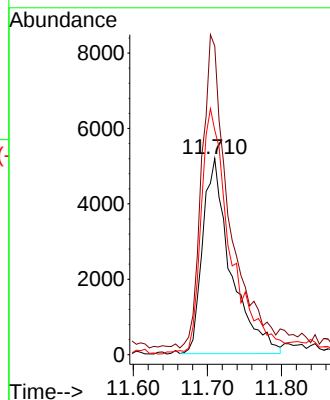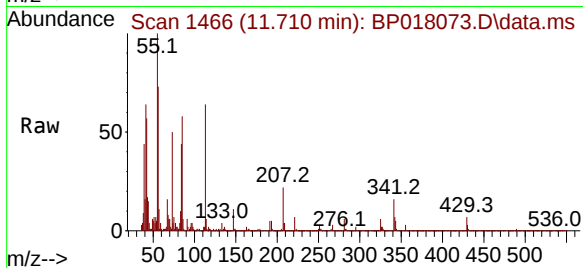

#59

Diethylphthalate

Concen: 4.920 ng/ul

RT: 15.351 min Scan# 2085

Delta R.T. -0.000 min

Lab File: BP018073.D

Acq: 11 Nov 2023 19:10

Tgt Ion:149 Resp: 75978

Ion Ratio Lower Upper

149 100

177 21.0 16.3 24.5

150 12.3 10.0 15.0

