

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018035.D
 Acq On : 10 Nov 2023 20:34
 Operator : MA/JU
 Sample : PB156738BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK738

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	31	rVB	20051	26799	1.47%	0.141%
2	3.664	95	98	112	rBV	227224	360146	19.71%	1.900%
3	3.969	146	150	155	rVB3	5113	6557	0.36%	0.035%
4	4.164	181	183	185	rBV3	2421	2218	0.12%	0.012%
5	4.199	185	189	191	rBV5	2578	3055	0.17%	0.016%
6	5.375	387	389	392	rBV4	1977	1962	0.11%	0.010%
7	5.405	392	394	397	rVB4	2003	2030	0.11%	0.011%
8	5.652	434	436	440	rVB5	1979	2092	0.11%	0.011%
9	6.393	558	562	564	rBV5	1671	2146	0.12%	0.011%
10	6.458	567	573	575	rVV7	1294	1834	0.10%	0.010%
11	6.622	598	601	605	rBV6	1667	2520	0.14%	0.013%
12	6.816	632	634	641	rVB7	3122	4203	0.23%	0.022%
13	7.016	662	668	683	rBV	262146	483799	26.48%	2.552%
14	7.199	693	699	711	rBV	219677	351021	19.21%	1.852%
15	7.375	722	729	741	rBV	295115	498951	27.31%	2.632%
16	7.852	802	810	822	rBV	254441	413388	22.62%	2.181%
17	8.575	926	933	950	rBV	318027	601492	32.92%	3.173%
18	9.057	1008	1015	1030	rBV	286794	497804	27.24%	2.626%
19	9.281	1051	1053	1059	rVB5	1655	2233	0.12%	0.012%
20	9.581	1100	1104	1106	rBV5	1595	1867	0.10%	0.010%
21	9.769	1129	1136	1147	rBV	248557	447586	24.50%	2.361%
22	10.298	1219	1226	1245	rBV	297291	597693	32.71%	3.153%
23	10.487	1256	1258	1265	rVB7	1769	3414	0.19%	0.018%
24	10.557	1267	1270	1275	rVB7	1794	2481	0.14%	0.013%
25	10.669	1283	1289	1298	rBV	333320	565252	30.94%	2.982%
26	10.851	1313	1320	1339	rBV	282909	602472	32.97%	3.178%
27	11.140	1366	1369	1373	rBV6	1342	1892	0.10%	0.010%
28	11.540	1433	1437	1438	rBV4	1877	2500	0.14%	0.013%
29	11.693	1459	1463	1467	rBV7	1540	3154	0.17%	0.017%
30	12.045	1520	1523	1526	rBV5	1905	2758	0.15%	0.015%
31	12.287	1558	1564	1569	rBV9	4181	8754	0.48%	0.046%
32	12.322	1569	1570	1575	rVB5	2201	2227	0.12%	0.012%
33	12.522	1596	1604	1605	rBV7	2843	4235	0.23%	0.022%
34	12.540	1605	1607	1612	rVB6	1982	3131	0.17%	0.017%
35	12.710	1632	1636	1638	rBV5	2423	3016	0.17%	0.016%
36	12.822	1652	1655	1657	rBV4	1886	2136	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018035.D
 Acq On : 10 Nov 2023 20:34
 Operator : MA/JU
 Sample : PB156738BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK738

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	12.875	1663	1664	1668	rVB4	2119	2002	0.11%	0.011%
38	12.910	1668	1670	1675	rBV6	2970	4669	0.26%	0.025%
39	13.269	1729	1731	1734	rVB4	2007	2094	0.11%	0.011%
40	13.369	1741	1748	1754	rVB4	3288	7135	0.39%	0.038%
41	13.439	1758	1760	1762	rBV3	1845	2064	0.11%	0.011%
42	13.516	1769	1773	1775	rVB4	2060	2160	0.12%	0.011%
43	13.634	1790	1793	1798	rBV7	3271	4589	0.25%	0.024%
44	13.734	1808	1810	1816	rVB7	1933	2425	0.13%	0.013%
45	13.892	1834	1837	1839	rBV3	2145	2011	0.11%	0.011%
46	13.945	1839	1846	1861	rBV	695409	1018828	55.76%	5.375%
47	14.228	1886	1894	1905	rBV	711753	1076870	58.94%	5.681%
48	14.357	1911	1916	1918	rBV6	2416	2514	0.14%	0.013%
49	14.528	1938	1945	1955	rBV	530815	762691	41.74%	4.024%
50	14.792	1984	1990	2007	rBV	128404	371529	20.33%	1.960%
51	15.086	2038	2040	2043	rVB3	2485	2171	0.12%	0.011%
52	15.528	2107	2115	2128	rBV	937917	1354734	74.14%	7.147%
53	15.686	2136	2142	2153	rBV	293035	477047	26.11%	2.517%
54	15.822	2163	2165	2168	rVB4	2226	2153	0.12%	0.011%
55	16.169	2220	2224	2226	rVB5	1670	2069	0.11%	0.011%
56	16.192	2226	2228	2231	rBV4	2250	2334	0.13%	0.012%
57	16.316	2247	2249	2253	rVB4	1570	1835	0.10%	0.010%
58	16.469	2271	2275	2277	rBV4	1815	2574	0.14%	0.014%
59	16.686	2310	2312	2316	rBV5	2032	2909	0.16%	0.015%
60	16.975	2357	2361	2366	rVV8	2655	5366	0.29%	0.028%
61	17.098	2378	2382	2384	rBV5	2340	3329	0.18%	0.018%
62	17.151	2387	2391	2392	rBV4	1640	2312	0.13%	0.012%
63	17.310	2410	2418	2428	rBV	659526	967104	52.93%	5.102%
64	17.410	2428	2435	2449	rVV	1084147	1524860	83.46%	8.045%
65	17.869	2512	2513	2516	rVB3	2610	1917	0.10%	0.010%
66	18.139	2554	2559	2560	rBV4	2395	2844	0.16%	0.015%
67	18.357	2595	2596	2598	rBV2	2220	2260	0.12%	0.012%
68	18.710	2654	2656	2658	rBV3	2316	2458	0.13%	0.013%
69	19.004	2704	2706	2707	rBV2	3018	2816	0.15%	0.015%
70	19.233	2742	2745	2750	rVB3	12090	16248	0.89%	0.086%
71	19.304	2754	2757	2761	rVB3	10554	13378	0.73%	0.071%
72	19.663	2812	2818	2828	rBV	1354232	1806768	98.88%	9.532%
73	21.433	3114	3119	3129	rBV	765306	1048432	57.38%	5.531%
74	23.774	3509	3517	3526	rVB2	904936	1827148	100.00%	9.639%
75	23.939	3538	3545	3557	rVB	531279	1099768	60.19%	5.802%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018035.D
Acq On : 10 Nov 2023 20:34
Operator : MA/JU
Sample : PB156738BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK738

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 18955233

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018035.D
Acq On : 10 Nov 2023 20:34
Operator : MA/JU
Sample : PB156738BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK738

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

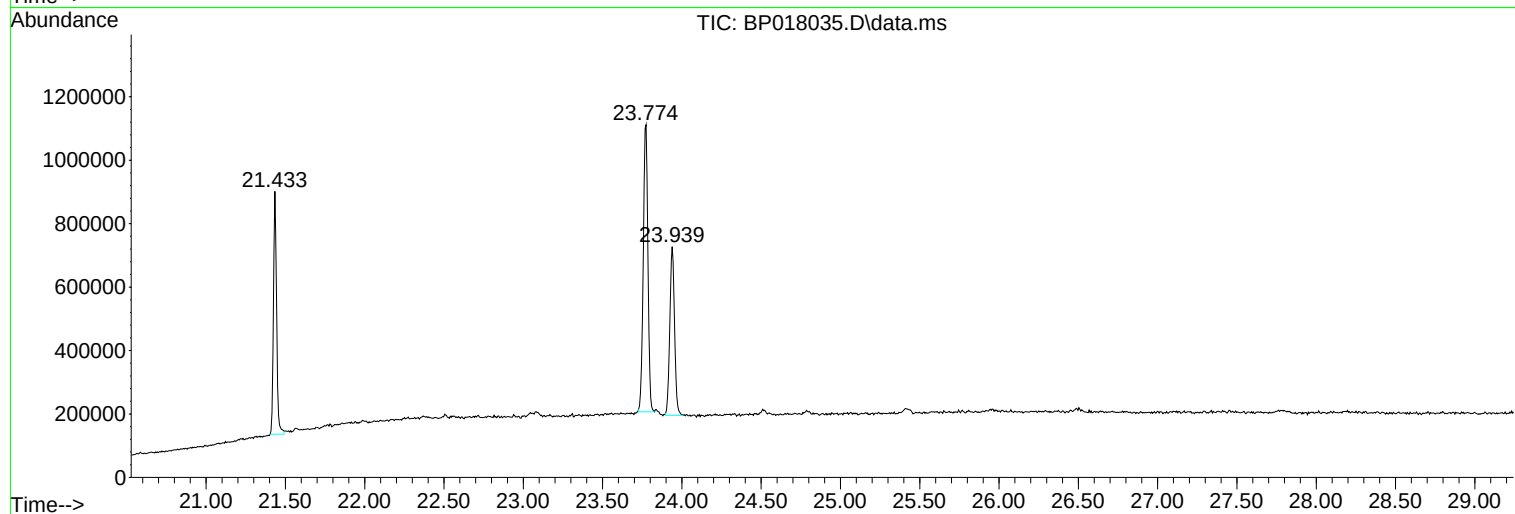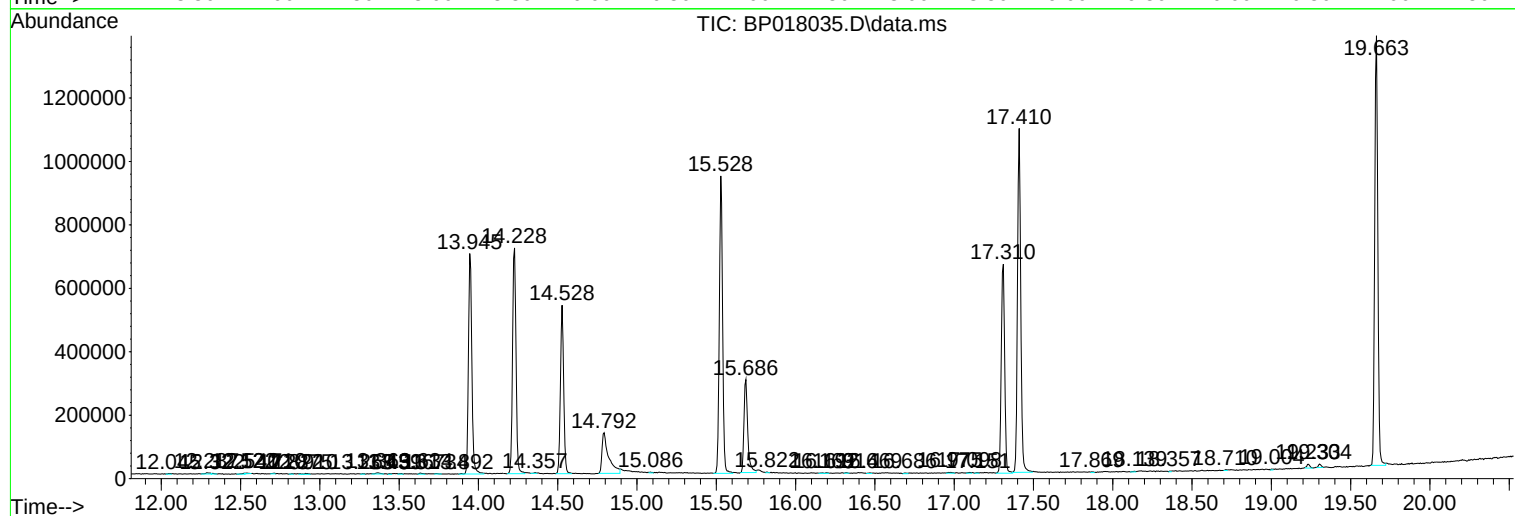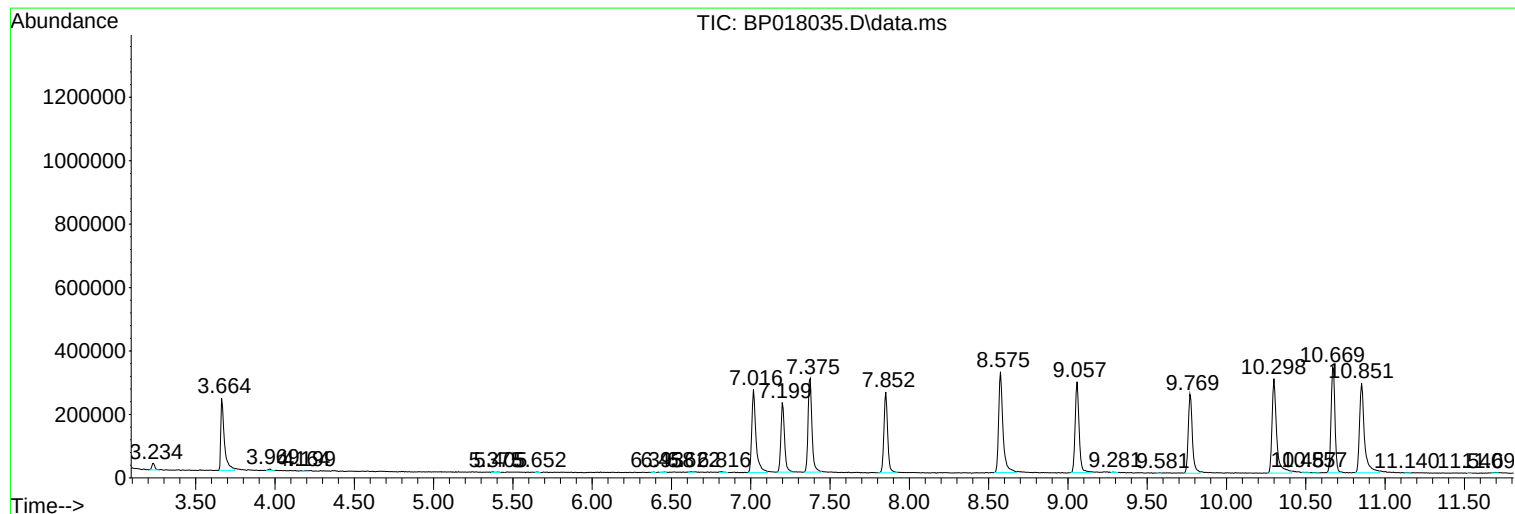

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018035.D
Acq On : 10 Nov 2023 20:34
Operator : MA/JU
Sample : PB156738BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK738

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018035.D
Acq On : 10 Nov 2023 20:34
Operator : MA/JU
Sample : PB156738BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK738

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------