

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018036.D
 Acq On : 10 Nov 2023 21:08
 Operator : MA/JU
 Sample : PB156717BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK717

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	31	rVB2	17266	24862	1.48%	0.159%
2	3.634	91	93	95	rBV3	1677	1916	0.11%	0.012%
3	3.664	95	98	117	rVV	183028	311047	18.54%	1.989%
4	3.964	147	149	154	rVB5	3826	3284	0.20%	0.021%
5	4.299	203	206	207	rBV2	2542	2868	0.17%	0.018%
6	4.452	230	232	235	rBV4	1644	2010	0.12%	0.013%
7	4.616	258	260	263	rVB4	2305	2068	0.12%	0.013%
8	5.634	431	433	437	rVB5	1528	2051	0.12%	0.013%
9	5.899	472	478	479	rBV6	1833	1863	0.11%	0.012%
10	5.958	485	488	489	rBV3	2063	2118	0.13%	0.014%
11	6.628	601	602	607	rVB5	1997	2339	0.14%	0.015%
12	6.810	631	633	637	rVB5	2843	4195	0.25%	0.027%
13	7.016	662	668	680	rBV	217159	410339	24.46%	2.624%
14	7.199	693	699	712	rVB	181052	293522	17.50%	1.877%
15	7.375	722	729	741	rBV	250408	436017	25.99%	2.789%
16	7.481	745	747	750	rVB4	1548	1855	0.11%	0.012%
17	7.634	769	773	774	rBV4	1659	1682	0.10%	0.011%
18	7.852	804	810	821	rVV	158924	265080	15.80%	1.695%
19	8.087	848	850	855	rVB6	1452	2113	0.13%	0.014%
20	8.252	875	878	884	rVV7	1366	2044	0.12%	0.013%
21	8.575	926	933	953	rBV	269994	526079	31.36%	3.365%
22	9.057	1009	1015	1026	rVV	244362	430751	25.67%	2.755%
23	9.446	1077	1081	1083	rVB5	1827	2179	0.13%	0.014%
24	9.769	1128	1136	1147	rBV	209748	388284	23.14%	2.483%
25	10.298	1217	1226	1242	rBV	246973	510793	30.45%	3.267%
26	10.669	1281	1289	1296	rBV	211953	372691	22.21%	2.384%
27	10.851	1312	1320	1339	rBV	237062	507731	30.26%	3.247%
28	11.334	1399	1402	1406	rBV6	1431	1910	0.11%	0.012%
29	11.681	1458	1461	1463	rBV4	2480	2838	0.17%	0.018%
30	11.928	1499	1503	1505	rBV5	1640	1784	0.11%	0.011%
31	11.951	1505	1507	1511	rVB5	1548	1944	0.12%	0.012%
32	12.175	1542	1545	1546	rBV3	2038	2139	0.13%	0.014%
33	12.275	1559	1562	1564	rBV4	1913	2300	0.14%	0.015%
34	12.298	1564	1566	1577	rVB4	3398	8634	0.51%	0.055%
35	12.475	1593	1596	1599	rBV5	1230	2181	0.13%	0.014%
36	12.534	1599	1606	1609	rBV5	3033	5389	0.32%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018036.D
 Acq On : 10 Nov 2023 21:08
 Operator : MA/JU
 Sample : PB156717BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK717

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	12.710	1633	1636	1639	rVV5	2153	3037	0.18%	0.019%
38	12.992	1681	1684	1686	rBV4	1725	1720	0.10%	0.011%
39	13.045	1692	1693	1697	rVB4	1470	1691	0.10%	0.011%
40	13.369	1743	1748	1753	rBV9	4258	7086	0.42%	0.045%
41	13.492	1762	1769	1770	rBV6	1850	2510	0.15%	0.016%
42	13.634	1790	1793	1794	rVV3	2256	2675	0.16%	0.017%
43	13.657	1796	1797	1802	rVV5	1563	2001	0.12%	0.013%
44	13.739	1808	1811	1817	rBV8	2249	3047	0.18%	0.019%
45	13.945	1840	1846	1860	rBV	604102	875208	52.17%	5.598%
46	14.034	1860	1861	1866	rVB5	1979	2124	0.13%	0.014%
47	14.163	1879	1883	1886	rBV6	1661	2241	0.13%	0.014%
48	14.228	1886	1894	1908	rBV	616564	933132	55.62%	5.968%
49	14.363	1915	1917	1927	rVB	1884	3738	0.22%	0.024%
50	14.428	1927	1928	1932	rVB4	1653	1745	0.10%	0.011%
51	14.528	1937	1945	1955	rBV	346934	504882	30.09%	3.229%
52	14.604	1955	1958	1962	rBV5	1707	2554	0.15%	0.016%
53	14.792	1983	1990	2012	rBV2	108534	349735	20.85%	2.237%
54	15.245	2063	2067	2070	rVB6	1947	2973	0.18%	0.019%
55	15.528	2108	2115	2125	rBV	824733	1177434	70.18%	7.531%
56	15.686	2135	2142	2152	rBV	248603	416833	24.84%	2.666%
57	15.769	2154	2156	2160	rVB5	7045	7979	0.48%	0.051%
58	16.022	2197	2199	2204	rVV6	1536	1950	0.12%	0.012%
59	16.110	2212	2214	2217	rVV4	2001	2285	0.14%	0.015%
60	16.181	2224	2226	2230	rBV5	1904	1719	0.10%	0.011%
61	16.322	2248	2250	2254	rVB5	2749	2121	0.13%	0.014%
62	16.410	2263	2265	2271	rVB6	2498	3173	0.19%	0.020%
63	16.563	2288	2291	2295	rBV6	2345	3229	0.19%	0.021%
64	16.645	2303	2305	2310	rVB6	1574	1847	0.11%	0.012%
65	16.763	2323	2325	2330	rBV6	1736	2464	0.15%	0.016%
66	16.951	2353	2357	2359	rBV5	1852	2516	0.15%	0.016%
67	17.310	2411	2418	2425	rBV	439040	633287	37.75%	4.050%
68	17.410	2428	2435	2453	rVV	918886	1342220	80.00%	8.585%
69	17.751	2492	2493	2498	rVB5	1871	2677	0.16%	0.017%
70	17.804	2498	2502	2504	rBV5	2344	2918	0.17%	0.019%
71	18.316	2587	2589	2593	rBV5	1643	2021	0.12%	0.013%
72	18.692	2651	2653	2654	rBV2	2239	1745	0.10%	0.011%
73	18.716	2654	2657	2660	rVV5	2536	3460	0.21%	0.022%
74	19.063	2714	2716	2719	rVB4	2799	2445	0.15%	0.016%
75	19.233	2741	2745	2750	rBV5	12444	18320	1.09%	0.117%
76	19.304	2754	2757	2760	rVV2	8913	10557	0.63%	0.068%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018036.D
Acq On : 10 Nov 2023 21:08
Operator : MA/JU
Sample : PB156717BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK717

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

77	19.663	2812	2818	2826	rBV	1249534	1603227	95.56%	10.254%
78	21.433	3114	3119	3128	rBV	499088	713646	42.54%	4.564%
79	23.768	3510	3516	3526	rVB2	826651	1677735	100.00%	10.730%
80	23.939	3539	3545	3554	rVB	357539	754514	44.97%	4.826%



Sum of corrected areas: 15635321

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018036.D
Acq On : 10 Nov 2023 21:08
Operator : MA/JU
Sample : PB156717BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK717

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

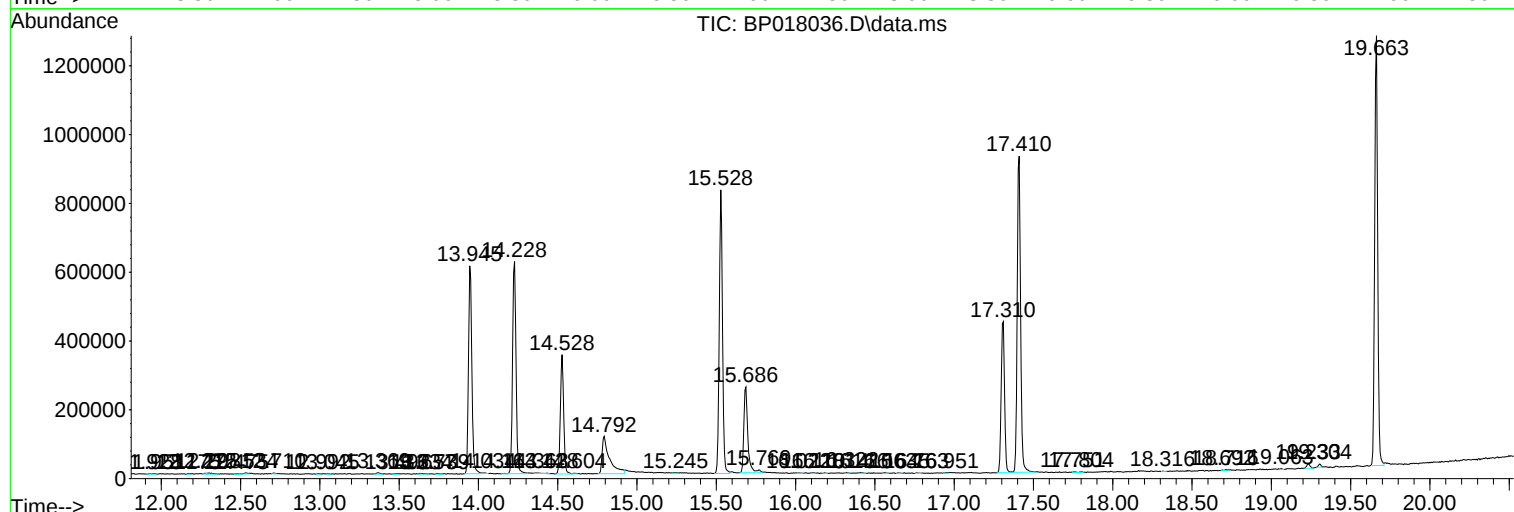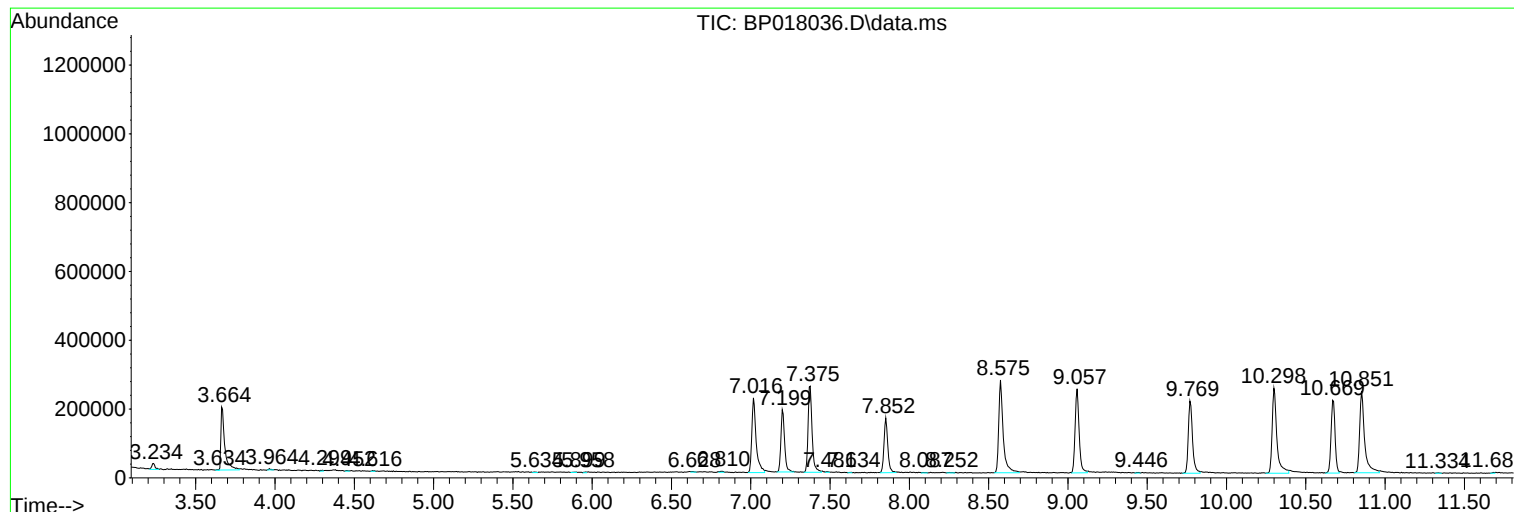

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018036.D
Acq On : 10 Nov 2023 21:08
Operator : MA/JU
Sample : PB156717BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK717

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018036.D
Acq On : 10 Nov 2023 21:08
Operator : MA/JU
Sample : PB156717BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK717

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------