

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018058.D
 Acq On : 11 Nov 2023 10:43
 Operator : MA/JU
 Sample : PB156765BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK765

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	33	rVB	29095	37414	2.14%	0.194%
2	3.528	73	75	77	rBV3	2581	2126	0.12%	0.011%
3	3.664	95	98	117	rBV	289152	451206	25.81%	2.335%
4	3.964	146	149	155	rBV5	6168	9000	0.51%	0.047%
5	4.793	287	290	293	rBV5	2424	2831	0.16%	0.015%
6	5.028	327	330	333	rBV5	2113	2649	0.15%	0.014%
7	5.187	353	357	358	rBV4	2599	2715	0.16%	0.014%
8	5.387	388	391	396	rBV7	1652	2864	0.16%	0.015%
9	5.593	423	426	431	rVV7	2432	4733	0.27%	0.024%
10	5.646	433	435	441	rVB7	1917	2959	0.17%	0.015%
11	5.875	471	474	475	rBV3	1870	2222	0.13%	0.011%
12	6.358	552	556	557	rBV4	1918	2432	0.14%	0.013%
13	6.564	588	591	594	rBV4	2213	3064	0.18%	0.016%
14	6.946	654	656	658	rBV3	2381	2603	0.15%	0.013%
15	7.016	662	668	683	rVV	325408	597318	34.16%	3.091%
16	7.199	693	699	708	rVV	280549	436884	24.99%	2.261%
17	7.299	713	716	717	rVB3	2965	2501	0.14%	0.013%
18	7.369	721	728	746	rBV	386758	635112	36.32%	3.287%
19	7.516	751	753	755	rBV3	2565	2181	0.12%	0.011%
20	7.746	790	792	794	rBV2	2778	1975	0.11%	0.010%
21	7.846	803	809	828	rBV	256365	440517	25.19%	2.280%
22	8.122	854	856	859	rBV4	1747	2500	0.14%	0.013%
23	8.569	926	932	947	rBV	393860	742396	42.46%	3.842%
24	9.052	1005	1014	1031	rBV	340656	615460	35.20%	3.185%
25	9.199	1035	1039	1040	rVV4	2952	4165	0.24%	0.022%
26	9.216	1040	1042	1046	rVB5	2015	2855	0.16%	0.015%
27	9.446	1077	1081	1082	rVB4	2450	2157	0.12%	0.011%
28	9.522	1089	1094	1095	rBV5	1812	2353	0.13%	0.012%
29	9.622	1107	1111	1114	rBV6	1784	2247	0.13%	0.012%
30	9.769	1127	1136	1148	rBV	302088	553052	31.63%	2.862%
31	9.887	1154	1156	1159	rVB3	1828	1818	0.10%	0.009%
32	10.157	1201	1202	1207	rVB5	1435	2198	0.13%	0.011%
33	10.293	1217	1225	1243	rBV	358933	749314	42.86%	3.878%
34	10.510	1260	1262	1265	rVB4	2641	2089	0.12%	0.011%
35	10.569	1271	1272	1276	rBV4	3043	2771	0.16%	0.014%
36	10.669	1281	1289	1297	rBV	359331	591950	33.86%	3.063%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018058.D
 Acq On : 11 Nov 2023 10:43
 Operator : MA/JU
 Sample : PB156765BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK765

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	10.852	1308	1320	1338	rBV	325223	715461	40.92%	3.703%
38	11.093	1359	1361	1365	rVB5	2027	2157	0.12%	0.011%
39	11.157	1369	1372	1375	rVB5	1995	2682	0.15%	0.014%
40	11.210	1378	1381	1383	rBV4	1879	2464	0.14%	0.013%
41	11.269	1389	1391	1394	rVB4	2026	2109	0.12%	0.011%
42	11.569	1439	1442	1444	rBV4	2231	2725	0.16%	0.014%
43	11.675	1456	1460	1461	rBV3	2629	3043	0.17%	0.016%
44	11.693	1461	1463	1468	rBV6	2328	3415	0.20%	0.018%
45	12.128	1534	1537	1541	rVV5	1228	1969	0.11%	0.010%
46	12.169	1541	1544	1545	rVB3	2031	1824	0.10%	0.009%
47	12.234	1553	1555	1557	rBV3	2063	2098	0.12%	0.011%
48	12.293	1557	1565	1570	rVV9	6175	12163	0.70%	0.063%
49	12.540	1603	1607	1608	rBV4	1925	3134	0.18%	0.016%
50	12.587	1614	1615	1620	rVB5	2537	2987	0.17%	0.015%
51	12.628	1620	1622	1624	rBV3	1641	1885	0.11%	0.010%
52	12.716	1633	1637	1642	rVV8	2928	6993	0.40%	0.036%
53	12.975	1679	1681	1685	rBV5	1506	1800	0.10%	0.009%
54	13.122	1704	1706	1709	rBV3	1825	2450	0.14%	0.013%
55	13.169	1712	1714	1717	rVB4	1915	2238	0.13%	0.012%
56	13.234	1721	1725	1727	rVB5	1885	2834	0.16%	0.015%
57	13.263	1727	1730	1731	rBV3	2829	2269	0.13%	0.012%
58	13.363	1742	1747	1754	rBV10	7465	14748	0.84%	0.076%
59	13.451	1759	1762	1766	rBV6	1947	3241	0.19%	0.017%
60	13.487	1766	1768	1773	rVV6	2636	4189	0.24%	0.022%
61	13.528	1773	1775	1778	rVB4	1910	1832	0.10%	0.009%
62	13.722	1806	1808	1816	rVB9	2013	3713	0.21%	0.019%
63	13.945	1840	1846	1855	rBV	723771	1037920	59.36%	5.371%
64	14.163	1880	1883	1885	rBV4	1516	1891	0.11%	0.010%
65	14.222	1885	1893	1905	rBV	830674	1222480	69.92%	6.326%
66	14.522	1938	1944	1955	rBV	489782	718178	41.07%	3.717%
67	14.728	1972	1979	1980	rVB6	1762	2325	0.13%	0.012%
68	14.793	1984	1990	2005	rBV2	109317	344522	19.70%	1.783%
69	15.151	2050	2051	2058	rVB7	3370	4317	0.25%	0.022%
70	15.298	2072	2076	2077	rBV4	3039	4184	0.24%	0.022%
71	15.528	2108	2115	2123	rBV	980895	1438910	82.30%	7.447%
72	15.681	2136	2141	2152	rBV	273314	436285	24.95%	2.258%
73	15.769	2154	2156	2167	rVB	11433	19352	1.11%	0.100%
74	16.104	2210	2213	2217	rBV6	2321	3645	0.21%	0.019%
75	16.498	2278	2280	2284	rBV5	2164	3267	0.19%	0.017%
76	16.563	2286	2291	2293	rBV5	2730	3984	0.23%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018058.D
 Acq On : 11 Nov 2023 10:43
 Operator : MA/JU
 Sample : PB156765BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK765

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

77	16.698	2312	2314	2317	rVB4	2716	3271	0.19%	0.017%
78	16.728	2317	2319	2321	rBV3	2650	2888	0.17%	0.015%
79	16.810	2331	2333	2336	rBV4	2208	2029	0.12%	0.011%
80	16.963	2356	2359	2361	rVB4	1765	1779	0.10%	0.009%
81	17.028	2369	2370	2373	rVB3	1807	1818	0.10%	0.009%
82	17.087	2377	2380	2383	rVV4	2346	3701	0.21%	0.019%
83	17.304	2409	2417	2425	rBV	556304	788577	45.10%	4.081%
84	17.404	2428	2434	2450	rVV	1031740	1476953	84.47%	7.643%
85	17.634	2472	2473	2477	rBV4	2957	2864	0.16%	0.015%
86	17.663	2477	2478	2481	rVB3	2323	1823	0.10%	0.009%
87	17.728	2488	2489	2493	rBV4	1574	1822	0.10%	0.009%
88	17.916	2516	2521	2523	rVB6	1847	2492	0.14%	0.013%
89	18.139	2558	2559	2562	rBV3	2302	2510	0.14%	0.013%
90	18.281	2581	2583	2586	rBV3	3045	2538	0.15%	0.013%
91	18.316	2587	2589	2593	rVV4	2529	2482	0.14%	0.013%
92	18.469	2613	2615	2616	rBV2	2408	1774	0.10%	0.009%
93	18.586	2633	2635	2637	rBV3	2127	2349	0.13%	0.012%
94	19.139	2727	2729	2730	rBV2	3116	1963	0.11%	0.010%
95	19.228	2740	2744	2749	rBV6	13930	21904	1.25%	0.113%
96	19.304	2754	2757	2760	rVB3	8350	11679	0.67%	0.060%
97	19.657	2811	2817	2825	rBV	1226413	1607724	91.95%	8.320%
98	21.433	3114	3119	3129	rBV	543254	783659	44.82%	4.056%
99	23.769	3509	3516	3526	rVB2	895508	1748478	100.00%	9.049%
100	23.933	3538	3544	3556	rVB	406499	875875	50.09%	4.533%




Sum of corrected areas: 19323266

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018058.D
Acq On : 11 Nov 2023 10:43
Operator : MA/JU
Sample : PB156765BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK765

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

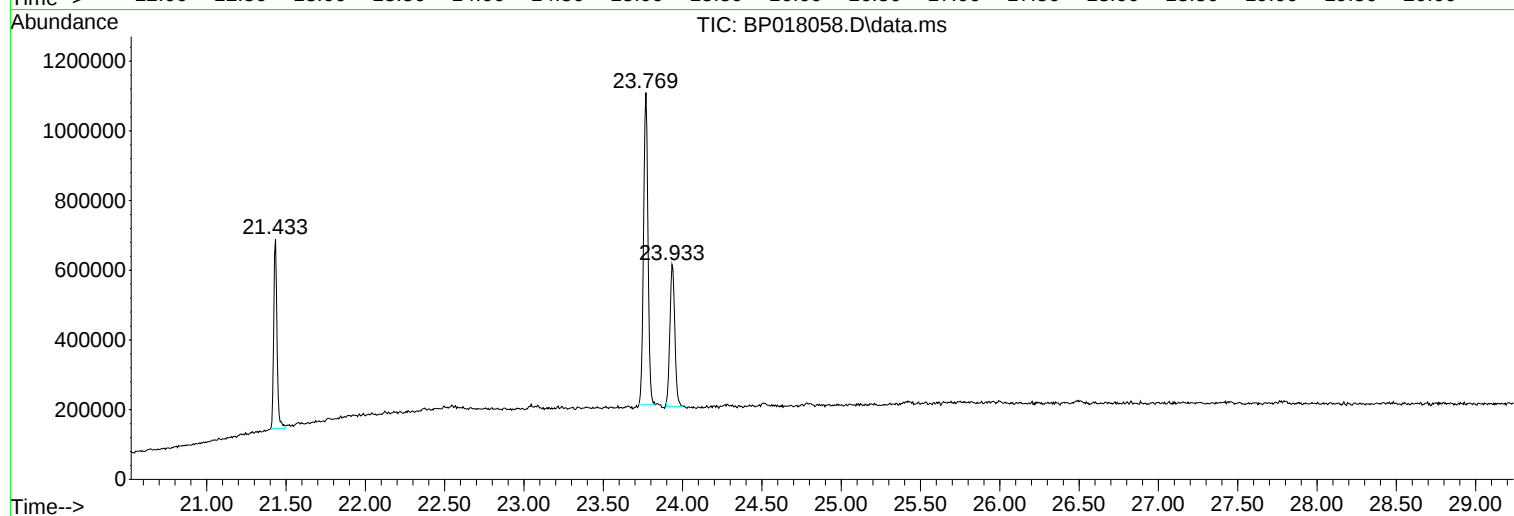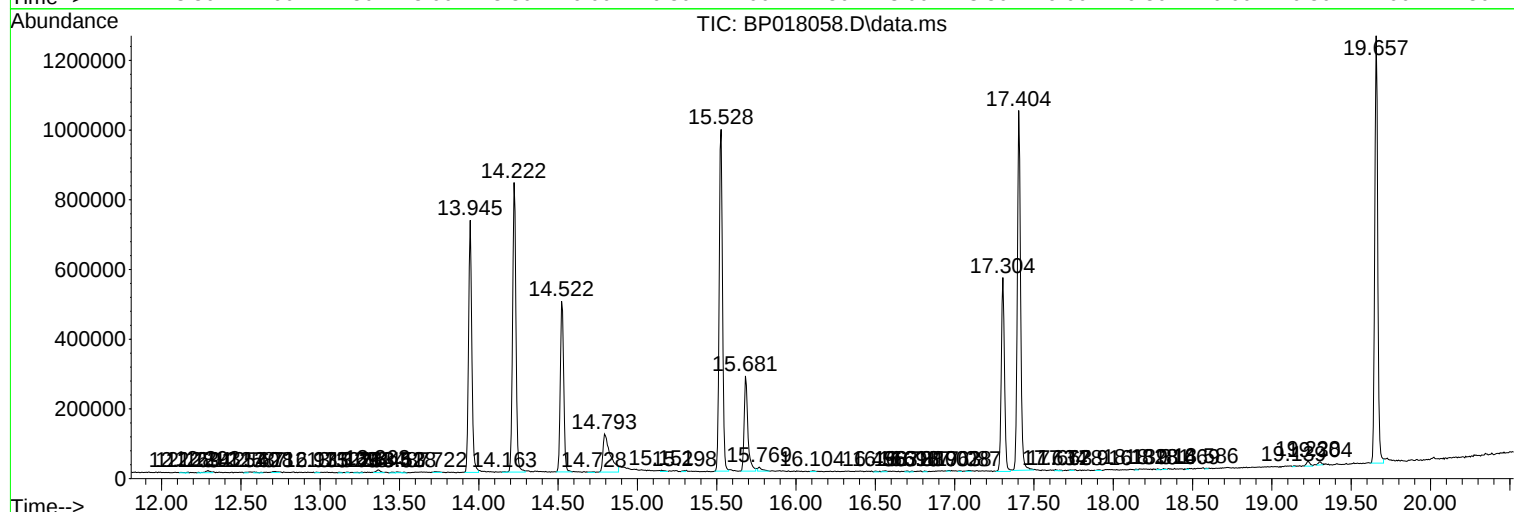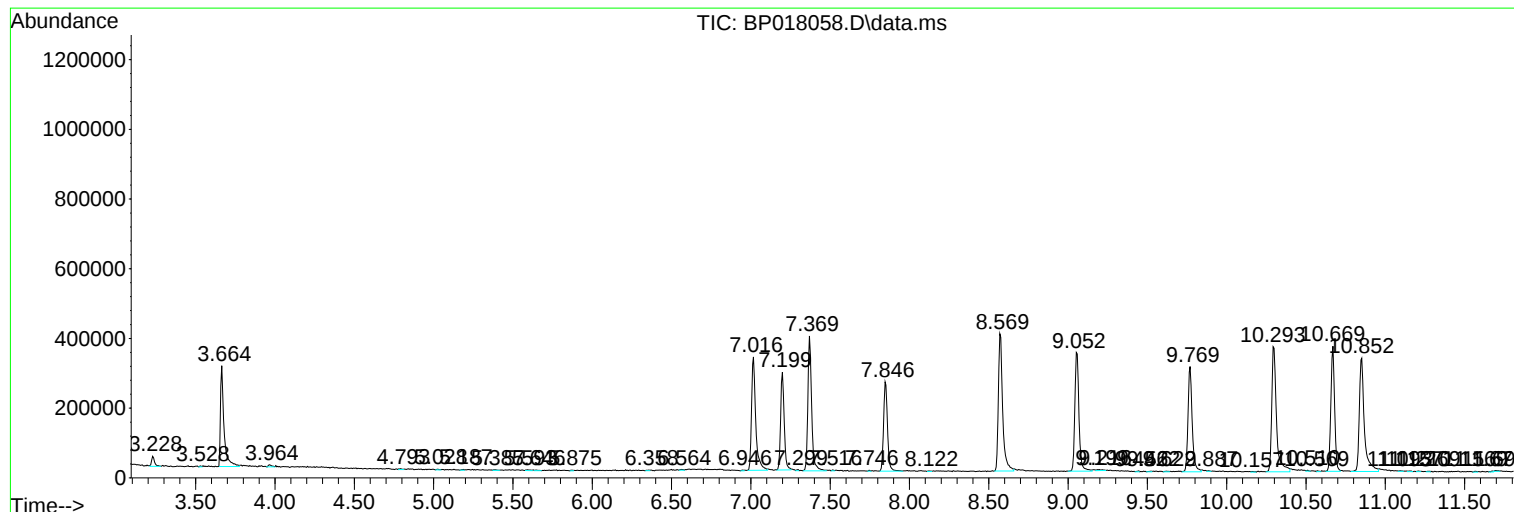

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018058.D
Acq On : 11 Nov 2023 10:43
Operator : MA/JU
Sample : PB156765BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK765

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018058.D
Acq On : 11 Nov 2023 10:43
Operator : MA/JU
Sample : PB156765BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK765

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------