

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018059.D
 Acq On : 11 Nov 2023 11:16
 Operator : MA/JU
 Sample : PB156721BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	29	rVB	22347	24226	1.60%	0.126%
2	3.664	95	98	119	rBV	254769	404531	26.78%	2.099%
3	3.958	146	148	153	rVB4	4636	6555	0.43%	0.034%
4	4.258	197	199	201	rBV3	2581	2130	0.14%	0.011%
5	4.358	214	216	220	rVB5	3560	3644	0.24%	0.019%
6	5.081	337	339	340	rBV2	2467	1710	0.11%	0.009%
7	5.146	347	350	352	rVB4	2374	2779	0.18%	0.014%
8	5.169	352	354	357	rBV3	1736	2851	0.19%	0.015%
9	5.258	366	369	371	rVV4	1744	2142	0.14%	0.011%
10	5.281	371	373	374	rVV2	2771	2037	0.13%	0.011%
11	5.322	378	380	382	rVB3	1921	1861	0.12%	0.010%
12	5.458	399	403	404	rBV4	2705	2991	0.20%	0.016%
13	5.534	412	416	419	rBV6	1764	2354	0.16%	0.012%
14	6.299	542	546	547	rVB3	1646	1907	0.13%	0.010%
15	6.387	559	561	564	rVB4	1877	2127	0.14%	0.011%
16	6.446	570	571	576	rBV5	1688	1923	0.13%	0.010%
17	6.616	597	600	601	rBV3	1874	2034	0.13%	0.011%
18	6.805	627	632	633	rBV5	1926	3393	0.22%	0.018%
19	6.963	658	659	661	rBV2	2047	1945	0.13%	0.010%
20	7.016	661	668	684	rVV	299514	553408	36.64%	2.871%
21	7.199	692	699	715	rVB	254233	408706	27.06%	2.121%
22	7.369	722	728	746	rVV	349483	571972	37.87%	2.968%
23	7.552	755	759	763	rVB5	1937	3425	0.23%	0.018%
24	7.787	796	799	802	rBV5	1644	2015	0.13%	0.010%
25	7.846	802	809	821	rBV	312174	509121	33.71%	2.642%
26	8.028	839	840	844	rVB4	2404	2487	0.16%	0.013%
27	8.099	849	852	855	rVB5	1948	2189	0.14%	0.011%
28	8.187	865	867	871	rBV5	1386	1696	0.11%	0.009%
29	8.510	918	922	923	rBV4	1853	2217	0.15%	0.012%
30	8.569	926	932	952	rVV	368031	705081	46.68%	3.658%
31	9.052	1008	1014	1030	rBV	314510	564658	37.39%	2.930%
32	9.193	1033	1038	1039	rBV5	1799	2808	0.19%	0.015%
33	9.428	1077	1078	1081	rVB3	2344	1950	0.13%	0.010%
34	9.769	1128	1136	1151	rBV	285758	520420	34.46%	2.700%
35	10.299	1217	1226	1245	rBV	343556	715759	47.39%	3.714%
36	10.593	1274	1276	1279	rVB3	2146	2529	0.17%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018059.D
 Acq On : 11 Nov 2023 11:16
 Operator : MA/JU
 Sample : PB156721BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	10.669	1281	1289	1299	rBV	428366	702047	46.48%	3.643%
38	10.851	1309	1320	1340	rBV	316472	690591	45.73%	3.583%
39	11.375	1404	1409	1412	rBV7	1372	2891	0.19%	0.015%
40	11.675	1458	1460	1461	rBV	3548	2579	0.17%	0.013%
41	11.693	1461	1463	1466	rVV4	4179	5488	0.36%	0.028%
42	11.716	1466	1467	1471	rVB4	2744	2735	0.18%	0.014%
43	11.810	1481	1483	1487	rVB5	2158	2914	0.19%	0.015%
44	11.857	1487	1491	1492	rBV4	1518	1861	0.12%	0.010%
45	12.169	1540	1544	1545	rBV4	2313	2058	0.14%	0.011%
46	12.245	1554	1557	1558	rVV3	1813	1789	0.12%	0.009%
47	12.281	1560	1563	1574	rVB8	4920	12895	0.85%	0.067%
48	12.393	1581	1582	1585	rVB3	2205	1910	0.13%	0.010%
49	12.422	1585	1587	1590	rBV3	1968	2973	0.20%	0.015%
50	12.557	1606	1610	1614	rVB7	1992	3711	0.25%	0.019%
51	12.716	1631	1637	1639	rBV7	2617	5105	0.34%	0.026%
52	12.769	1644	1646	1650	rBV5	1330	1878	0.12%	0.010%
53	12.822	1653	1655	1658	rBV4	1596	2058	0.14%	0.011%
54	12.940	1672	1675	1680	rVV7	1674	2486	0.16%	0.013%
55	12.987	1680	1683	1691	rVB10	1235	2631	0.17%	0.014%
56	13.063	1694	1696	1701	rBV6	1975	3171	0.21%	0.016%
57	13.251	1725	1728	1731	rBV5	1552	1661	0.11%	0.009%
58	13.369	1743	1748	1753	rBV7	7679	13807	0.91%	0.072%
59	13.569	1778	1782	1783	rBV4	1355	1656	0.11%	0.009%
60	13.622	1789	1791	1795	rBV5	3777	5206	0.34%	0.027%
61	13.669	1798	1799	1803	rVV4	1616	2031	0.13%	0.011%
62	13.734	1803	1810	1815	rVV10	3609	8892	0.59%	0.046%
63	13.945	1840	1846	1865	rVB	725943	1043823	69.11%	5.416%
64	14.140	1876	1879	1881	rBV4	1606	2084	0.14%	0.011%
65	14.222	1887	1893	1907	rBV	796859	1174041	77.74%	6.092%
66	14.369	1917	1918	1922	rVB4	3007	2708	0.18%	0.014%
67	14.522	1937	1944	1957	rVV	617241	902563	59.76%	4.683%
68	14.669	1966	1969	1970	rVB3	1959	1836	0.12%	0.010%
69	14.681	1970	1971	1976	rBV5	1738	1975	0.13%	0.010%
70	14.792	1985	1990	2011	rBV2	104091	345764	22.89%	1.794%
71	15.151	2046	2051	2052	rBV5	2829	3734	0.25%	0.019%
72	15.304	2073	2077	2081	rVB7	3693	5221	0.35%	0.027%
73	15.528	2108	2115	2123	rBV	961015	1401914	92.82%	7.274%
74	15.681	2136	2141	2152	rBV	239774	382021	25.29%	1.982%
75	15.769	2153	2156	2161	rVB6	7642	11521	0.76%	0.060%
76	16.104	2211	2213	2216	rBV4	2168	2203	0.15%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018059.D
 Acq On : 11 Nov 2023 11:16
 Operator : MA/JU
 Sample : PB156721BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

77	16.169	2221	2224	2228	rBV6	2260	3517	0.23%	0.018%
78	16.222	2228	2233	2234	rBV5	1148	1663	0.11%	0.009%
79	16.410	2261	2265	2266	rBV4	2464	2789	0.18%	0.014%
80	16.563	2287	2291	2298	rBV10	2380	4424	0.29%	0.023%
81	16.669	2308	2309	2314	rBV5	1701	2351	0.16%	0.012%
82	16.910	2348	2350	2353	rVB4	2242	2510	0.17%	0.013%
83	16.957	2353	2358	2359	rBV5	3087	4195	0.28%	0.022%
84	17.057	2372	2375	2377	rBV4	2578	2563	0.17%	0.013%
85	17.092	2377	2381	2384	rVB5	3800	5820	0.39%	0.030%
86	17.139	2388	2389	2393	rBV4	2204	2495	0.17%	0.013%
87	17.304	2411	2417	2427	rBV	742363	1000729	66.26%	5.193%
88	17.404	2427	2434	2452	rVV2	968745	1425997	94.42%	7.399%
89	17.704	2482	2485	2488	rVB5	1975	2432	0.16%	0.013%
90	17.739	2488	2491	2493	rBV4	1782	2364	0.16%	0.012%
91	17.833	2503	2507	2508	rBV4	2506	2899	0.19%	0.015%
92	18.157	2561	2562	2566	rVB4	3627	3361	0.22%	0.017%
93	18.469	2611	2615	2619	rBV7	4193	5856	0.39%	0.030%
94	18.551	2628	2629	2630	rBV	4046	2554	0.17%	0.013%
95	19.227	2740	2744	2750	rBV7	11018	18812	1.25%	0.098%
96	19.304	2755	2757	2761	rVB	9492	8715	0.58%	0.045%
97	19.657	2811	2817	2824	rBV	1151708	1510302	100.00%	7.837%
98	21.433	3114	3119	3130	rBV	647206	929070	61.52%	4.821%
99	23.768	3509	3516	3523	rVB2	745953	1494801	98.97%	7.756%
100	23.933	3538	3544	3555	rVB	488812	1020280	67.55%	5.294%




Sum of corrected areas: 19272512

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018059.D
Acq On : 11 Nov 2023 11:16
Operator : MA/JU
Sample : PB156721BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

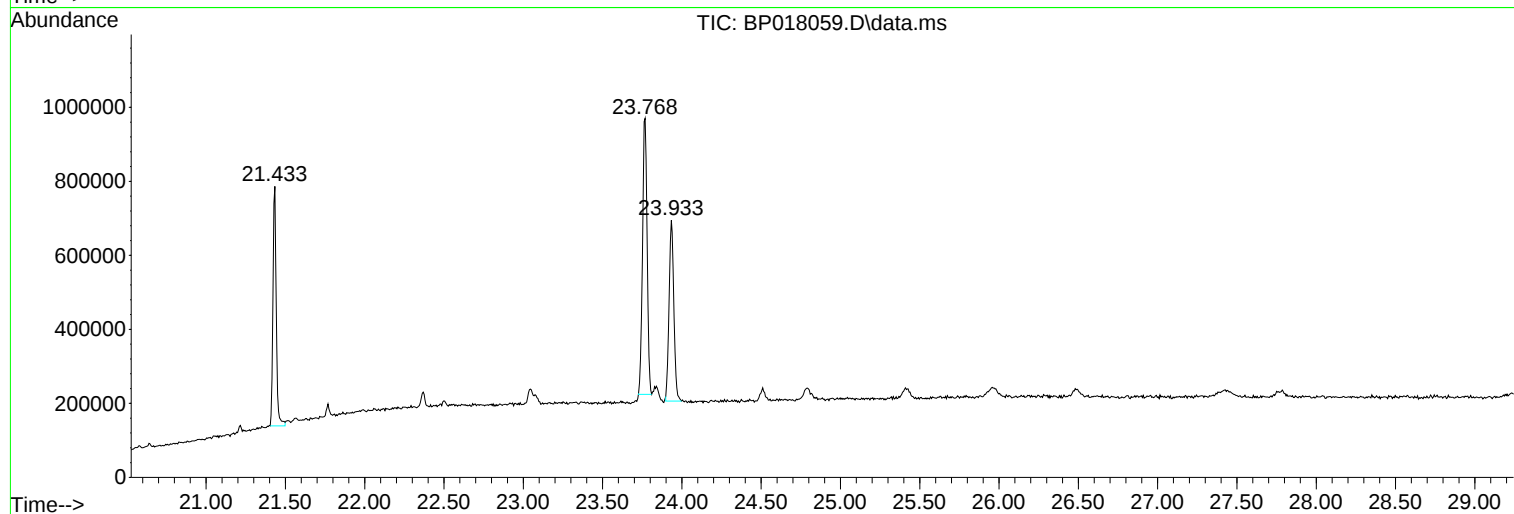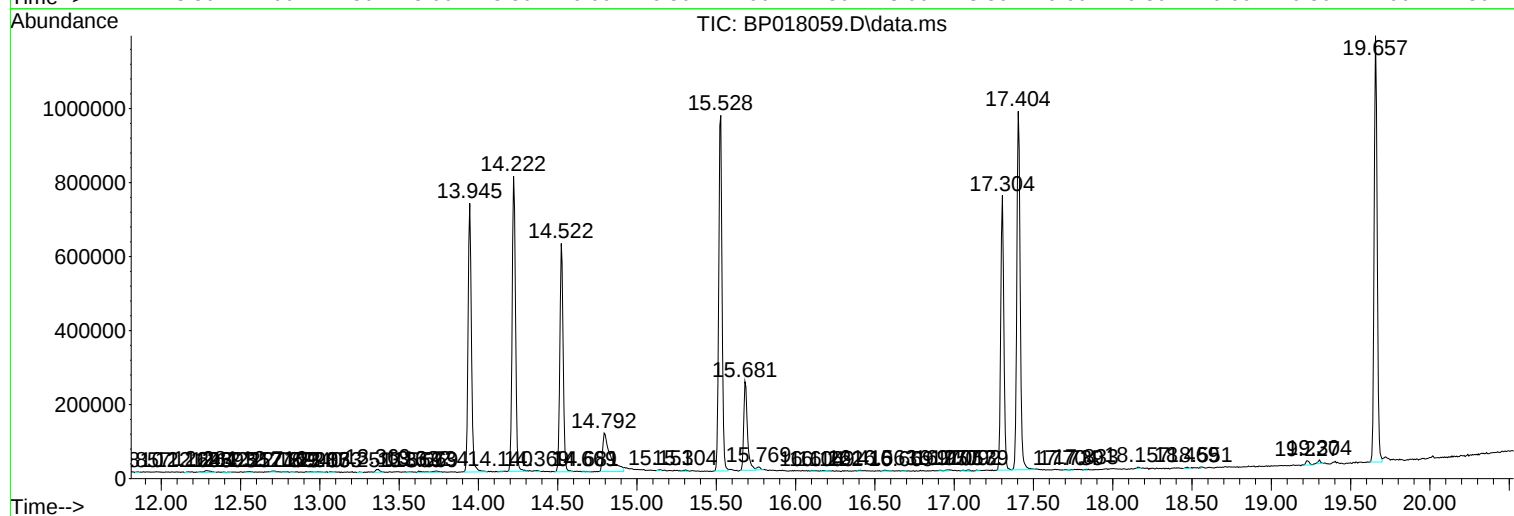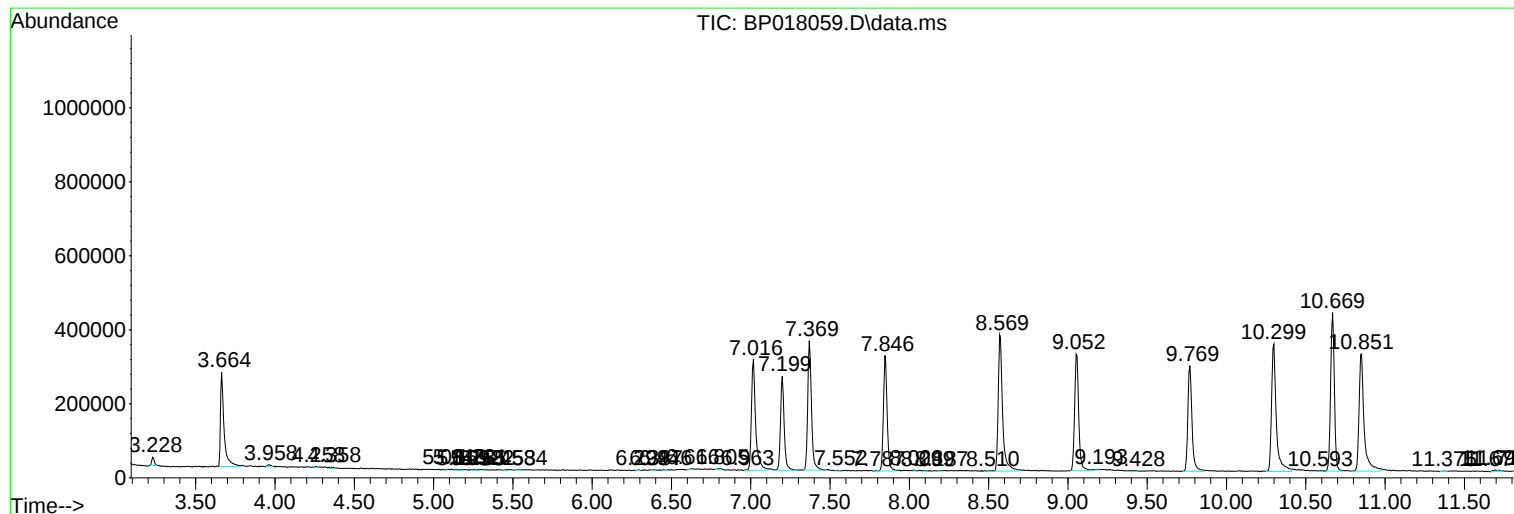

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018059.D
Acq On : 11 Nov 2023 11:16
Operator : MA/JU
Sample : PB156721BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018059.D
Acq On : 11 Nov 2023 11:16
Operator : MA/JU
Sample : PB156721BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------