

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018063.D
 Acq On : 11 Nov 2023 13:32
 Operator : MA/JU
 Sample : 05079-05
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.717	103	107	112	rVB	253789	349913	7.61%	0.449%
2	3.981	144	152	161	rBV2	237386	487089	10.59%	0.624%
3	4.305	201	207	212	rVV	672995	954628	20.76%	1.224%
4	5.017	320	328	335	rVB4	301184	724238	15.75%	0.928%
5	5.146	344	350	356	rBV	2765223	3930597	85.47%	5.039%
6	5.434	389	399	411	rVB	519270	1073486	23.34%	1.376%
7	5.622	426	431	435	rBV	312019	430764	9.37%	0.552%
8	5.722	442	448	455	rBV2	318797	519789	11.30%	0.666%
9	6.005	489	496	511	rVB3	203799	439447	9.56%	0.563%
10	6.128	511	517	525	rVB	218058	331721	7.21%	0.425%
11	6.505	569	581	586	rBV2	219922	399921	8.70%	0.513%
12	6.558	586	590	594	rVV2	177792	292703	6.36%	0.375%
13	6.605	594	598	609	rVV3	124666	382985	8.33%	0.491%
14	6.705	609	615	617	rVV5	127687	253932	5.52%	0.326%
15	6.740	617	621	628	rVV	322884	557942	12.13%	0.715%
16	6.916	643	651	655	rVV2	320756	555108	12.07%	0.712%
17	6.987	659	663	668	rVV	942465	1497862	32.57%	1.920%
18	7.028	668	670	680	rVV4	155150	390451	8.49%	0.501%
19	7.134	684	688	693	rVV4	109157	205210	4.46%	0.263%
20	7.193	693	698	705	rVB2	1217987	1831621	39.83%	2.348%
21	7.299	710	716	723	rVB3	116536	267035	5.81%	0.342%
22	7.375	723	729	734	rBV	407250	664751	14.45%	0.852%
23	7.440	734	740	745	rVV3	148083	360569	7.84%	0.462%
24	7.675	760	780	784	rBV	110911	430842	9.37%	0.552%
25	7.722	784	788	798	rVB3	175604	329782	7.17%	0.423%
26	7.846	798	809	815	rBV2	324344	549784	11.95%	0.705%
27	7.928	818	823	829	rBV	437004	724017	15.74%	0.928%
28	8.105	844	853	857	rBV6	116074	236125	5.13%	0.303%
29	8.152	857	861	864	rBV	173760	255066	5.55%	0.327%
30	8.199	864	869	876	rVB	2053924	3079421	66.96%	3.948%
31	8.299	876	886	896	rBV6	108855	344006	7.48%	0.441%
32	8.505	915	921	926	rBV5	170157	428830	9.32%	0.550%
33	8.581	930	934	937	rBV2	271808	363198	7.90%	0.466%
34	8.763	960	965	969	rBV	155140	246243	5.35%	0.316%
35	8.816	969	974	980	rVV	241750	404274	8.79%	0.518%
36	8.922	986	992	998	rVV2	829175	1468413	31.93%	1.883%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018063.D
 Acq On : 11 Nov 2023 13:32
 Operator : MA/JU
 Sample : 05079-05
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	9.005	1000	1006	1011	rVV	1394520	2250111	48.93%	2.885%
38	9.057	1011	1015	1021	rVV	398190	674342	14.66%	0.865%
39	9.163	1030	1033	1039	rVV4	131166	229380	4.99%	0.294%
40	9.293	1039	1055	1066	rVB	1187430	2176760	47.33%	2.791%

41	9.446	1076	1081	1089	rVB	575621	855738	18.61%	1.097%
42	9.622	1106	1111	1117	rVB3	107309	206905	4.50%	0.265%
43	9.769	1128	1136	1140	rBV3	372689	680086	14.79%	0.872%
44	9.816	1140	1144	1147	rBV2	218339	335465	7.29%	0.430%
45	9.881	1152	1155	1164	rVB2	393788	726865	15.81%	0.932%

46	10.028	1167	1180	1186	rBV	2853068	4598808	100.00%	5.896%
47	10.087	1186	1190	1196	rVB4	127851	220542	4.80%	0.283%
48	10.199	1196	1209	1215	rBV6	166297	483853	10.52%	0.620%
49	10.299	1218	1226	1235	rBV3	506448	1084110	23.57%	1.390%
50	10.481	1252	1257	1265	rBV5	73674	189124	4.11%	0.242%

51	10.610	1270	1279	1283	rVV	572123	1226050	26.66%	1.572%
52	10.669	1283	1289	1295	rVV3	651909	1379971	30.01%	1.769%
53	10.740	1295	1301	1307	rVB2	592306	1205562	26.21%	1.546%
54	10.840	1307	1318	1325	rBV4	233976	616100	13.40%	0.790%
55	11.063	1352	1356	1361	rVV4	93725	212031	4.61%	0.272%

56	11.222	1375	1383	1386	rBV4	108025	251447	5.47%	0.322%
57	11.299	1390	1396	1407	rVV5	454791	1066050	23.18%	1.367%
58	11.404	1407	1414	1422	rVB5	119524	330793	7.19%	0.424%
59	11.551	1434	1439	1443	rVV	554292	911814	19.83%	1.169%
60	11.593	1443	1446	1451	rVB	387099	494020	10.74%	0.633%

61	11.746	1467	1472	1477	rVB	285890	405624	8.82%	0.520%
62	11.846	1484	1489	1495	rBV4	170692	318647	6.93%	0.409%
63	11.904	1495	1499	1504	rBV2	183483	301038	6.55%	0.386%
64	12.028	1516	1520	1525	rBV2	127581	206529	4.49%	0.265%
65	12.104	1528	1533	1541	rVB2	383531	716427	15.58%	0.918%

66	12.222	1546	1553	1557	rBV4	168113	418710	9.10%	0.537%
67	12.340	1568	1573	1580	rBV	143149	309151	6.72%	0.396%
68	12.557	1606	1610	1613	rVV	194141	325188	7.07%	0.417%
69	12.604	1613	1618	1621	rVV5	121107	281344	6.12%	0.361%
70	12.646	1622	1625	1633	rVB5	148050	279010	6.07%	0.358%

71	12.751	1640	1643	1648	rVB2	155163	206616	4.49%	0.265%
72	12.957	1675	1678	1683	rVB2	488103	668969	14.55%	0.858%
73	13.051	1691	1694	1703	rVB3	160690	315348	6.86%	0.404%
74	13.569	1777	1782	1792	rVB	199812	393997	8.57%	0.505%
75	13.681	1792	1801	1805	rBV4	222959	569553	12.38%	0.730%

76	13.734	1805	1810	1817	rVB5	235179	542919	11.81%	0.696%
----	--------	------	------	------	------	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018063.D
 Acq On : 11 Nov 2023 13:32
 Operator : MA/JU
 Sample : 05079-05
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEF2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

77	13.910	1835	1840	1843	rVV	505878	768576	16.71%	0.985%
78	13.945	1843	1846	1852	rVB	1023346	1285451	27.95%	1.648%
79	14.028	1856	1860	1865	rVB	285311	383413	8.34%	0.492%
80	14.222	1888	1893	1899	rVB	1060698	1595561	34.70%	2.046%
81	14.334	1908	1912	1921	rVB	225163	447462	9.73%	0.574%
82	14.522	1939	1944	1953	rVB	560940	977212	21.25%	1.253%
83	14.904	2006	2009	2015	rVB2	134158	189905	4.13%	0.243%
84	14.987	2020	2023	2028	rVB2	180936	231204	5.03%	0.296%
85	15.040	2028	2032	2042	rVB	229623	408850	8.89%	0.524%
86	15.128	2042	2047	2051	rBV	130047	261138	5.68%	0.335%
87	15.528	2109	2115	2123	rVV	1314519	1899295	41.30%	2.435%
88	15.681	2137	2141	2143	rBV	542308	783965	17.05%	1.005%
89	16.187	2222	2227	2232	rBV	689512	965412	20.99%	1.238%
90	16.792	2327	2330	2339	rVB	212677	341846	7.43%	0.438%
91	17.016	2364	2368	2373	rVB	305058	440147	9.57%	0.564%
92	17.304	2412	2417	2428	rVB	771537	1120410	24.36%	1.436%
93	17.404	2429	2434	2440	rBV2	1614525	2265634	49.27%	2.905%
94	17.769	2493	2496	2502	rVB	155106	203536	4.43%	0.261%
95	18.157	2558	2562	2570	rBV	404270	579074	12.59%	0.742%
96	19.657	2812	2817	2824	rBV	2218651	2886953	62.78%	3.701%
97	21.086	3058	3060	3066	rVB2	191896	220477	4.79%	0.283%
98	21.433	3114	3119	3123	rBV	898141	1155370	25.12%	1.481%
99	23.774	3510	3517	3525	rVB	1504187	2889451	62.83%	3.704%
100	23.933	3538	3544	3553	rVB	612104	1274028	27.70%	1.633%




Sum of corrected areas: 78001130

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018063.D
Acq On : 11 Nov 2023 13:32
Operator : MA/JU
Sample : 05079-05
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

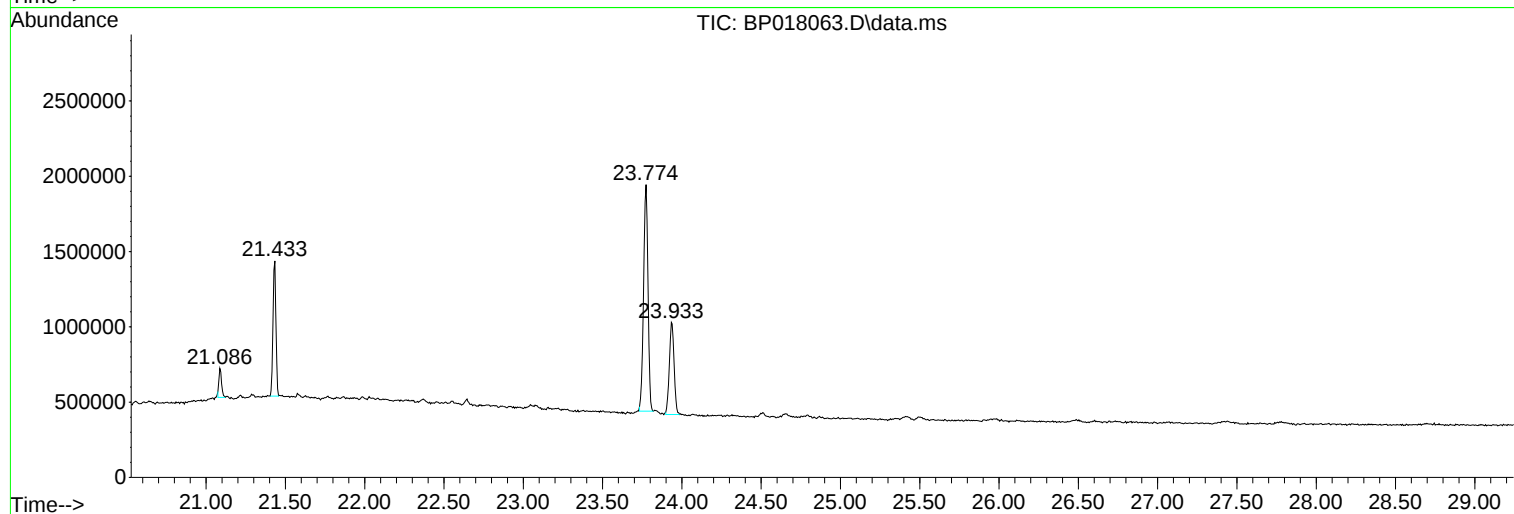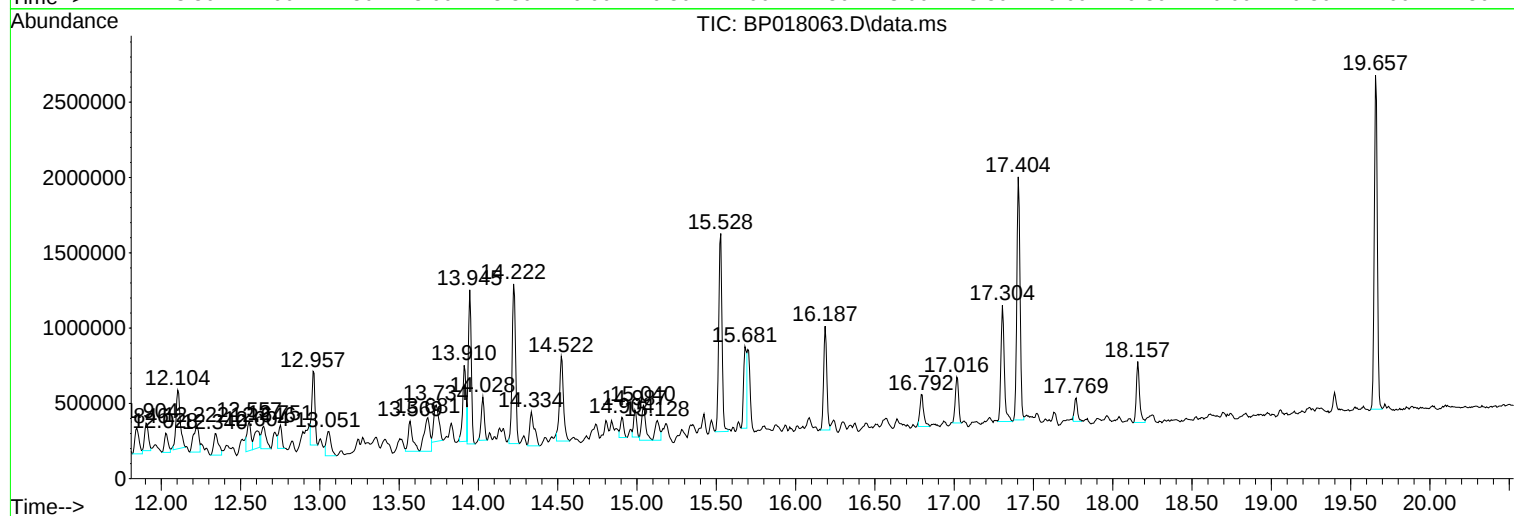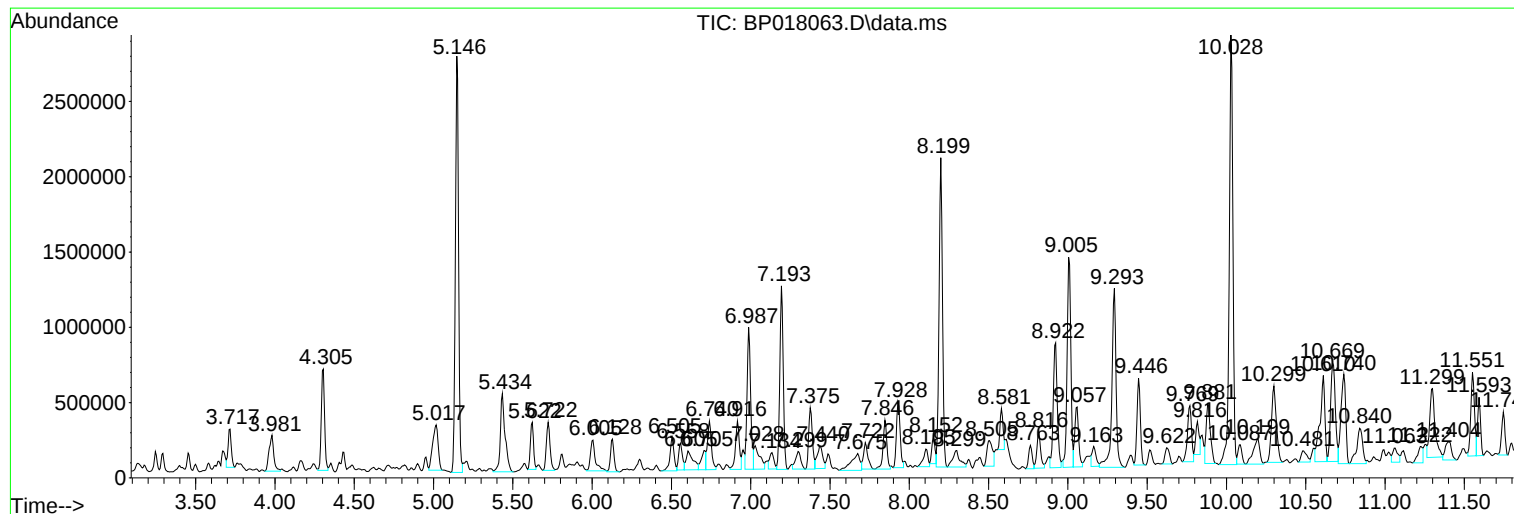

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018063.D
Acq On : 11 Nov 2023 13:32
Operator : MA/JU
Sample : 05079-05
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018063.D
Acq On : 11 Nov 2023 13:32
Operator : MA/JU
Sample : 05079-05
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEF2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------