

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018077.D
 Acq On : 11 Nov 2023 21:59
 Operator : MA/JU
 Sample : PB156805BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK805

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018077.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	29	rBV	25288	29911	1.60%	0.146%
2	3.446	58	61	63	rBV4	3601	3206	0.17%	0.016%
3	3.663	95	98	120	rBV	269279	438987	23.46%	2.150%
4	3.963	146	149	157	rVB5	6143	9009	0.48%	0.044%
5	4.869	299	303	304	rBV4	1593	2104	0.11%	0.010%
6	4.975	318	321	323	rBV4	1616	1930	0.10%	0.009%
7	5.093	340	341	342	rBV	2816	1877	0.10%	0.009%
8	5.504	410	411	414	rBV3	2162	2123	0.11%	0.010%
9	6.451	571	572	575	rBV3	2147	2248	0.12%	0.011%
10	6.569	589	592	593	rBV3	1761	1873	0.10%	0.009%
11	6.851	638	640	643	rVB4	2125	1933	0.10%	0.009%
12	7.016	662	668	684	rBV	307687	570809	30.51%	2.795%
13	7.198	693	699	713	rVB	259721	420460	22.47%	2.059%
14	7.369	720	728	744	rBV	358976	598294	31.98%	2.930%
15	7.845	801	809	824	rBV	305212	498299	26.63%	2.440%
16	8.304	880	887	891	rBV10	1456	2405	0.13%	0.012%
17	8.463	911	914	916	rVB4	2417	2110	0.11%	0.010%
18	8.575	926	933	953	rBV	370644	710227	37.96%	3.478%
19	9.051	1008	1014	1028	rBV	324171	571993	30.57%	2.801%
20	9.222	1041	1043	1046	rVB4	1760	1933	0.10%	0.009%
21	9.510	1090	1092	1095	rBV3	1991	2204	0.12%	0.011%
22	9.769	1128	1136	1150	rBV	286886	523635	27.99%	2.564%
23	10.298	1218	1226	1245	rBV	343986	725713	38.79%	3.554%
24	10.669	1280	1289	1303	rVB	398370	689386	36.85%	3.376%
25	10.845	1313	1319	1338	rBV	307883	674559	36.06%	3.303%
26	11.298	1393	1396	1398	rBV4	1649	1926	0.10%	0.009%
27	11.392	1410	1412	1416	rVB5	1892	2166	0.12%	0.011%
28	11.486	1425	1428	1433	rVB7	1610	2807	0.15%	0.014%
29	11.681	1458	1461	1462	rVV3	2923	2455	0.13%	0.012%
30	11.710	1464	1466	1469	rVB4	2904	2916	0.16%	0.014%
31	12.292	1559	1565	1567	rBV7	4419	7380	0.39%	0.036%
32	12.375	1577	1579	1582	rBV3	1817	2057	0.11%	0.010%
33	12.551	1606	1609	1612	rVB5	1719	2131	0.11%	0.010%
34	12.704	1631	1635	1640	rVB8	1962	3407	0.18%	0.017%
35	12.992	1682	1684	1686	rBV3	1864	2138	0.11%	0.010%
36	13.233	1722	1725	1727	rBV4	1901	2084	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018077.D
 Acq On : 11 Nov 2023 21:59
 Operator : MA/JU
 Sample : PB156805BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK805

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	13.357	1740	1746	1754	rBV4	5967	11657	0.62%	0.057%
38	13.492	1760	1769	1771	rBV8	2124	3868	0.21%	0.019%
39	13.627	1789	1792	1793	rBV3	2159	2357	0.13%	0.012%
40	13.733	1804	1810	1814	rBV8	2316	4014	0.21%	0.020%
41	13.945	1836	1846	1860	rBV	709924	1051624	56.21%	5.150%
42	14.033	1860	1861	1865	rVV4	2663	3451	0.18%	0.017%
43	14.063	1865	1866	1870	rVB4	1832	1874	0.10%	0.009%
44	14.222	1886	1893	1904	rBV2	800741	1161415	62.08%	5.688%
45	14.369	1915	1918	1922	rVB6	2997	4660	0.25%	0.023%
46	14.422	1926	1927	1932	rVB5	2213	3003	0.16%	0.015%
47	14.522	1936	1944	1954	rBV	592960	858203	45.87%	4.203%
48	14.798	1983	1991	2006	rBV2	112900	364564	19.49%	1.785%
49	15.145	2048	2050	2053	rVB4	2515	1897	0.10%	0.009%
50	15.304	2075	2077	2082	rVB6	3181	3004	0.16%	0.015%
51	15.521	2107	2114	2127	rBV	961675	1423677	76.10%	6.972%
52	15.680	2135	2141	2152	rBV	275269	449755	24.04%	2.202%
53	15.763	2153	2155	2161	rVB7	9030	14389	0.77%	0.070%
54	16.033	2199	2201	2204	rVB4	2042	2164	0.12%	0.011%
55	16.069	2204	2207	2209	rBV4	2187	2360	0.13%	0.012%
56	16.310	2245	2248	2251	rBV5	1829	2543	0.14%	0.012%
57	16.404	2261	2264	2266	rVV4	2783	2713	0.15%	0.013%
58	16.539	2282	2287	2288	rBV5	1931	2346	0.13%	0.011%
59	16.563	2288	2291	2294	rVB5	2048	2641	0.14%	0.013%
60	16.745	2319	2322	2324	rBV4	2260	2253	0.12%	0.011%
61	16.886	2343	2346	2348	rBV4	1816	2380	0.13%	0.012%
62	17.063	2373	2376	2378	rBV4	1990	2428	0.13%	0.012%
63	17.098	2378	2382	2386	rVV7	2442	4651	0.25%	0.023%
64	17.304	2410	2417	2425	rBV	708441	1007527	53.85%	4.934%
65	17.404	2428	2434	2447	rVV	1078646	1538827	82.25%	7.536%
66	17.515	2451	2453	2455	rVV3	3130	2533	0.14%	0.012%
67	17.557	2458	2460	2463	rBV4	2661	2560	0.14%	0.013%
68	17.633	2471	2473	2476	rBV4	1923	2412	0.13%	0.012%
69	18.157	2560	2562	2567	rVV6	2057	2776	0.15%	0.014%
70	18.268	2579	2581	2585	rBV5	1917	2427	0.13%	0.012%
71	18.557	2628	2630	2634	rVB5	2956	3473	0.19%	0.017%
72	19.227	2740	2744	2750	rBV4	13853	19937	1.07%	0.098%
73	19.304	2754	2757	2760	rVB2	9026	10572	0.57%	0.052%
74	19.657	2811	2817	2828	rBV	1338972	1760996	94.13%	8.624%
75	21.427	3113	3118	3130	rBV	793313	1117009	59.70%	5.470%
76	23.762	3508	3515	3526	rVB2	932140	1870890	100.00%	9.162%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018077.D
Acq On : 11 Nov 2023 21:59
Operator : MA/JU
Sample : PB156805BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK805

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

77	23.927	3537	3543	3554	rVB	550883	1169718	62.52%	5.728%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 20420243

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018077.D
Acq On : 11 Nov 2023 21:59
Operator : MA/JU
Sample : PB156805BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK805

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

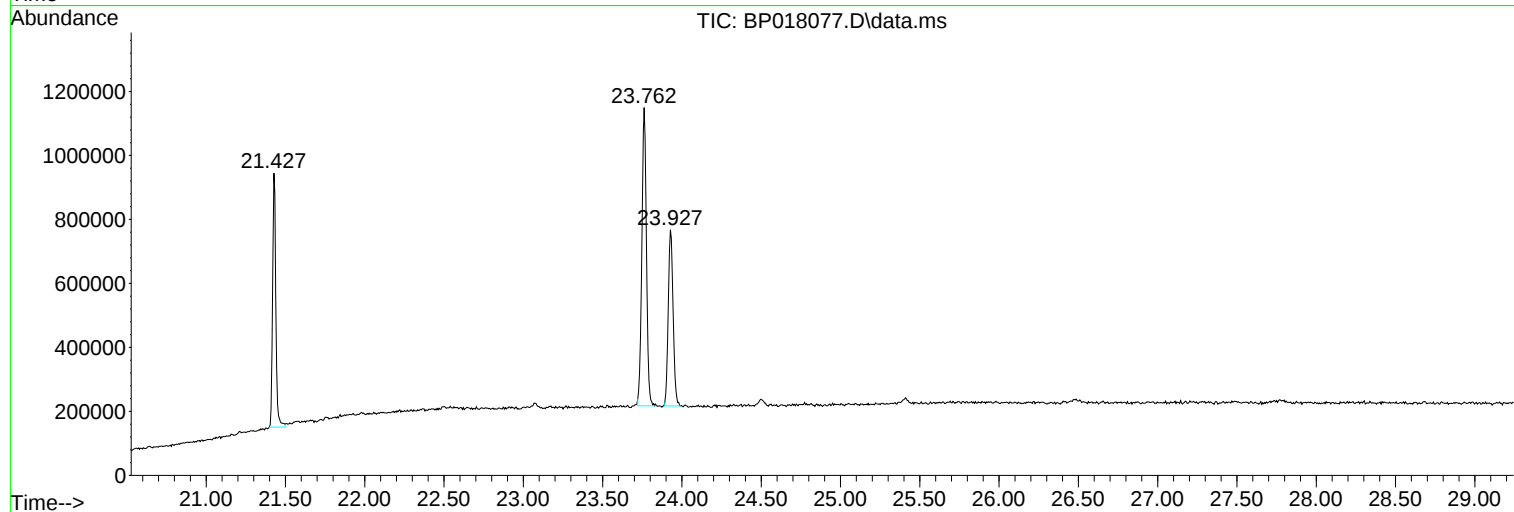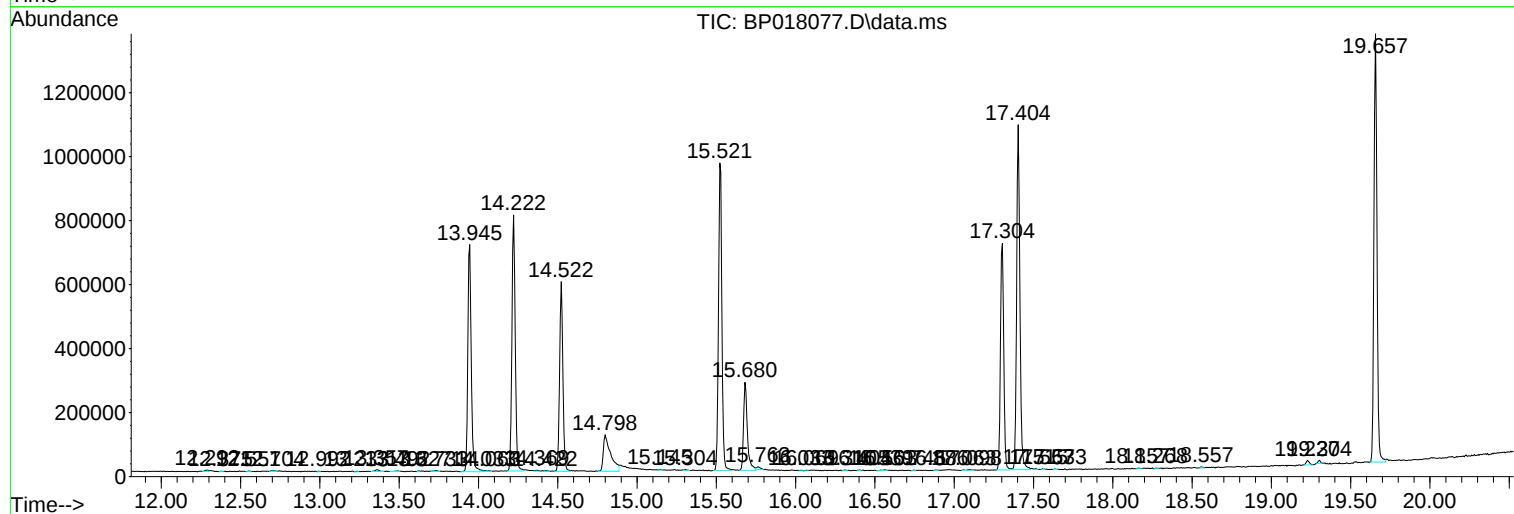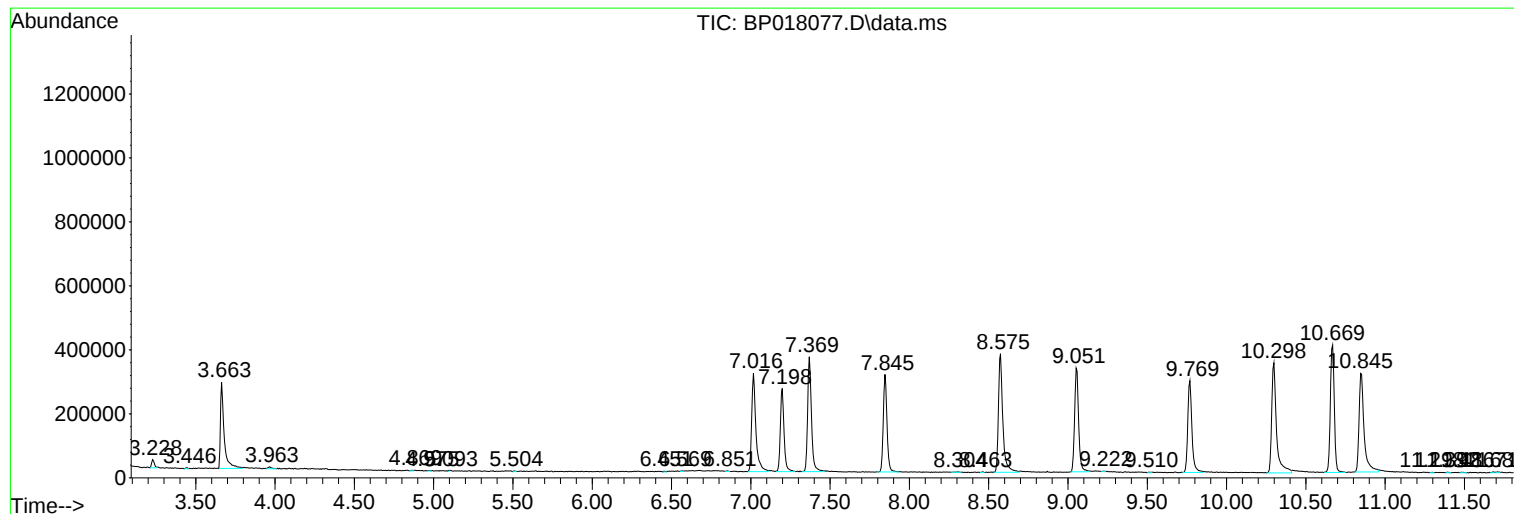

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018077.D
Acq On : 11 Nov 2023 21:59
Operator : MA/JU
Sample : PB156805BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK805

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018077.D
Acq On : 11 Nov 2023 21:59
Operator : MA/JU
Sample : PB156805BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK805

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc