

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018078.D
 Acq On : 11 Nov 2023 22:33
 Operator : MA/JU
 Sample : PB156719BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK719

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	28	rVB	22397	25304	1.29%	0.128%
2	3.664	95	98	115	rBV	238429	377791	19.29%	1.907%
3	3.964	147	149	151	rVB2	4407	3365	0.17%	0.017%
4	4.169	182	184	188	rBV4	2333	3040	0.16%	0.015%
5	5.046	331	333	337	rVB5	2501	3692	0.19%	0.019%
6	5.546	415	418	420	rBV4	2771	2900	0.15%	0.015%
7	5.775	453	457	460	rBV6	1908	1980	0.10%	0.010%
8	6.158	519	522	524	rVB3	2597	3044	0.16%	0.015%
9	6.258	536	539	541	rBV4	1623	2274	0.12%	0.011%
10	6.316	547	549	551	rBV3	2914	2249	0.11%	0.011%
11	6.493	578	579	582	rBV3	1983	2399	0.12%	0.012%
12	6.628	598	602	604	rBV3	1676	2479	0.13%	0.013%
13	6.840	636	638	641	rVV4	2222	1974	0.10%	0.010%
14	7.016	662	668	687	rBV	260806	495287	25.28%	2.501%
15	7.199	693	699	714	rVB	226479	361077	18.43%	1.823%
16	7.369	721	728	739	rBV	321690	526032	26.85%	2.656%
17	7.587	762	765	767	rVB3	2107	2508	0.13%	0.013%
18	7.846	802	809	819	rBV	288903	473129	24.15%	2.389%
19	8.075	846	848	851	rBV4	1482	2358	0.12%	0.012%
20	8.257	874	879	881	rVV6	2161	3275	0.17%	0.017%
21	8.299	884	886	889	rVV3	1999	2206	0.11%	0.011%
22	8.575	925	933	944	rBV	321557	619002	31.60%	3.125%
23	9.052	1008	1014	1027	rBV	286946	509098	25.99%	2.570%
24	9.769	1129	1136	1151	rBV	253151	473826	24.19%	2.392%
25	10.228	1212	1214	1217	rVB4	2300	2768	0.14%	0.014%
26	10.299	1217	1226	1246	rBV	308548	653124	33.34%	3.297%
27	10.669	1280	1289	1296	rBV	377721	641884	32.77%	3.241%
28	10.846	1311	1319	1334	rBV	274890	598277	30.54%	3.021%
29	11.198	1377	1379	1382	rVB4	2230	2449	0.13%	0.012%
30	11.257	1382	1389	1392	rBV9	2210	4034	0.21%	0.020%
31	11.681	1459	1461	1463	rBV3	1825	2220	0.11%	0.011%
32	12.287	1559	1564	1566	rBV6	3839	6391	0.33%	0.032%
33	12.310	1566	1568	1573	rVB6	2327	3086	0.16%	0.016%
34	12.540	1604	1607	1609	rBV4	1933	2455	0.13%	0.012%
35	12.716	1632	1637	1639	rVB6	1932	2488	0.13%	0.013%
36	13.363	1739	1747	1753	rBV6	5174	12855	0.66%	0.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018078.D
 Acq On : 11 Nov 2023 22:33
 Operator : MA/JU
 Sample : PB156719BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK719

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	13.622	1788	1791	1795	rBV6	1908	3108	0.16%	0.016%
38	13.734	1805	1810	1813	rBV6	2488	4111	0.21%	0.021%
39	13.945	1837	1846	1862	rBV	659718	980639	50.06%	4.951%
40	14.222	1886	1893	1909	rBV	729662	1075471	54.90%	5.430%
41	14.363	1916	1917	1924	rVB7	2773	3453	0.18%	0.017%
42	14.522	1936	1944	1953	rBV	582186	834776	42.61%	4.215%
43	14.798	1985	1991	2010	rBV2	118027	386147	19.71%	1.950%
44	15.298	2073	2076	2080	rVB6	2376	3226	0.16%	0.016%
45	15.522	2108	2114	2122	rBV	886590	1307978	66.77%	6.604%
46	15.681	2134	2141	2152	rBV	291429	479730	24.49%	2.422%
47	16.422	2265	2267	2270	rVB4	2637	2888	0.15%	0.015%
48	16.463	2270	2274	2276	rBV5	3377	3663	0.19%	0.018%
49	16.733	2318	2320	2321	rBV2	2816	2226	0.11%	0.011%
50	17.092	2379	2381	2385	rVB5	1909	2252	0.11%	0.011%
51	17.175	2392	2395	2397	rBV4	1991	2979	0.15%	0.015%
52	17.304	2409	2417	2427	rBV	761320	1053715	53.79%	5.320%
53	17.404	2428	2434	2446	rVV2	1012169	1489071	76.01%	7.518%
54	17.545	2455	2458	2461	rVB5	2404	2357	0.12%	0.012%
55	17.828	2502	2506	2507	rBV4	1790	2090	0.11%	0.011%
56	17.922	2520	2522	2523	rBV2	2525	1981	0.10%	0.010%
57	18.057	2543	2545	2548	rVB4	2193	2311	0.12%	0.012%
58	18.263	2579	2580	2583	rBV3	2791	2625	0.13%	0.013%
59	18.322	2588	2590	2593	rVB4	1911	2043	0.10%	0.010%
60	18.563	2626	2631	2634	rBV7	3164	7089	0.36%	0.036%
61	19.227	2741	2744	2749	rVB5	14225	18721	0.96%	0.095%
62	19.298	2753	2756	2759	rVV2	10602	13167	0.67%	0.066%
63	19.657	2811	2817	2827	rBV	1349534	1817133	92.76%	9.174%
64	21.427	3113	3118	3127	rBV2	876553	1222830	62.42%	6.174%
65	23.763	3508	3515	3527	rVB2	930140	1958962	100.00%	9.890%
66	23.933	3537	3544	3557	rVB	608761	1287867	65.74%	6.502%




Sum of corrected areas: 19806929

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018078.D
Acq On : 11 Nov 2023 22:33
Operator : MA/JU
Sample : PB156719BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

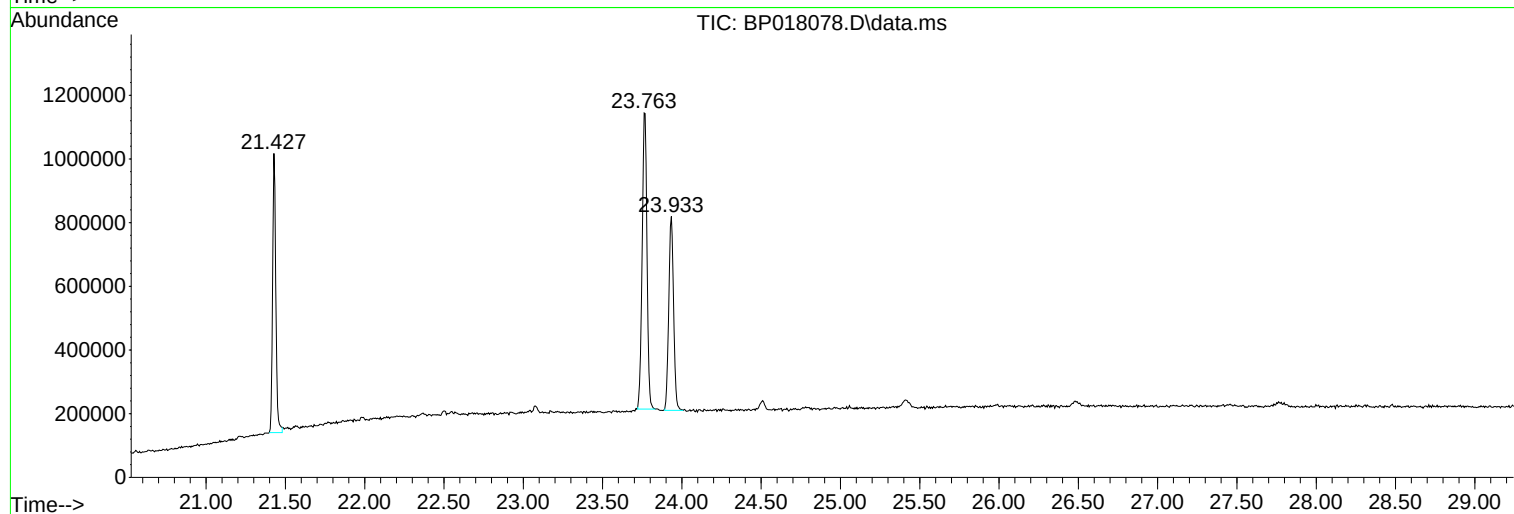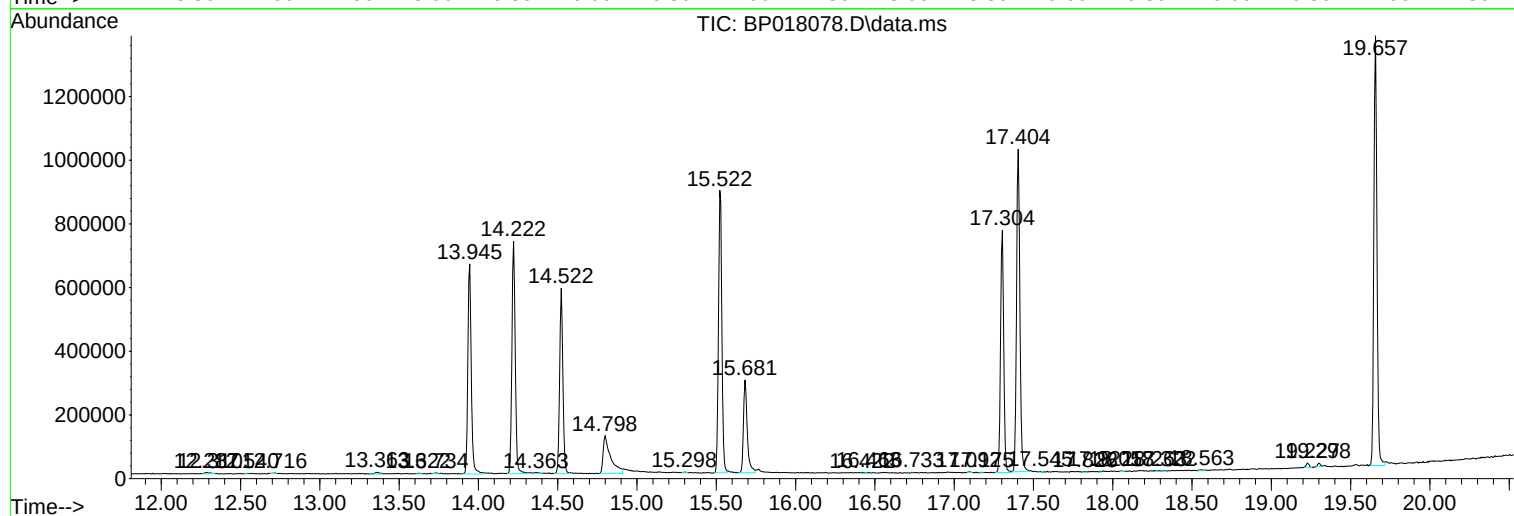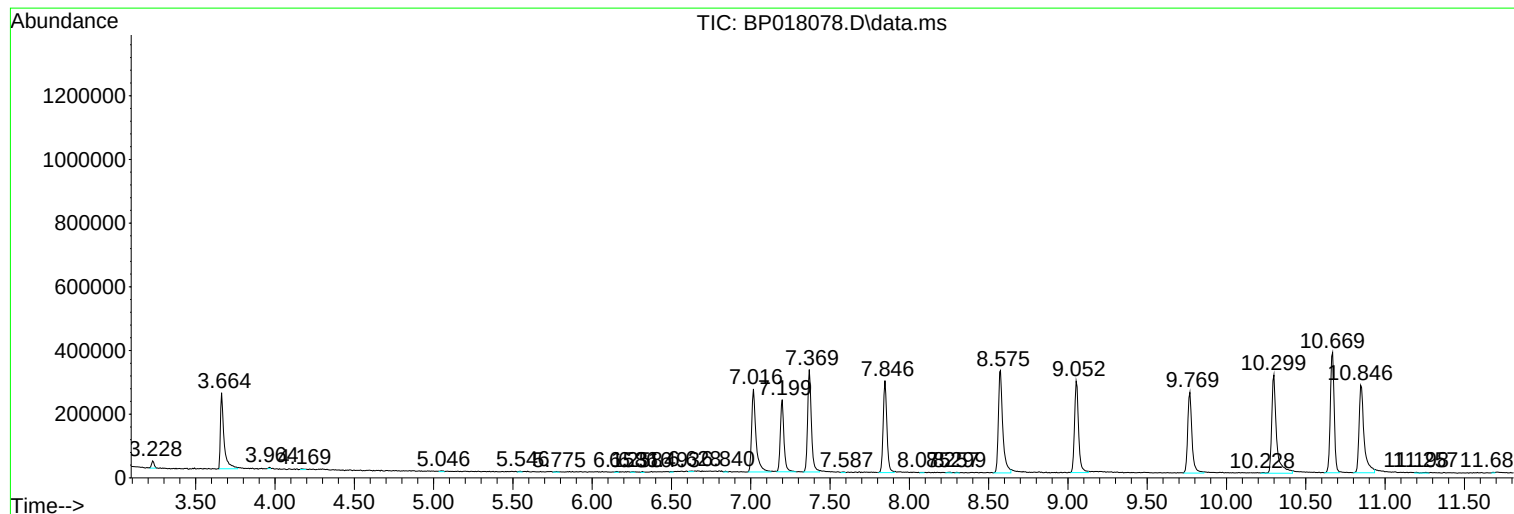

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018078.D
Acq On : 11 Nov 2023 22:33
Operator : MA/JU
Sample : PB156719BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018078.D
Acq On : 11 Nov 2023 22:33
Operator : MA/JU
Sample : PB156719BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------