

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018085.D
 Acq On : 12 Nov 2023 02:31
 Operator : MA/JU
 Sample : 05044-17
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	28	rVB	14322	16909	0.63%	0.080%
2	3.499	66	70	74	rBV	10312	13112	0.48%	0.062%
3	3.670	96	99	108	rBV	146785	235903	8.72%	1.110%
4	3.764	112	115	121	rVB7	9714	17065	0.63%	0.080%
5	3.840	126	128	132	rVB4	7275	8879	0.33%	0.042%
6	3.964	146	149	156	rVB7	6059	9495	0.35%	0.045%
7	4.281	200	203	207	rBV6	8263	15839	0.59%	0.075%
8	4.481	231	237	243	rBV2	42366	61852	2.29%	0.291%
9	4.646	263	265	267	rBV3	2822	3059	0.11%	0.014%
10	4.705	273	275	279	rVB5	3098	4243	0.16%	0.020%
11	4.922	307	312	313	rBV5	2388	3579	0.13%	0.017%
12	4.946	313	316	320	rVV5	5856	8735	0.32%	0.041%
13	5.022	325	329	331	rVV5	4799	7183	0.27%	0.034%
14	5.058	331	335	339	rVB7	4729	7313	0.27%	0.034%
15	5.287	369	374	376	rBV5	4512	5157	0.19%	0.024%
16	5.481	405	407	412	rBV6	2874	3346	0.12%	0.016%
17	5.716	446	447	449	rBV2	3338	2838	0.10%	0.013%
18	5.734	449	450	454	rVB4	2848	3445	0.13%	0.016%
19	6.087	508	510	514	rVB4	2432	3375	0.12%	0.016%
20	6.122	514	516	520	rBV5	1850	3397	0.13%	0.016%
21	6.222	528	533	537	rBV8	1872	3142	0.12%	0.015%
22	6.640	602	604	607	rVB4	2346	2710	0.10%	0.013%
23	6.816	631	634	639	rVB7	2662	3307	0.12%	0.016%
24	7.028	662	670	683	rBV	65930	153126	5.66%	0.720%
25	7.116	683	685	689	rVB5	2962	3405	0.13%	0.016%
26	7.199	693	699	714	rBV	247624	410460	15.17%	1.931%
27	7.369	720	728	742	rBV	257461	459370	16.98%	2.161%
28	7.846	802	809	820	rBV	269525	431699	15.96%	2.031%
29	8.305	883	887	892	rBV7	2100	4280	0.16%	0.020%
30	8.581	927	934	947	rBV	202238	395737	14.63%	1.862%
31	8.875	982	984	987	rBV4	2957	3418	0.13%	0.016%
32	9.052	1008	1014	1031	rBV	323734	582930	21.55%	2.743%
33	9.169	1031	1034	1035	rVV3	3434	3044	0.11%	0.014%
34	9.216	1039	1042	1048	rVB8	6302	10161	0.38%	0.048%
35	9.381	1066	1070	1072	rBV5	1833	2961	0.11%	0.014%
36	9.428	1076	1078	1082	rVB5	2459	2864	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018085.D
 Acq On : 12 Nov 2023 02:31
 Operator : MA/JU
 Sample : 05044-17
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	9.487	1082	1088	1090	rBV7	1690	2866	0.11%	0.013%
38	9.681	1118	1121	1127	rVB8	1888	3248	0.12%	0.015%
39	9.763	1129	1135	1150	rVV	237832	447787	16.55%	2.107%
40	9.869	1150	1153	1155	rVB4	2906	2991	0.11%	0.014%

41	10.299	1217	1226	1247	rBV	311530	656358	24.26%	3.088%
42	10.663	1280	1288	1297	rBV	338199	591439	21.86%	2.783%
43	10.752	1300	1303	1308	rVB7	1807	3767	0.14%	0.018%
44	10.846	1312	1319	1337	rBV	319470	679592	25.12%	3.198%
45	11.710	1465	1466	1471	rVB5	4794	5591	0.21%	0.026%

46	11.940	1501	1505	1511	rVB9	4559	5679	0.21%	0.027%
47	12.040	1517	1522	1524	rBV6	2509	3635	0.13%	0.017%
48	12.204	1544	1550	1554	rBV9	2810	4413	0.16%	0.021%
49	12.275	1559	1562	1564	rBV4	3475	4826	0.18%	0.023%
50	12.434	1586	1589	1594	rBV7	2438	3485	0.13%	0.016%

51	12.716	1630	1637	1638	rBV7	4875	7239	0.27%	0.034%
52	12.910	1669	1670	1674	rBV4	2750	3513	0.13%	0.017%
53	13.046	1690	1693	1696	rBV5	3499	4196	0.16%	0.020%
54	13.269	1727	1731	1737	rBV9	3059	6970	0.26%	0.033%
55	13.357	1740	1746	1752	rBV	67826	103957	3.84%	0.489%

56	13.481	1760	1767	1769	rBV8	3204	5806	0.21%	0.027%
57	13.498	1769	1770	1774	rVB4	4475	5150	0.19%	0.024%
58	13.704	1801	1805	1806	rBV4	2533	3390	0.13%	0.016%
59	13.728	1806	1809	1810	rBV3	3522	3545	0.13%	0.017%
60	13.940	1839	1845	1858	rBV	803173	1179706	43.61%	5.551%

61	14.222	1886	1893	1910	rVV2	841450	1293471	47.82%	6.086%
62	14.522	1937	1944	1955	rBV	536535	776028	28.69%	3.651%
63	14.887	2002	2006	2007	rBV4	2102	3190	0.12%	0.015%
64	14.928	2009	2013	2014	rVV4	3296	4428	0.16%	0.021%
65	15.028	2028	2030	2033	rVB4	3763	3690	0.14%	0.017%

66	15.234	2064	2065	2068	rBV3	2346	2717	0.10%	0.013%
67	15.292	2070	2075	2076	rBV5	4279	5651	0.21%	0.027%
68	15.522	2107	2114	2130	rBV	1153158	1701987	62.92%	8.008%
69	15.704	2142	2145	2146	rBV2	4981	3914	0.14%	0.018%
70	15.763	2152	2155	2161	rVB8	5862	9509	0.35%	0.045%

71	16.939	2352	2355	2356	rBV3	3938	4690	0.17%	0.022%
72	17.092	2379	2381	2384	rBV4	3686	3930	0.15%	0.018%
73	17.298	2410	2416	2428	rBV	655240	977983	36.15%	4.602%
74	17.404	2428	2434	2446	rVV	1332970	1951210	72.13%	9.181%
75	17.628	2470	2472	2476	rBV5	4408	5667	0.21%	0.027%

76	17.922	2520	2522	2526	rVB5	5705	7226	0.27%	0.034%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018085.D
 Acq On : 12 Nov 2023 02:31
 Operator : MA/JU
 Sample : 05044-17
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHEF3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

77	18.145	2556	2560	2569	rBV	51398	91645	3.39%	0.431%
78	19.063	2713	2716	2720	rVB3	44054	48046	1.78%	0.226%
79	19.222	2741	2743	2747	rVB4	19556	21321	0.79%	0.100%
80	19.298	2753	2756	2759	rVB4	18694	24195	0.89%	0.114%
81	19.392	2769	2772	2779	rBV8	29709	38721	1.43%	0.182%
82	19.657	2811	2817	2825	rBV	1970967	2539712	93.89%	11.950%
83	21.080	3056	3059	3065	rVB5	59425	77967	2.88%	0.367%
84	21.427	3113	3118	3125	rBV	875112	1144009	42.29%	5.383%
85	23.763	3508	3515	3528	rVB2	1303425	2705005	100.00%	12.728%
86	23.927	3537	3543	3551	rVB	577895	1160691	42.91%	5.461%




Sum of corrected areas: 21253090

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018085.D
Acq On : 12 Nov 2023 02:31
Operator : MA/JU
Sample : 05044-17
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

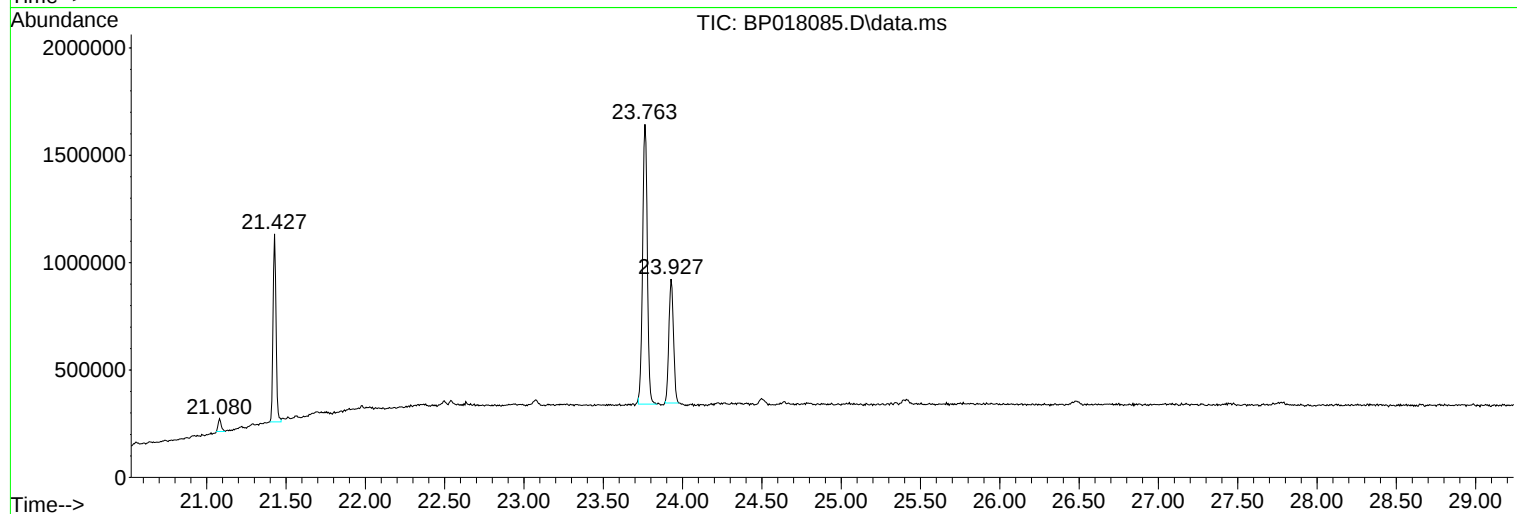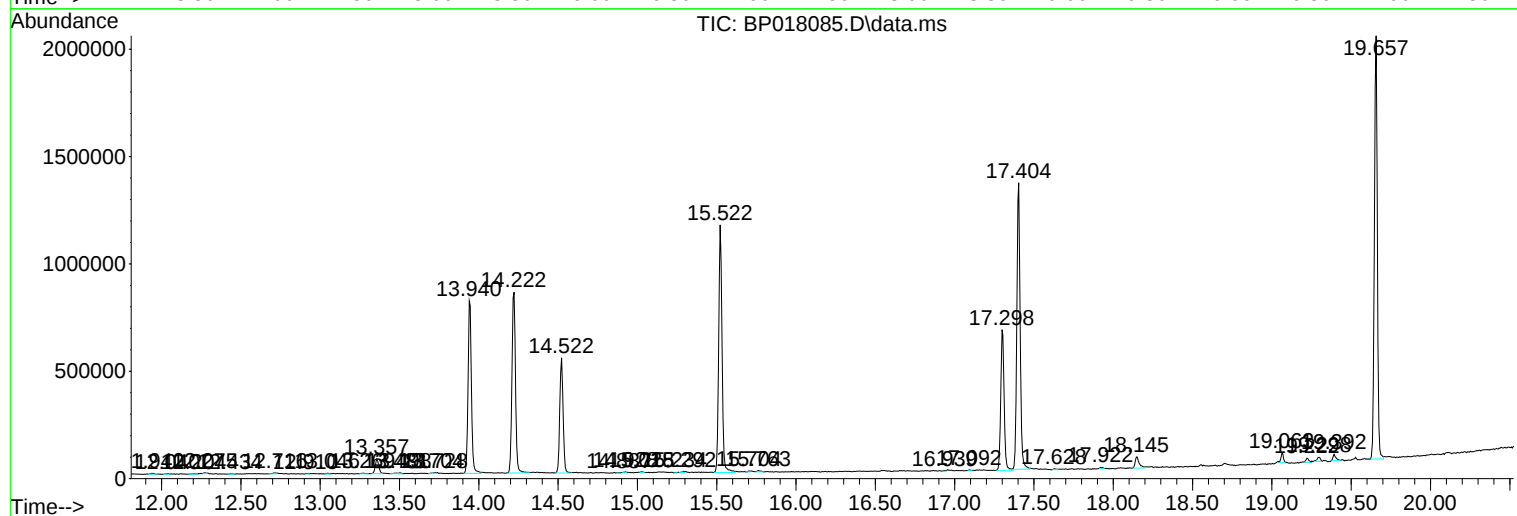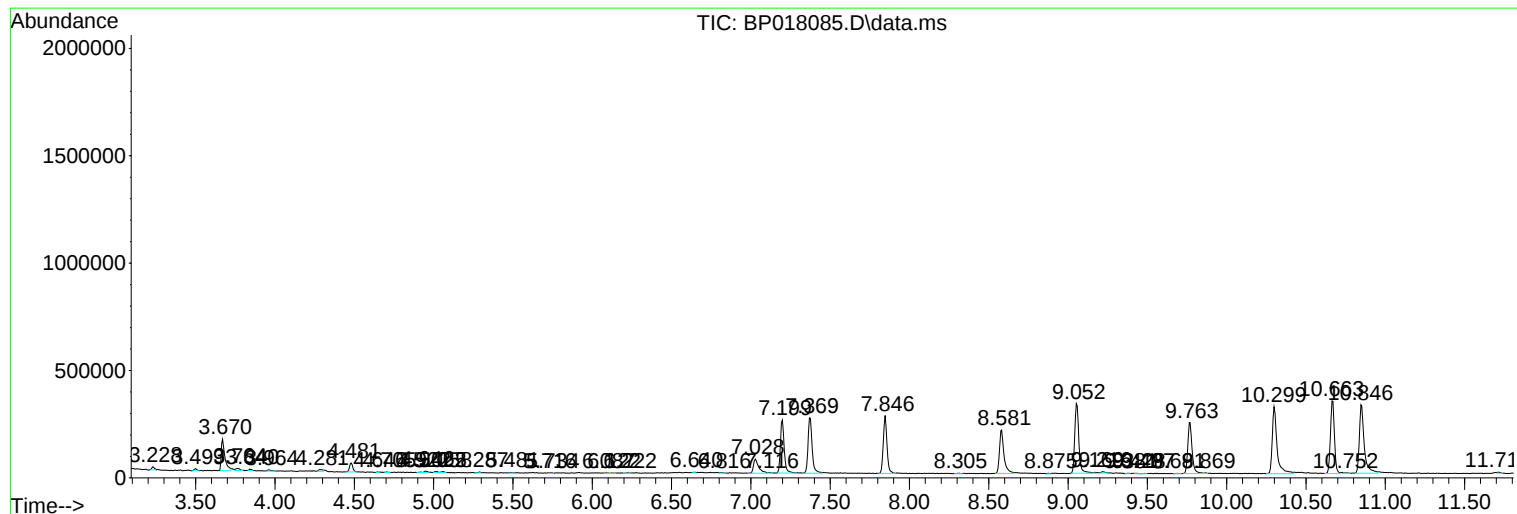

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018085.D
Acq On : 12 Nov 2023 02:31
Operator : MA/JU
Sample : 05044-17
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEF3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.481	2.87 ng/ul	61852	1,4-Dichlorobenzene-d4	7.846

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	12

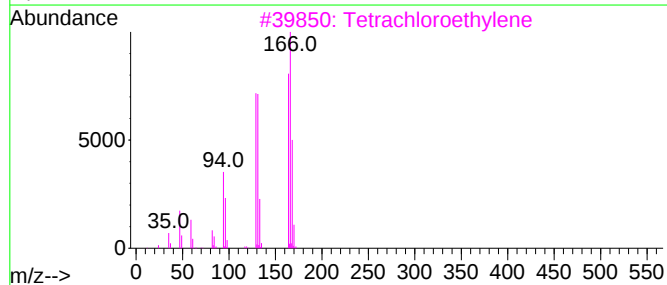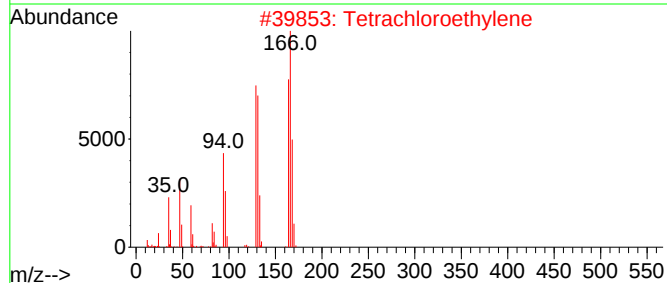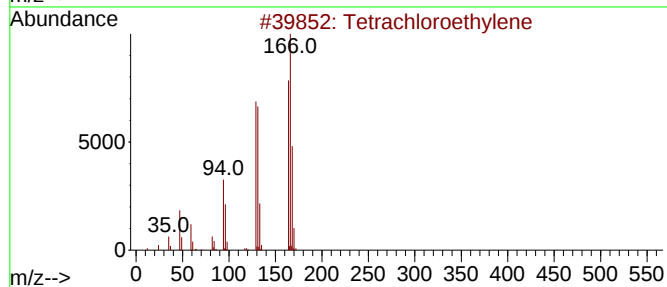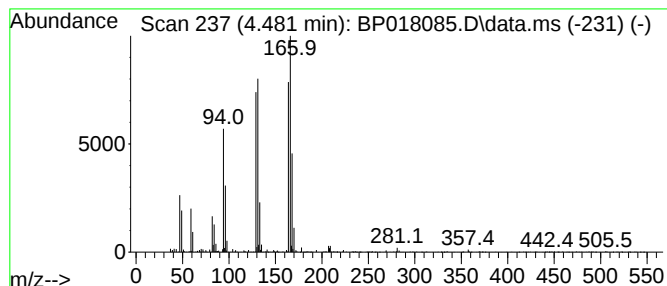

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018085.D
Acq On : 12 Nov 2023 02:31
Operator : MA/JU
Sample : 05044-17
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEF3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 N-(4-tert-Butoxyphenyl)acet... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.357	2.68 ng/ul	103957	Acenaphthene-d10	14.522

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			N-(4-tert-Butoxyphenyl)acetamide	207	C12H17NO2	002109-73-1	58
2			Metacetamol	151	C8H9NO2	000621-42-1	58
3			2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	58
4			Metacetamol	151	C8H9NO2	000621-42-1	58
5			Acetaminophen	151	C8H9NO2	000103-90-2	53

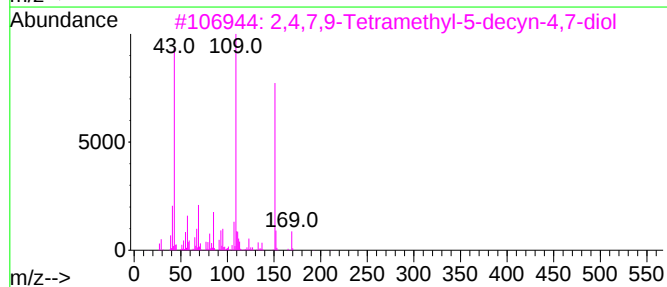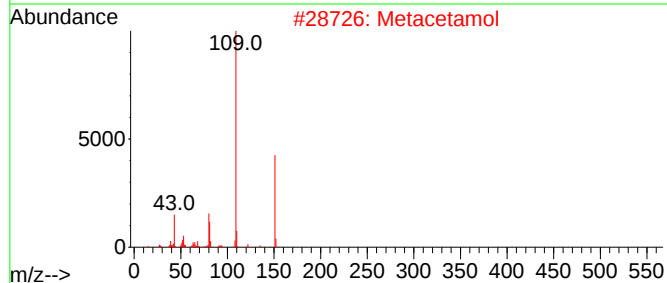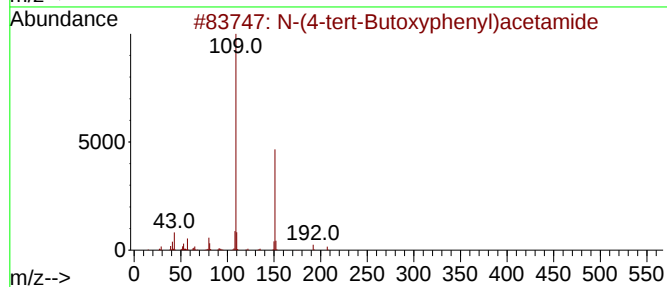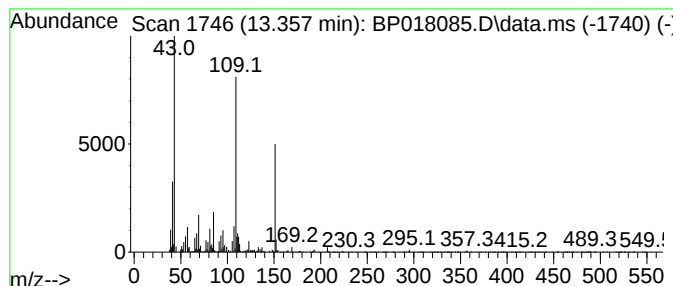

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018085.D
Acq On : 12 Nov 2023 02:31
Operator : MA/JU
Sample : 05044-17
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHEF3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.481	2.9	ng/u1	61852	1	7.846	431699	20.0
N-(4-tert-Butox...	13.357	2.7	ng/u1	103957	3	14.522	776028	20.0