

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018087.D
 Acq On : 12 Nov 2023 03:39
 Operator : MA/JU
 Sample : 05091-11RE
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKI8RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	30	rVB3	7431	9595	0.52%	0.053%
2	3.658	95	97	99	rBV3	2353	2730	0.15%	0.015%
3	3.717	102	107	111	rVV5	7600	20446	1.10%	0.113%
4	3.769	114	116	122	rVV4	10261	17042	0.92%	0.094%
5	3.846	124	129	136	rVB2	19549	29071	1.56%	0.160%
6	3.958	145	148	153	rBV3	5615	7768	0.42%	0.043%
7	4.493	237	239	244	rVB6	2874	4132	0.22%	0.023%
8	4.734	277	280	282	rBV3	2127	2041	0.11%	0.011%
9	4.893	302	307	315	rVB	22973	36257	1.95%	0.200%
10	5.064	332	336	337	rBV4	3249	3389	0.18%	0.019%
11	5.452	401	402	405	rVV3	3000	2197	0.12%	0.012%
12	5.475	405	406	410	rVV4	2380	2736	0.15%	0.015%
13	5.516	410	413	415	rVV4	2675	3374	0.18%	0.019%
14	5.558	417	420	423	rVB5	3772	3686	0.20%	0.020%
15	5.969	488	490	493	rBV4	1903	2166	0.12%	0.012%
16	6.340	550	553	555	rBV4	2472	2602	0.14%	0.014%
17	6.511	576	582	583	rBV6	1465	2048	0.11%	0.011%
18	6.681	609	611	613	rBV2	3834	3990	0.21%	0.022%
19	6.846	637	639	641	rVB3	2521	2403	0.13%	0.013%
20	6.922	650	652	656	rBV5	1853	2678	0.14%	0.015%
21	7.022	663	669	688	rBV	155928	359605	19.33%	1.984%
22	7.199	693	699	707	rVV	137843	223566	12.02%	1.233%
23	7.369	722	728	742	rBV	189413	331017	17.79%	1.826%
24	7.587	762	765	769	rVB5	1764	2059	0.11%	0.011%
25	7.846	803	809	821	rBV	428522	690018	37.09%	3.807%
26	8.005	835	836	841	rVB5	1892	2134	0.11%	0.012%
27	8.334	891	892	897	rBV5	1765	2829	0.15%	0.016%
28	8.581	926	934	950	rBV	121111	254849	13.70%	1.406%
29	8.705	950	955	970	rVB	117027	218243	11.73%	1.204%
30	9.057	1007	1015	1025	rBV	177365	323639	17.40%	1.786%
31	9.593	1103	1106	1108	rBV4	1555	2055	0.11%	0.011%
32	9.769	1128	1136	1150	rBV	152862	291252	15.66%	1.607%
33	9.975	1164	1171	1178	rBV6	11390	34228	1.84%	0.189%
34	10.146	1195	1200	1209	rBV3	12371	24726	1.33%	0.136%
35	10.304	1220	1227	1245	rBV	169662	381935	20.53%	2.107%
36	10.663	1281	1288	1297	rBV	558063	939999	50.53%	5.186%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018087.D
 Acq On : 12 Nov 2023 03:39
 Operator : MA/JU
 Sample : 05091-11RE
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKI8RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	10.857	1308	1321	1333	rBV	111822	266837	14.34%	1.472%
38	11.128	1362	1367	1369	rBV5	1686	3298	0.18%	0.018%
39	11.216	1378	1382	1385	rBV6	2600	4265	0.23%	0.024%
40	11.263	1385	1390	1396	rVB10	5626	10340	0.56%	0.057%
41	11.546	1434	1438	1441	rBV5	2701	4573	0.25%	0.025%
42	11.622	1449	1451	1454	rVB4	2687	2897	0.16%	0.016%
43	11.698	1459	1464	1466	rBV6	1763	3299	0.18%	0.018%
44	11.816	1481	1484	1487	rVB5	2262	2806	0.15%	0.015%
45	12.263	1556	1560	1565	rVB8	3584	6448	0.35%	0.036%
46	12.457	1589	1593	1595	rVB5	2086	2237	0.12%	0.012%
47	12.545	1604	1608	1609	rBV4	2590	3061	0.16%	0.017%
48	12.822	1652	1655	1658	rBV5	2466	3663	0.20%	0.020%
49	12.940	1674	1675	1679	rBV4	2159	2141	0.12%	0.012%
50	13.028	1687	1690	1693	rVB5	2441	2819	0.15%	0.016%
51	13.087	1697	1700	1704	rBV5	2788	4398	0.24%	0.024%
52	13.257	1727	1729	1733	rBV5	2807	2379	0.13%	0.013%
53	13.357	1738	1746	1753	rBV2	22832	43510	2.34%	0.240%
54	13.457	1759	1763	1766	rBV6	1513	2291	0.12%	0.013%
55	13.481	1766	1767	1772	rVB5	2977	2858	0.15%	0.016%
56	13.734	1806	1810	1812	rVV5	2717	3481	0.19%	0.019%
57	13.775	1815	1817	1820	rBV3	3289	2991	0.16%	0.017%
58	13.869	1829	1833	1834	rVB4	2737	2621	0.14%	0.014%
59	13.940	1838	1845	1853	rBV	418564	629485	33.84%	3.473%
60	14.004	1853	1856	1862	rVB8	15365	23723	1.28%	0.131%
61	14.222	1886	1893	1903	rBV	478052	710040	38.17%	3.917%
62	14.340	1909	1913	1915	rBV5	2760	3340	0.18%	0.018%
63	14.522	1936	1944	1952	rBV	846812	1237797	66.53%	6.829%
64	14.657	1965	1967	1971	rVB5	1981	2047	0.11%	0.011%
65	14.816	1987	1994	2006	rBV3	52396	170543	9.17%	0.941%
66	14.998	2022	2025	2033	rVB10	8754	17467	0.94%	0.096%
67	15.104	2042	2043	2045	rBV2	2562	2020	0.11%	0.011%
68	15.298	2074	2076	2081	rVB5	4241	5129	0.28%	0.028%
69	15.522	2105	2114	2122	rBV	633244	911915	49.02%	5.031%
70	15.681	2136	2141	2152	rBV	114243	200626	10.78%	1.107%
71	15.910	2177	2180	2183	rBV5	3868	4716	0.25%	0.026%
72	16.298	2241	2246	2247	rBV5	2189	2887	0.16%	0.016%
73	16.469	2271	2275	2279	rVB6	6558	10182	0.55%	0.056%
74	16.510	2279	2282	2285	rBV4	2771	4194	0.23%	0.023%
75	16.669	2303	2309	2312	rBV8	3914	7265	0.39%	0.040%
76	16.822	2331	2335	2340	rBV7	8401	13727	0.74%	0.076%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018087.D
 Acq On : 12 Nov 2023 03:39
 Operator : MA/JU
 Sample : 05091-11RE
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKI8RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

77	16.975	2358	2361	2365	rVB6	3992	5189	0.28%	0.029%
78	17.092	2378	2381	2384	rBV4	3019	5338	0.29%	0.029%
79	17.298	2408	2416	2428	rBV	1088101	1600501	86.03%	8.830%
80	17.404	2428	2434	2448	rVV	653379	1009310	54.25%	5.569%
81	17.510	2448	2452	2457	rVB7	7289	13018	0.70%	0.072%
82	17.633	2471	2473	2475	rBV3	3149	3260	0.18%	0.018%
83	17.716	2485	2487	2489	rBV3	3580	2993	0.16%	0.017%
84	17.792	2498	2500	2506	rVB6	5185	7205	0.39%	0.040%
85	17.922	2519	2522	2528	rBV8	6209	11901	0.64%	0.066%
86	18.075	2545	2548	2552	rVB	5893	6186	0.33%	0.034%
87	18.145	2556	2560	2570	rBV	85167	138704	7.46%	0.765%
88	18.545	2625	2628	2633	rBV6	13679	22264	1.20%	0.123%
89	18.751	2660	2663	2668	rVB4	22524	33676	1.81%	0.186%
90	18.975	2698	2701	2705	rBV	27755	33741	1.81%	0.186%
91	19.016	2705	2708	2714	rVB6	16454	21869	1.18%	0.121%
92	19.327	2758	2761	2765	rVB	34179	43507	2.34%	0.240%
93	19.392	2768	2772	2777	rBV3	49426	68146	3.66%	0.376%
94	19.527	2792	2795	2798	rBV5	17010	21214	1.14%	0.117%
95	19.651	2811	2816	2826	rBV	956886	1350808	72.61%	7.453%
96	20.604	2976	2978	2981	rVB	30838	25796	1.39%	0.142%
97	21.080	3054	3059	3063	rBV6	94500	160999	8.65%	0.888%
98	21.427	3113	3118	3129	rVB	1421918	1851721	99.53%	10.216%
99	23.763	3509	3515	3522	rVB2	637592	1244741	66.91%	6.867%
100	23.927	3536	3543	3555	rVB	870340	1860398	100.00%	10.264%




Sum of corrected areas: 18125306

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018087.D
Acq On : 12 Nov 2023 03:39
Operator : MA/JU
Sample : 05091-11RE
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKI8RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

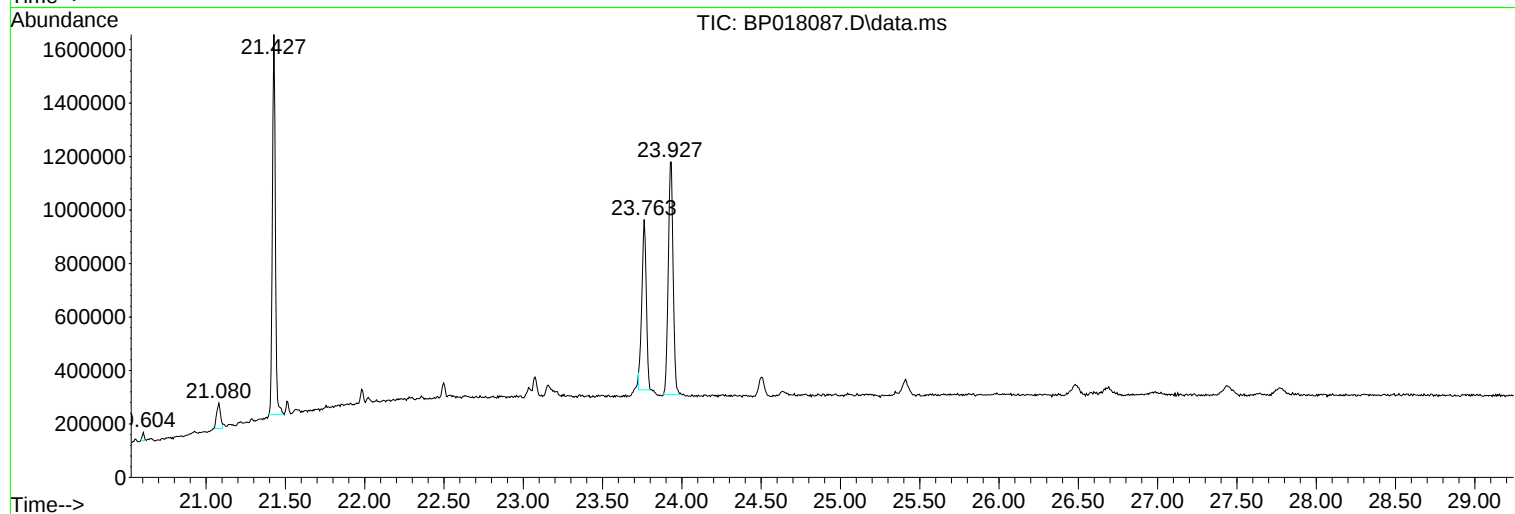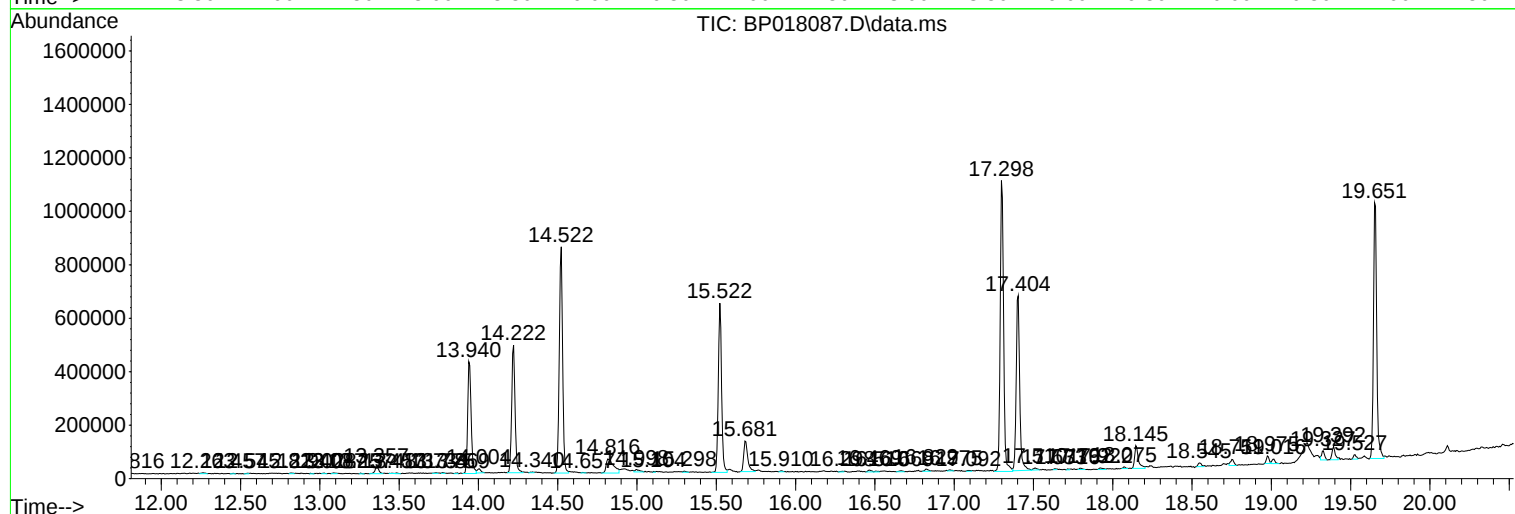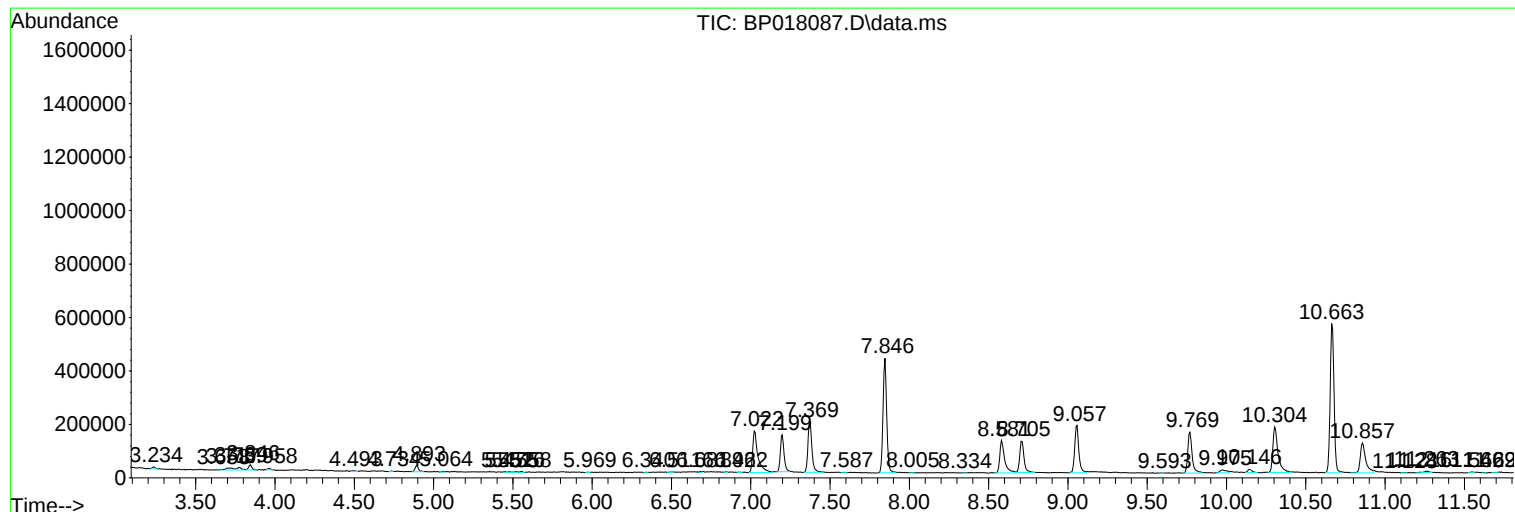

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018087.D
Acq On : 12 Nov 2023 03:39
Operator : MA/JU
Sample : 05091-11RE
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKI8RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018087.D
Acq On : 12 Nov 2023 03:39
Operator : MA/JU
Sample : 05091-11RE
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKI8RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------