

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018090.D
 Acq On : 12 Nov 2023 05:21
 Operator : MA/JU
 Sample : 05082-01
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH321

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	35	rVB	18556	25958	0.91%	0.093%
2	3.669	96	99	109	rBV	91859	147388	5.19%	0.529%
3	3.840	125	128	133	rVB3	7459	11625	0.41%	0.042%
4	3.964	146	149	154	rVB6	7894	12526	0.44%	0.045%
5	4.605	254	258	261	rBV5	2698	3534	0.12%	0.013%
6	5.852	468	470	474	rVB5	2417	3082	0.11%	0.011%
7	7.022	663	669	681	rBV	78630	169229	5.96%	0.607%
8	7.193	692	698	711	rBV	378914	609658	21.46%	2.187%
9	7.369	719	728	742	rBV	388541	653608	23.01%	2.344%
10	7.846	801	809	829	rBV	423123	724495	25.50%	2.599%
11	8.575	921	933	950	rBV	274540	533435	18.78%	1.913%
12	8.710	954	956	961	rVB5	4544	5931	0.21%	0.021%
13	9.052	1005	1014	1031	rBV	506094	892161	31.41%	3.200%
14	9.587	1102	1105	1108	rBV5	2520	3058	0.11%	0.011%
15	9.763	1126	1135	1153	rBV	437341	772619	27.20%	2.771%
16	9.899	1156	1158	1162	rVB5	2670	2991	0.11%	0.011%
17	10.293	1218	1225	1246	rVV	493342	1006584	35.43%	3.611%
18	10.663	1276	1288	1302	rBV	599453	1001001	35.24%	3.591%
19	10.846	1312	1319	1343	rBV	448510	921415	32.44%	3.305%
20	12.028	1516	1520	1523	rBV5	6408	10578	0.37%	0.038%
21	12.269	1554	1561	1566	rBV6	7878	14275	0.50%	0.051%
22	12.351	1570	1575	1578	rBV3	6780	12561	0.44%	0.045%
23	12.575	1607	1613	1616	rBV4	8671	16740	0.59%	0.060%
24	12.616	1618	1620	1623	rVB3	2649	3128	0.11%	0.011%
25	12.704	1630	1635	1640	rBV10	1800	3672	0.13%	0.013%
26	12.834	1652	1657	1659	rBV5	2447	3006	0.11%	0.011%
27	13.263	1725	1730	1736	rBV7	15544	33247	1.17%	0.119%
28	13.363	1741	1747	1752	rVB2	18283	33002	1.16%	0.118%
29	13.445	1758	1761	1763	rBV4	3214	3567	0.13%	0.013%
30	13.734	1804	1810	1813	rVB7	3140	5639	0.20%	0.020%
31	13.940	1839	1845	1859	rBV	1203881	1725865	60.75%	6.191%
32	14.134	1875	1878	1882	rVB6	1872	2918	0.10%	0.010%
33	14.222	1886	1893	1908	rVV2	1250627	1881549	66.23%	6.749%
34	14.522	1936	1944	1955	rBV	883224	1271458	44.76%	4.561%
35	14.839	1990	1998	2009	rBV4	21349	78908	2.78%	0.283%
36	15.010	2023	2027	2028	rBV4	3151	3786	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018090.D
 Acq On : 12 Nov 2023 05:21
 Operator : MA/JU
 Sample : 05082-01
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH321

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	15.139	2044	2049	2056	rVB4	4262	8264	0.29%	0.030%
38	15.216	2059	2062	2064	rVV4	3674	4582	0.16%	0.016%
39	15.257	2068	2069	2072	rVV3	5135	4265	0.15%	0.015%
40	15.304	2072	2077	2082	rVV9	10960	21890	0.77%	0.079%
41	15.345	2082	2084	2088	rVV5	6539	10051	0.35%	0.036%
42	15.522	2107	2114	2123	rBV	1630079	2314393	81.47%	8.302%
43	15.681	2134	2141	2152	rBV	428838	667510	23.50%	2.394%
44	15.757	2152	2154	2164	rVB10	11811	25445	0.90%	0.091%
45	16.145	2218	2220	2223	rVB4	3367	3252	0.11%	0.012%
46	16.563	2286	2291	2293	rBV6	4745	6235	0.22%	0.022%
47	17.251	2404	2408	2410	rBV5	2702	3005	0.11%	0.011%
48	17.298	2410	2416	2427	rVV	933276	1344783	47.34%	4.824%
49	17.404	2427	2434	2448	rVV	1768757	2593248	91.29%	9.302%
50	17.792	2496	2500	2501	rBV4	2247	2936	0.10%	0.011%
51	17.933	2520	2524	2528	rBV5	17874	21417	0.75%	0.077%
52	18.145	2557	2560	2568	rBV2	34099	51854	1.83%	0.186%
53	18.245	2572	2577	2580	rBV3	6674	11782	0.41%	0.042%
54	18.463	2611	2614	2615	rBV3	3335	3000	0.11%	0.011%
55	18.551	2626	2629	2633	rVB6	6833	7308	0.26%	0.026%
56	19.222	2739	2743	2747	rBV	23231	30109	1.06%	0.108%
57	19.298	2753	2756	2761	rVB2	16529	21688	0.76%	0.078%
58	19.392	2768	2772	2778	rBV2	40837	59892	2.11%	0.215%
59	19.522	2792	2794	2799	rVB5	10784	11827	0.42%	0.042%
60	19.657	2811	2817	2825	rBV	2009665	2689058	94.66%	9.645%
61	21.427	3113	3118	3126	rBV	897258	1218993	42.91%	4.372%
62	23.763	3508	3515	3524	rVB2	1418292	2840718	100.00%	10.189%
63	23.927	3537	3543	3551	rVB	631374	1297241	45.67%	4.653%




Sum of corrected areas: 27878943

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018090.D
Acq On : 12 Nov 2023 05:21
Operator : MA/JU
Sample : 05082-01
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

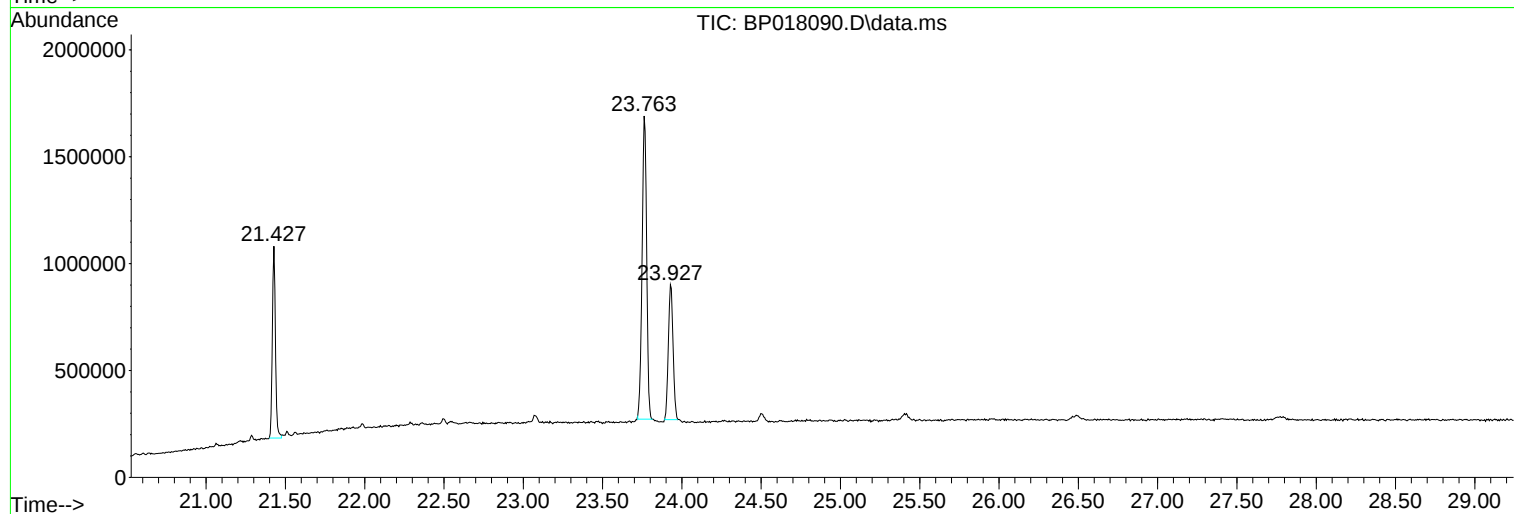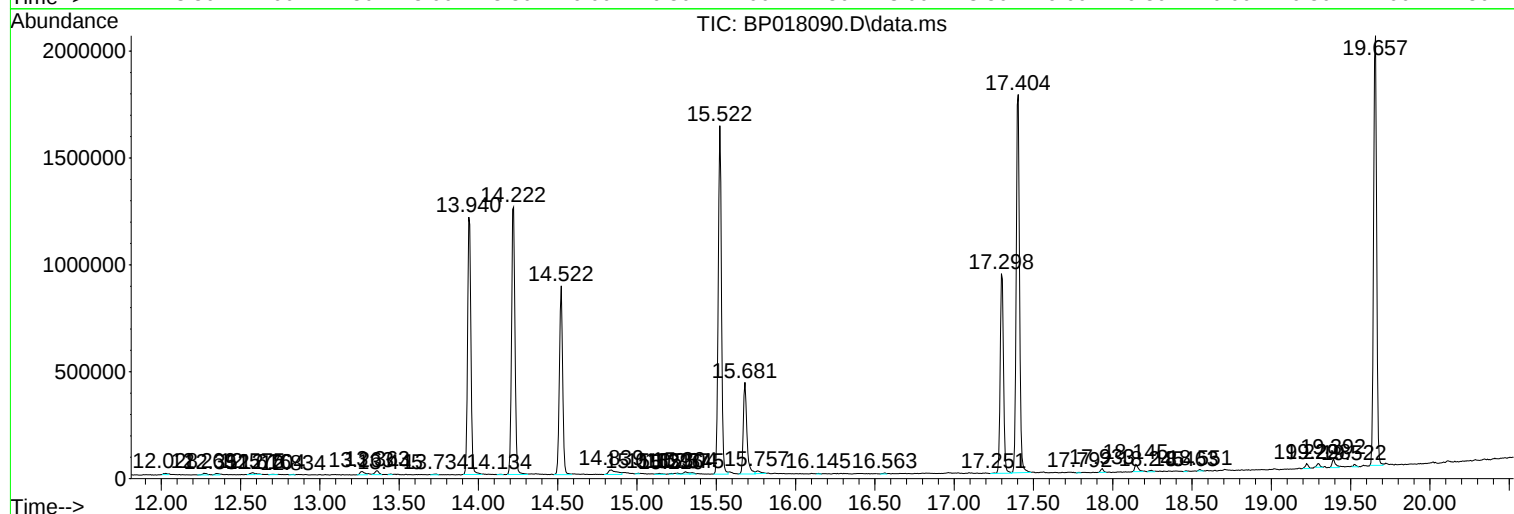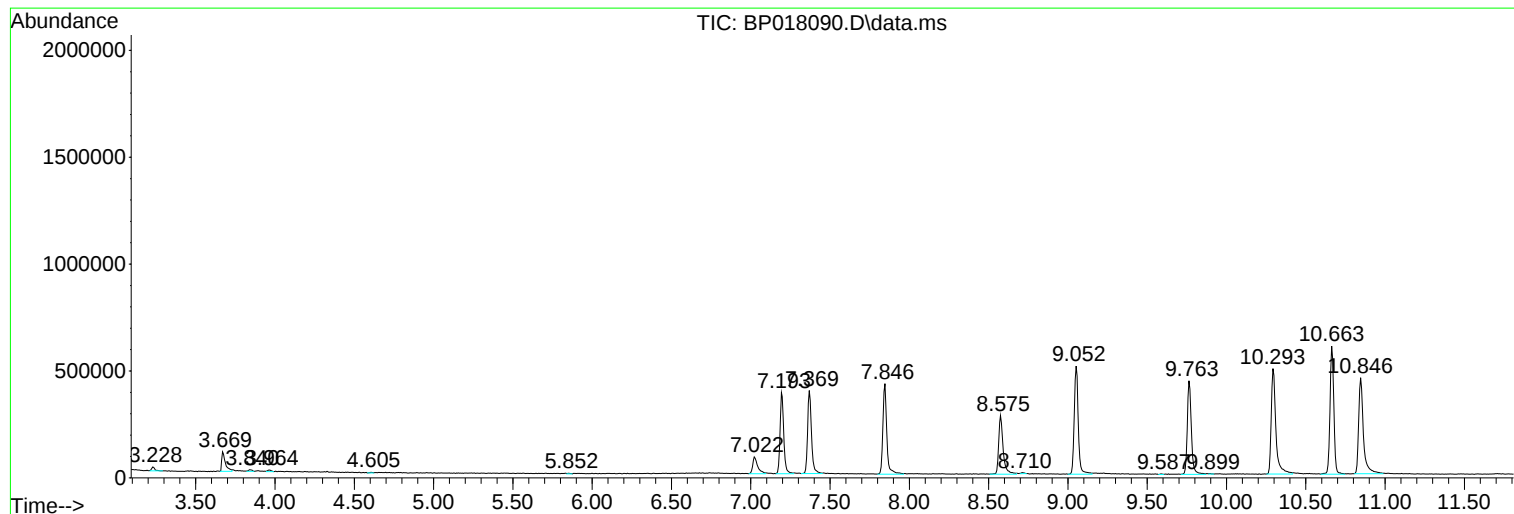

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018090.D
Acq On : 12 Nov 2023 05:21
Operator : MA/JU
Sample : 05082-01
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018090.D
Acq On : 12 Nov 2023 05:21
Operator : MA/JU
Sample : 05082-01
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------