

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018096.D
 Acq On : 12 Nov 2023 09:51
 Operator : MA/JU
 Sample : PB156817BL
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK817

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	33	rVB	35015	47665	1.71%	0.150%
2	3.664	94	98	116	rBV	376499	636885	22.88%	2.001%
3	3.964	145	149	154	rVB3	5816	9286	0.33%	0.029%
4	4.105	169	173	177	rVB7	3672	5927	0.21%	0.019%
5	5.446	397	401	402	rBV4	2311	3067	0.11%	0.010%
6	7.017	661	668	683	rBV	511834	926688	33.28%	2.912%
7	7.193	692	698	709	rBV	421886	657766	23.63%	2.067%
8	7.364	721	727	749	rVB	558382	950020	34.12%	2.986%
9	7.846	801	809	821	rBV	413366	674539	24.23%	2.120%
10	8.569	926	932	952	rBV	679655	1206561	43.34%	3.792%
11	9.052	1006	1014	1026	rBV	566903	969432	34.82%	3.047%
12	9.763	1128	1135	1152	rBV	526856	911177	32.73%	2.863%
13	10.205	1207	1210	1213	rVB5	2496	3603	0.13%	0.011%
14	10.293	1216	1225	1251	rBV	634762	1299693	46.68%	4.084%
15	10.663	1279	1288	1296	rBV	601301	991866	35.63%	3.117%
16	10.846	1309	1319	1337	rBV	609202	1236443	44.41%	3.886%
17	12.287	1560	1564	1570	rBV6	6040	13280	0.48%	0.042%
18	12.987	1679	1683	1686	rVB6	2581	3355	0.12%	0.011%
19	13.363	1741	1747	1752	rBV6	6434	11786	0.42%	0.037%
20	13.487	1764	1768	1772	rVB6	3140	4643	0.17%	0.015%
21	13.628	1788	1792	1794	rBV5	3481	4450	0.16%	0.014%
22	13.728	1804	1809	1812	rVB7	3319	4537	0.16%	0.014%
23	13.940	1837	1845	1859	rBV	1376677	1987618	71.39%	6.246%
24	14.216	1885	1892	1906	rBV	1495333	2173289	78.06%	6.830%
25	14.516	1937	1943	1951	rBV	937377	1392487	50.01%	4.376%
26	14.793	1982	1990	2011	rBV2	184777	591074	21.23%	1.858%
27	15.228	2062	2064	2070	rVB7	2890	4959	0.18%	0.016%
28	15.340	2081	2083	2088	rVB6	2606	3181	0.11%	0.010%
29	15.522	2107	2114	2131	rBV	1935508	2665754	95.75%	8.377%
30	15.681	2134	2141	2152	rBV	308856	511669	18.38%	1.608%
31	15.757	2152	2154	2160	rVB7	12086	18695	0.67%	0.059%
32	15.904	2177	2179	2183	rVB5	2777	3792	0.14%	0.012%
33	16.316	2244	2249	2251	rVB6	2664	3026	0.11%	0.010%
34	16.887	2343	2346	2349	rBV5	2390	4194	0.15%	0.013%
35	16.963	2355	2359	2361	rBV4	2799	3260	0.12%	0.010%
36	17.187	2394	2397	2400	rVB5	2365	3244	0.12%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018096.D
 Acq On : 12 Nov 2023 09:51
 Operator : MA/JU
 Sample : PB156817BL
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK817

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	17.216	2400	2402	2405	rBV4	2247	2838	0.10%	0.009%
38	17.298	2409	2416	2425	rBV	1171166	1627480	58.46%	5.114%
39	17.398	2427	2433	2444	rBV	1866461	2729557	98.04%	8.578%
40	17.634	2470	2473	2481	rVB9	2117	4488	0.16%	0.014%
41	17.728	2486	2489	2490	rBV3	2249	2835	0.10%	0.009%
42	18.151	2558	2561	2562	rBV3	2529	3158	0.11%	0.010%
43	18.369	2596	2598	2602	rBV5	2422	3021	0.11%	0.009%
44	19.222	2740	2743	2747	rBV5	19478	27414	0.98%	0.086%
45	19.298	2752	2756	2759	rBV	19454	24619	0.88%	0.077%
46	19.657	2810	2817	2832	rBV	2037797	2784157	100.00%	8.749%
47	21.428	3113	3118	3128	rBV	903094	1243197	44.65%	3.907%
48	23.763	3507	3515	3527	rVB2	1071458	2205834	79.23%	6.932%
49	23.927	3537	3543	3558	rVB	567097	1223396	43.94%	3.845%




Sum of corrected areas: 31820905

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018096.D
Acq On : 12 Nov 2023 09:51
Operator : MA/JU
Sample : PB156817BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK817

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

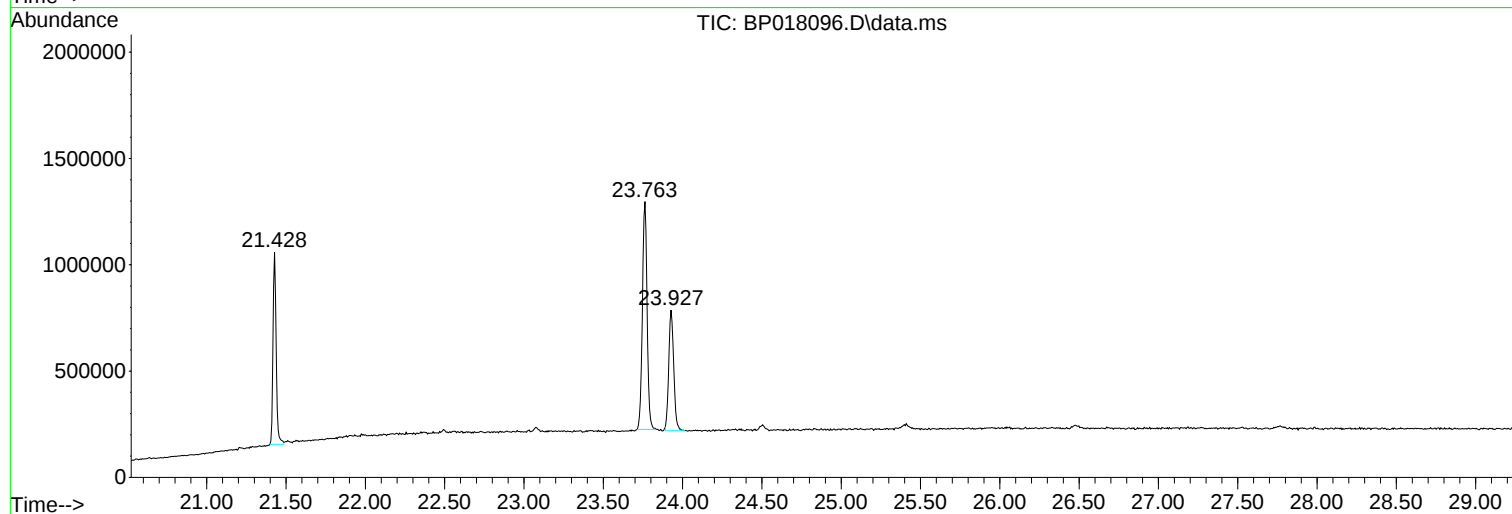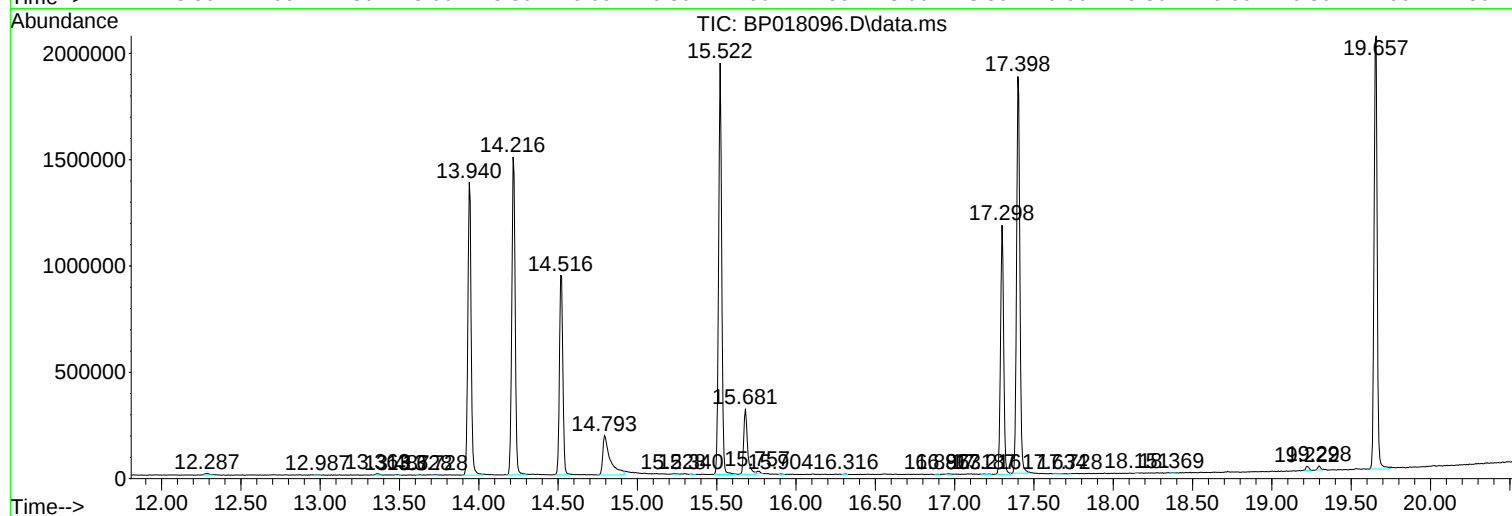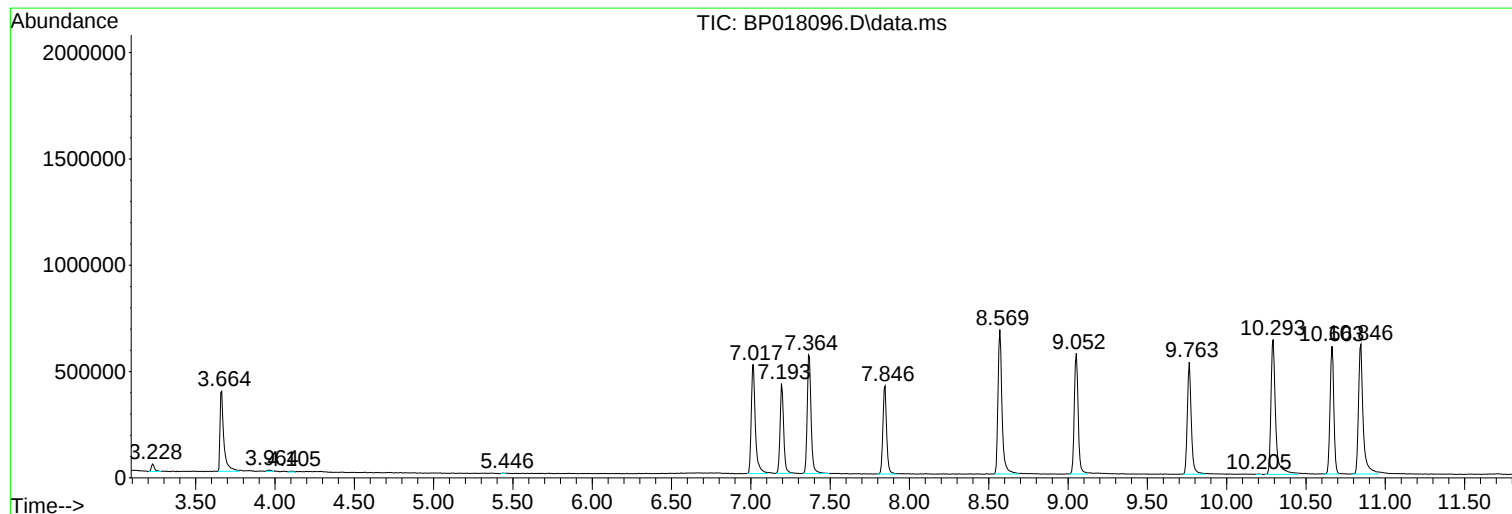

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018096.D
Acq On : 12 Nov 2023 09:51
Operator : MA/JU
Sample : PB156817BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK817

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018096.D
Acq On : 12 Nov 2023 09:51
Operator : MA/JU
Sample : PB156817BL
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK817

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------