

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018097.D
 Acq On : 12 Nov 2023 10:25
 Operator : MA/JU
 Sample : PB156819BL
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK819

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	33	rVB	33771	44936	1.99%	0.172%
2	3.658	94	97	112	rBV	369873	572923	25.36%	2.188%
3	3.964	146	149	152	rBV3	5732	6494	0.29%	0.025%
4	5.164	351	353	355	rBV2	2261	2503	0.11%	0.010%
5	5.840	467	468	472	rBV3	1738	2422	0.11%	0.009%
6	5.922	477	482	484	rBV6	1417	2666	0.12%	0.010%
7	6.069	501	507	509	rBV7	1429	2640	0.12%	0.010%
8	6.146	519	520	527	rVB6	1649	2355	0.10%	0.009%
9	6.263	536	540	542	rBV6	2192	3239	0.14%	0.012%
10	6.352	548	555	556	rBV7	2165	4576	0.20%	0.017%
11	6.834	634	637	639	rVB4	3109	3075	0.14%	0.012%
12	7.010	659	667	685	rBV	450323	833431	36.89%	3.183%
13	7.193	692	698	712	rBV	380061	593942	26.29%	2.268%
14	7.363	721	727	744	rBV	508195	855540	37.87%	3.267%
15	7.675	779	780	785	rBV4	1915	2262	0.10%	0.009%
16	7.846	802	809	821	rVB	366766	602523	26.67%	2.301%
17	8.316	886	889	894	rVV6	1948	3423	0.15%	0.013%
18	8.569	923	932	952	rBV	588481	1040245	46.05%	3.973%
19	8.746	959	962	965	rVB4	2229	2786	0.12%	0.011%
20	9.052	1006	1014	1028	rBV	493004	852049	37.72%	3.254%
21	9.387	1067	1071	1075	rVB7	1544	2955	0.13%	0.011%
22	9.416	1075	1076	1081	rBV5	1513	2302	0.10%	0.009%
23	9.510	1089	1092	1097	rVB7	1608	2860	0.13%	0.011%
24	9.763	1128	1135	1146	rBV	445242	773997	34.26%	2.956%
25	10.204	1204	1210	1212	rVB6	1862	2837	0.13%	0.011%
26	10.293	1218	1225	1245	rBV	524224	1054766	46.69%	4.028%
27	10.663	1280	1288	1300	rBV	522684	861326	38.13%	3.290%
28	10.846	1312	1319	1337	rVV	492552	1009808	44.70%	3.857%
29	11.287	1392	1394	1399	rVB5	2316	2356	0.10%	0.009%
30	11.687	1453	1462	1463	rBV7	2764	6607	0.29%	0.025%
31	11.710	1463	1466	1471	rVV6	3382	6920	0.31%	0.026%
32	11.757	1471	1474	1479	rVB7	1534	2639	0.12%	0.010%
33	12.181	1541	1546	1549	rBV7	1462	2577	0.11%	0.010%
34	12.287	1559	1564	1573	rVB7	4767	12078	0.53%	0.046%
35	13.357	1741	1746	1752	rBV6	10191	15394	0.68%	0.059%
36	13.487	1766	1768	1773	rBV6	2188	3716	0.16%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018097.D
 Acq On : 12 Nov 2023 10:25
 Operator : MA/JU
 Sample : PB156819BL
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK819

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	13.722	1807	1808	1814	rVB6	2453	3163	0.14%	0.012%
38	13.940	1838	1845	1857	rBV	1030229	1507570	66.74%	5.758%
39	14.128	1875	1877	1881	rVB5	1885	2532	0.11%	0.010%
40	14.216	1885	1892	1903	rBV	1134358	1708637	75.64%	6.526%
41	14.522	1937	1944	1958	rBV	715495	1085059	48.03%	4.144%
42	14.798	1984	1991	2017	rBV2	139728	486687	21.54%	1.859%
43	15.034	2029	2031	2035	rVB5	2940	3887	0.17%	0.015%
44	15.245	2060	2067	2068	rBV7	3272	5469	0.24%	0.021%
45	15.292	2073	2075	2078	rBV4	2197	2829	0.13%	0.011%
46	15.522	2107	2114	2124	rBV	1381271	1991770	88.17%	7.607%
47	15.681	2135	2141	2152	rBV	266404	451123	19.97%	1.723%
48	15.763	2152	2155	2162	rVV9	11002	21722	0.96%	0.083%
49	15.816	2162	2164	2167	rVB4	2746	2374	0.11%	0.009%
50	16.257	2236	2239	2244	rVB7	2441	2607	0.12%	0.010%
51	16.304	2244	2247	2249	rBV4	2391	3196	0.14%	0.012%
52	16.557	2284	2290	2292	rBV7	3641	4999	0.22%	0.019%
53	16.722	2317	2318	2322	rVB4	3076	2920	0.13%	0.011%
54	16.951	2354	2357	2359	rBV4	1878	2393	0.11%	0.009%
55	17.098	2379	2382	2387	rVB7	2840	4405	0.19%	0.017%
56	17.163	2391	2393	2396	rBV4	1832	2715	0.12%	0.010%
57	17.298	2410	2416	2427	rBV	788753	1119545	49.56%	4.276%
58	17.404	2427	2434	2448	rVV	1313708	1958773	86.71%	7.481%
59	17.804	2498	2502	2507	rBV8	2317	3540	0.16%	0.014%
60	18.275	2580	2582	2584	rBV3	1969	2462	0.11%	0.009%
61	18.551	2627	2629	2632	rBV3	2421	2427	0.11%	0.009%
62	18.710	2650	2656	2658	rBV7	3037	6016	0.27%	0.023%
63	19.227	2740	2744	2748	rVB4	16478	20415	0.90%	0.078%
64	19.298	2753	2756	2761	rVB2	12835	18416	0.82%	0.070%
65	19.651	2811	2816	2826	rBV	1463168	2039382	90.28%	7.789%
66	21.427	3113	3118	3126	rBV	770334	1082140	47.90%	4.133%
67	23.763	3508	3515	3527	rVB2	1118265	2259033	100.00%	8.628%
68	23.927	3537	3543	3553	rVB2	553220	1178599	52.17%	4.501%




Sum of corrected areas: 26183973

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018097.D
Acq On : 12 Nov 2023 10:25
Operator : MA/JU
Sample : PB156819BL
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK819

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

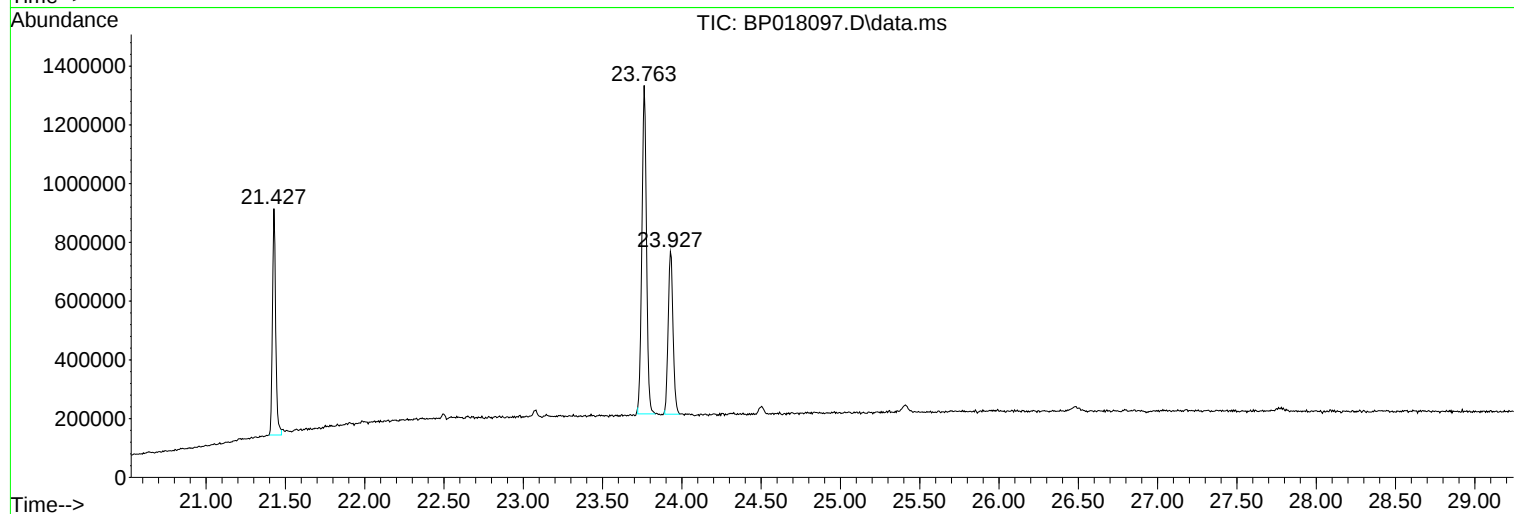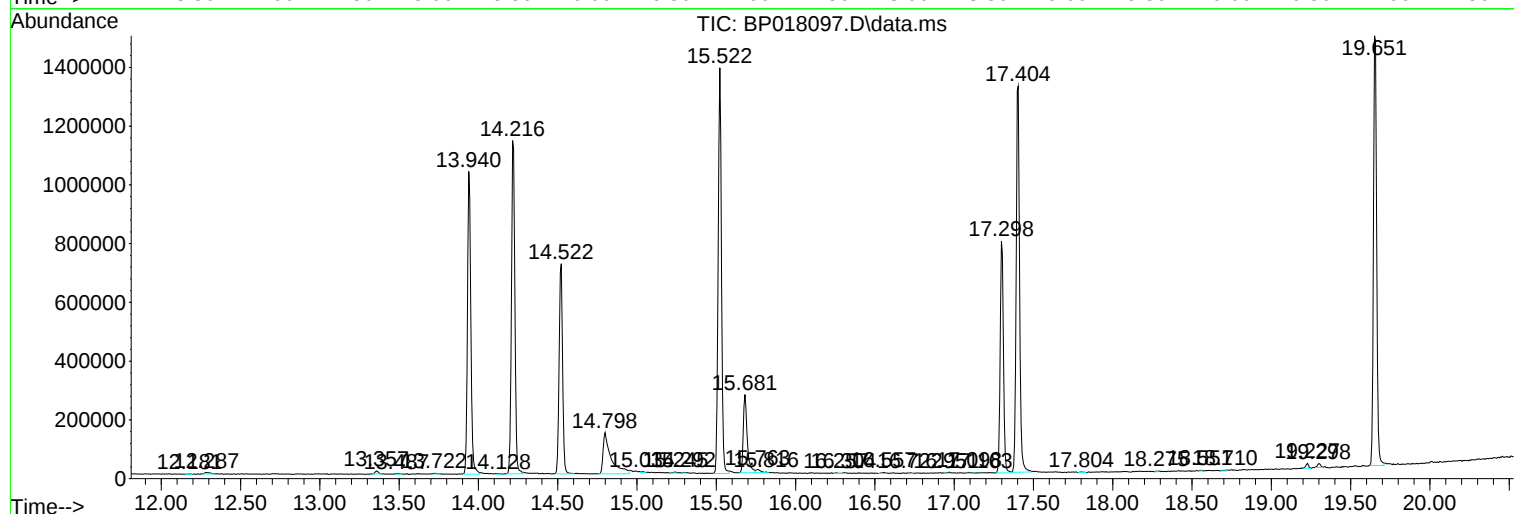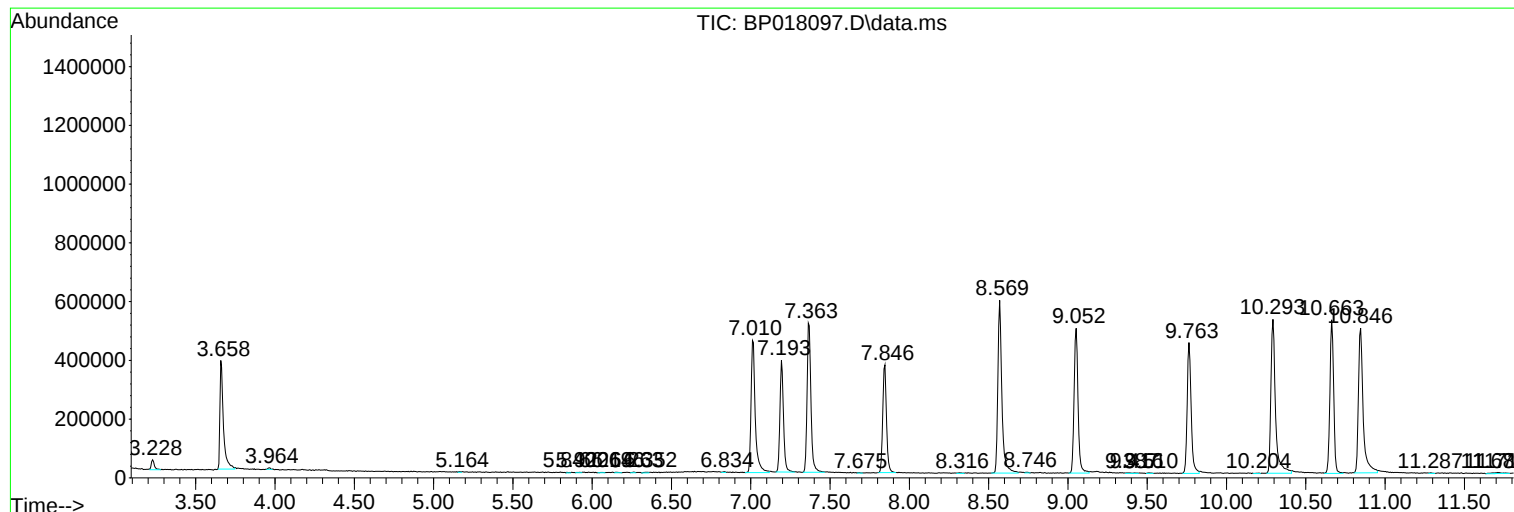

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018097.D
Acq On : 12 Nov 2023 10:25
Operator : MA/JU
Sample : PB156819BL
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK819

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018097.D
Acq On : 12 Nov 2023 10:25
Operator : MA/JU
Sample : PB156819BL
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK819

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------