

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018098.D
 Acq On : 12 Nov 2023 10:59
 Operator : MA/JU
 Sample : 05158-07
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH367

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018098.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	29	rVB3	13618	17278	0.69%	0.085%
2	3.669	96	99	115	rBV	60623	120725	4.84%	0.594%
3	3.964	146	149	152	rVB2	5827	8371	0.34%	0.041%
4	5.634	430	433	436	rVB5	1752	2678	0.11%	0.013%
5	5.669	436	439	440	rBV3	3041	2911	0.12%	0.014%
6	5.763	453	455	459	rVB4	2448	2965	0.12%	0.015%
7	5.916	476	481	483	rBV6	1980	2814	0.11%	0.014%
8	6.275	539	542	545	rVB4	1871	2535	0.10%	0.012%
9	6.458	569	573	575	rBV5	1763	2938	0.12%	0.014%
10	6.587	592	595	597	rBV4	2249	2538	0.10%	0.012%
11	6.887	643	646	652	rVB8	1852	2705	0.11%	0.013%
12	7.022	663	669	684	rBV2	51686	125246	5.02%	0.616%
13	7.193	693	698	713	rBV	231569	378729	15.19%	1.863%
14	7.369	719	728	741	rBV	252174	445350	17.86%	2.190%
15	7.846	801	809	821	rVV	298890	506495	20.31%	2.491%
16	8.575	926	933	948	rBV2	174689	360373	14.45%	1.772%
17	9.052	1003	1014	1027	rBV	314098	556877	22.33%	2.739%
18	9.222	1037	1043	1049	rVB	17525	27938	1.12%	0.137%
19	9.269	1049	1051	1056	rVB6	2392	3535	0.14%	0.017%
20	9.763	1127	1135	1148	rBV	257821	480715	19.28%	2.364%
21	9.851	1148	1150	1155	rVV6	3479	5909	0.24%	0.029%
22	10.299	1217	1226	1243	rBV	287832	646890	25.94%	3.181%
23	10.663	1281	1288	1304	rVB	407251	683634	27.41%	3.362%
24	10.846	1310	1319	1339	rBV	237499	559345	22.43%	2.751%
25	12.281	1560	1563	1564	rBV3	3369	3892	0.16%	0.019%
26	12.351	1570	1575	1576	rBV3	6994	8784	0.35%	0.043%
27	12.734	1637	1640	1644	rVB6	2418	2627	0.11%	0.013%
28	13.257	1727	1729	1733	rVB5	1980	2548	0.10%	0.013%
29	13.357	1742	1746	1752	rBV8	4437	7321	0.29%	0.036%
30	13.498	1766	1770	1772	rVB4	1786	2669	0.11%	0.013%
31	13.687	1798	1802	1804	rVB5	1944	2734	0.11%	0.013%
32	13.734	1804	1810	1813	rBV7	3746	7808	0.31%	0.038%
33	13.939	1839	1845	1857	rBV	732303	1046311	41.96%	5.146%
34	14.216	1886	1892	1908	rBV	731191	1115075	44.72%	5.484%
35	14.522	1936	1944	1957	rBV	572453	847212	33.97%	4.166%
36	14.839	1992	1998	2008	rBV7	15685	54888	2.20%	0.270%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018098.D
 Acq On : 12 Nov 2023 10:59
 Operator : MA/JU
 Sample : 05158-07
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH367

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	14.922	2010	2012	2019	rVB8	5482	9350	0.37%	0.046%
38	15.057	2032	2035	2039	rVB6	1719	2605	0.10%	0.013%
39	15.269	2065	2071	2079	rBV3	8135	17446	0.70%	0.086%
40	15.522	2106	2114	2127	rBV	977880	1432390	57.44%	7.044%
41	15.681	2135	2141	2152	rBV	311842	513088	20.58%	2.523%
42	15.763	2153	2155	2160	rVB5	10615	14158	0.57%	0.070%
43	16.557	2286	2290	2293	rBV6	2549	3623	0.15%	0.018%
44	16.798	2326	2331	2333	rBV2	6431	9778	0.39%	0.048%
45	17.298	2410	2416	2427	rBV	735071	1052133	42.19%	5.174%
46	17.398	2427	2433	2448	rVV	1187042	1749072	70.14%	8.602%
47	17.722	2486	2488	2490	rBV3	2533	2908	0.12%	0.014%
48	17.928	2519	2523	2527	rBV7	4580	8532	0.34%	0.042%
49	18.145	2556	2560	2568	rBV3	44819	75227	3.02%	0.370%
50	18.551	2627	2629	2632	rBV4	3158	3890	0.16%	0.019%
51	19.222	2740	2743	2748	rBV5	13635	19753	0.79%	0.097%
52	19.298	2752	2756	2760	rVB	16125	23296	0.93%	0.115%
53	19.392	2768	2772	2778	rBV5	26692	44349	1.78%	0.218%
54	19.651	2811	2816	2826	rBV	1628615	2175865	87.25%	10.700%
55	21.427	3113	3118	3126	rBV	953097	1245059	49.93%	6.123%
56	23.763	3507	3515	3528	rVB2	1224842	2493721	100.00%	12.264%
57	23.927	3536	3543	3557	rVB	652876	1386743	55.61%	6.820%




Sum of corrected areas: 20334349

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018098.D
Acq On : 12 Nov 2023 10:59
Operator : MA/JU
Sample : 05158-07
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH367

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

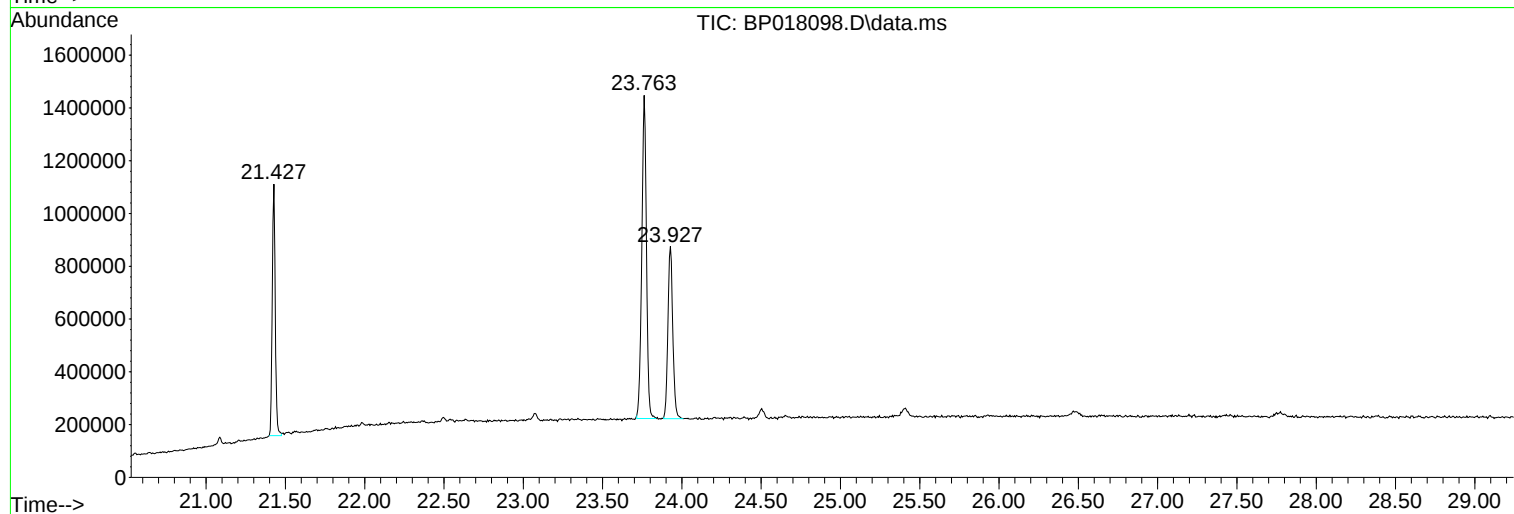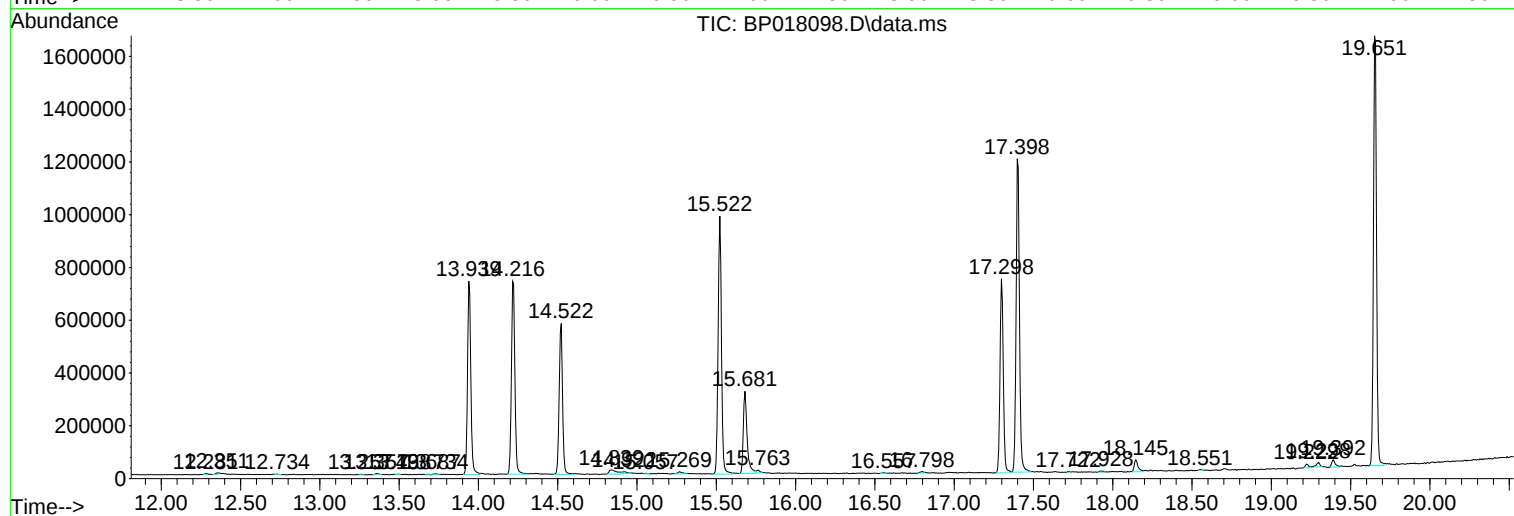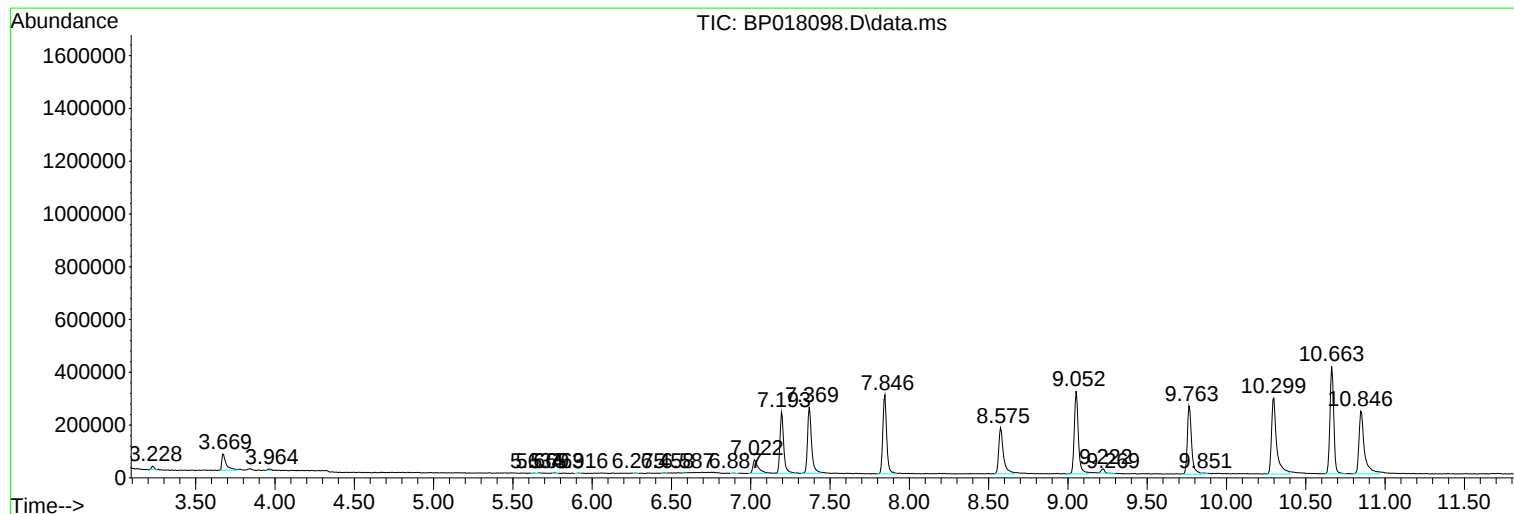

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018098.D
Acq On : 12 Nov 2023 10:59
Operator : MA/JU
Sample : 05158-07
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH367

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018098.D
Acq On : 12 Nov 2023 10:59
Operator : MA/JU
Sample : 05158-07
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH367

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc