

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018099.D
 Acq On : 12 Nov 2023 11:33
 Operator : MA/JU
 Sample : 05158-08
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	27	rBV	12274	13662	0.44%	0.057%
2	3.264	27	30	34	rVB2	8009	9604	0.31%	0.040%
3	3.670	96	99	115	rBV	56124	110795	3.54%	0.463%
4	3.905	136	139	142	rBV4	3083	4982	0.16%	0.021%
5	3.958	146	148	152	rBV4	4401	6076	0.19%	0.025%
6	5.499	406	410	413	rBV5	2433	3840	0.12%	0.016%
7	5.911	474	480	485	rBV8	5866	11098	0.35%	0.046%
8	6.887	642	646	648	rBV5	2485	3829	0.12%	0.016%
9	7.022	663	669	682	rBV	59382	136681	4.37%	0.571%
10	7.193	691	698	711	rBV	308714	496126	15.85%	2.073%
11	7.369	721	728	744	rBV	324211	557877	17.82%	2.331%
12	7.846	802	809	822	rBV	257255	436361	13.94%	1.824%
13	8.575	926	933	951	rBV	213457	435279	13.91%	1.819%
14	8.716	954	957	964	rVB8	4767	8847	0.28%	0.037%
15	9.052	1006	1014	1030	rBV	406038	726975	23.23%	3.038%
16	9.216	1039	1042	1047	rVB3	10213	16217	0.52%	0.068%
17	9.763	1127	1135	1150	rBV	343329	634913	20.29%	2.653%
18	9.881	1153	1155	1160	rVB6	3135	3306	0.11%	0.014%
19	10.293	1218	1225	1252	rBV	387721	845807	27.02%	3.535%
20	10.663	1281	1288	1302	rVB	351962	590026	18.85%	2.466%
21	10.846	1312	1319	1344	rBV	293246	660023	21.09%	2.758%
22	11.710	1464	1466	1474	rVB9	3157	5021	0.16%	0.021%
23	12.293	1558	1565	1573	rVB9	5653	15233	0.49%	0.064%
24	12.704	1631	1635	1639	rVB7	2463	4411	0.14%	0.018%
25	13.357	1740	1746	1752	rBV6	7249	13935	0.45%	0.058%
26	13.940	1838	1845	1865	rBV	948732	1423554	45.48%	5.949%
27	14.216	1884	1892	1905	rBV	996360	1514117	48.38%	6.327%
28	14.522	1937	1944	1955	rBV	497074	752083	24.03%	3.143%
29	14.610	1955	1959	1965	rVV9	3278	6818	0.22%	0.028%
30	14.663	1965	1968	1975	rVB8	2005	3890	0.12%	0.016%
31	14.840	1992	1998	2006	rBV3	18218	55463	1.77%	0.232%
32	15.522	2107	2114	2129	rBV	1382480	1977008	63.16%	8.262%
33	15.681	2135	2141	2153	rBV	433547	712205	22.75%	2.976%
34	16.245	2233	2237	2242	rVB8	1663	3238	0.10%	0.014%
35	16.557	2286	2290	2292	rBV5	2771	3190	0.10%	0.013%
36	16.963	2356	2359	2364	rVB7	2417	4238	0.14%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018099.D
 Acq On : 12 Nov 2023 11:33
 Operator : MA/JU
 Sample : 05158-08
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH374

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	17.092	2378	2381	2385	rBV5	1891	3368	0.11%	0.014%
38	17.298	2407	2416	2427	rBV	682912	964183	30.81%	4.029%
39	17.398	2427	2433	2448	rVV	1570758	2372257	75.79%	9.914%
40	18.145	2556	2560	2567	rBV4	19773	34780	1.11%	0.145%
41	18.245	2573	2577	2580	rBV6	3426	5085	0.16%	0.021%
42	19.228	2740	2744	2749	rBV5	19748	26216	0.84%	0.110%
43	19.298	2752	2756	2759	rVB	18759	23988	0.77%	0.100%
44	19.392	2769	2772	2777	rVB6	14117	19459	0.62%	0.081%
45	19.651	2811	2816	2826	rBV	2122414	2885201	92.18%	12.057%
46	21.427	3113	3118	3127	rBV	823044	1107514	35.38%	4.628%
47	23.763	3507	3515	3528	rVB2	1489495	3129918	100.00%	13.080%
48	23.927	3536	3543	3554	rBV	525046	1150646	36.76%	4.809%




Sum of corrected areas: 23929343

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018099.D
Acq On : 12 Nov 2023 11:33
Operator : MA/JU
Sample : 05158-08
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH374

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

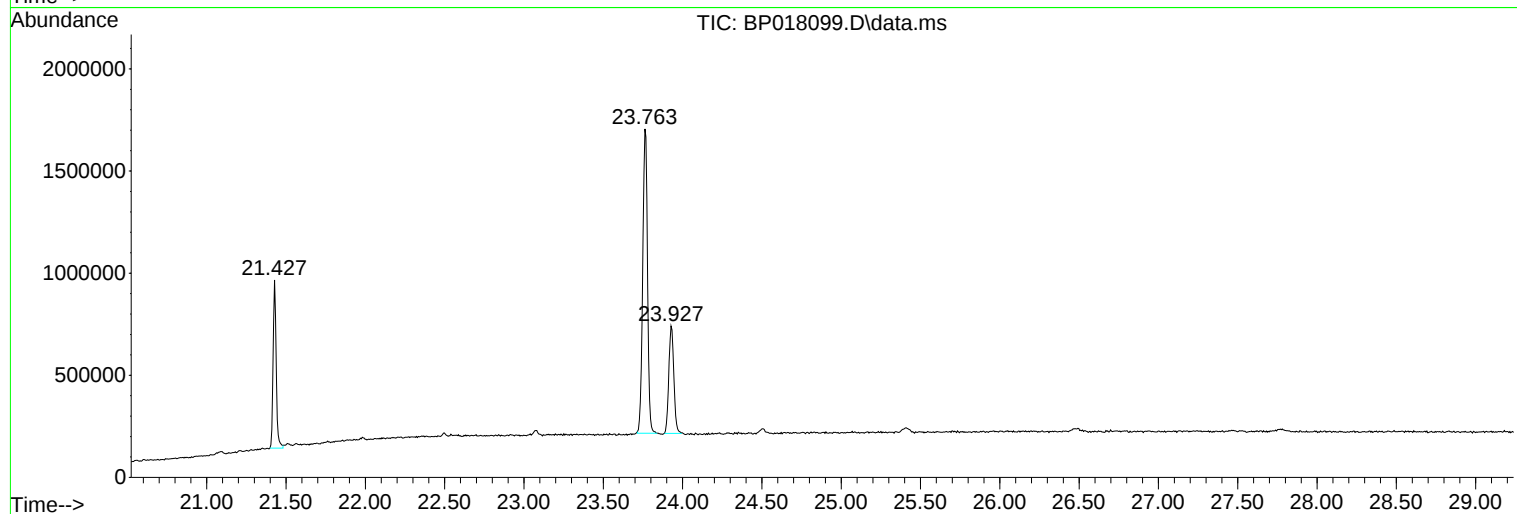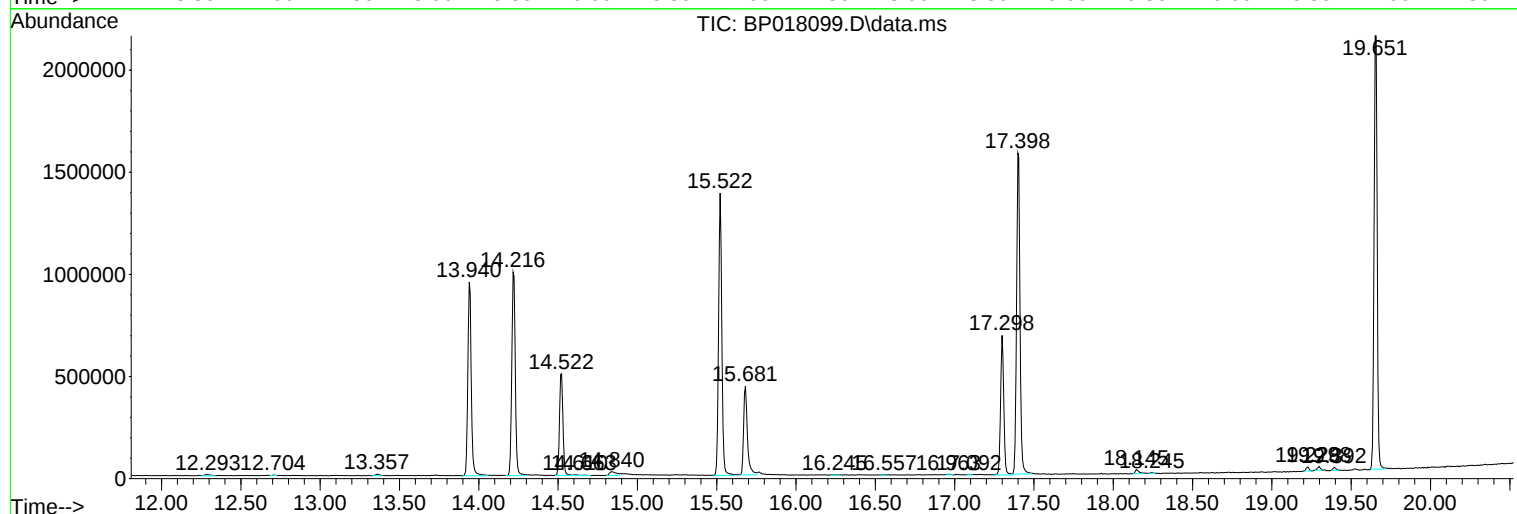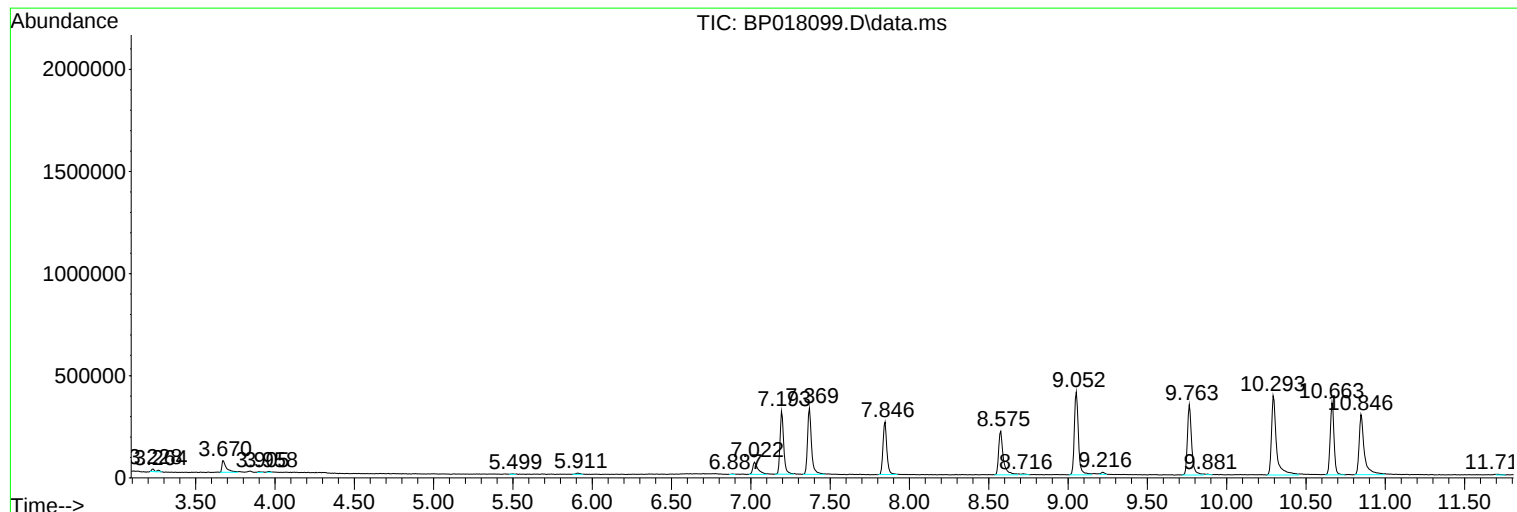

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018099.D
Acq On : 12 Nov 2023 11:33
Operator : MA/JU
Sample : 05158-08
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH374

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018099.D
Acq On : 12 Nov 2023 11:33
Operator : MA/JU
Sample : 05158-08
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH374

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------