

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018106.D
 Acq On : 12 Nov 2023 15:30
 Operator : MA/JU
 Sample : 05158-15
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	27	rBV3	9172	11396	1.02%	0.142%
2	3.681	98	101	110	rVV	23361	45250	4.03%	0.562%
3	4.051	162	164	165	rBV2	2519	2304	0.21%	0.029%
4	4.163	181	183	186	rBV4	2998	3101	0.28%	0.039%
5	5.187	353	357	359	rBV5	2287	2976	0.27%	0.037%
6	5.393	391	392	395	rBV3	1648	1997	0.18%	0.025%
7	5.457	400	403	405	rBV4	2591	2823	0.25%	0.035%
8	5.522	409	414	419	rBV8	1596	3734	0.33%	0.046%
9	5.846	465	469	471	rVB5	1669	2607	0.23%	0.032%
10	5.875	471	474	476	rBV4	1498	2256	0.20%	0.028%
11	5.910	478	480	484	rVB5	1953	2629	0.23%	0.033%
12	5.987	490	493	497	rBV6	1911	3186	0.28%	0.040%
13	6.269	539	541	545	rVB5	2073	1780	0.16%	0.022%
14	6.469	572	575	578	rBV5	1782	2419	0.22%	0.030%
15	6.528	582	585	587	rBV4	2764	3290	0.29%	0.041%
16	6.545	587	588	591	rVB3	2208	1789	0.16%	0.022%
17	6.651	604	606	609	rBV4	2513	2181	0.19%	0.027%
18	7.045	669	673	674	rBV4	4976	4527	0.40%	0.056%
19	7.069	674	677	682	rVB7	4064	6918	0.62%	0.086%
20	7.198	691	699	711	rBV	52069	104437	9.31%	1.297%
21	7.281	711	713	716	rVB4	2722	2242	0.20%	0.028%
22	7.381	722	730	748	rBV	46485	106711	9.51%	1.325%
23	7.657	774	777	780	rVV5	1381	2172	0.19%	0.027%
24	7.722	784	788	791	rVB5	1654	2133	0.19%	0.026%
25	7.845	802	809	821	rBV	265062	453231	40.41%	5.628%
26	7.981	830	832	834	rBV2	1984	1828	0.16%	0.023%
27	8.010	835	837	840	rVB4	2338	2509	0.22%	0.031%
28	8.216	869	872	874	rVV4	1450	2103	0.19%	0.026%
29	8.475	914	916	920	rVB5	1944	2418	0.22%	0.030%
30	8.504	920	921	925	rBV3	1596	2108	0.19%	0.026%
31	8.598	929	937	947	rBV2	25316	65743	5.86%	0.816%
32	8.945	994	996	999	rVB4	2031	1937	0.17%	0.024%
33	9.063	1006	1016	1025	rBV	61977	135332	12.07%	1.680%
34	9.175	1032	1035	1037	rBV4	2419	3041	0.27%	0.038%
35	9.222	1038	1043	1051	rVB	21635	36158	3.22%	0.449%
36	9.516	1091	1093	1095	rVB3	1897	1790	0.16%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018106.D
 Acq On : 12 Nov 2023 15:30
 Operator : MA/JU
 Sample : 05158-15
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	9.675	1117	1120	1124	rBV6	1248	1881	0.17%	0.023%
38	9.775	1128	1137	1148	rBV3	46711	103785	9.25%	1.289%
39	9.857	1148	1151	1157	rVV7	3052	5919	0.53%	0.073%
40	9.904	1157	1159	1163	rVV5	1662	2569	0.23%	0.032%

41	9.939	1163	1165	1168	rVV4	2767	3065	0.27%	0.038%
42	10.322	1224	1230	1241	rVV2	36799	106112	9.46%	1.318%
43	10.492	1258	1259	1263	rVB4	2343	1922	0.17%	0.024%
44	10.545	1265	1268	1272	rBV6	2662	3362	0.30%	0.042%
45	10.663	1280	1288	1297	rBV	343672	606272	54.05%	7.528%

46	10.863	1316	1322	1338	rBV3	46173	128943	11.50%	1.601%
47	11.222	1382	1383	1387	rVB4	1810	1989	0.18%	0.025%
48	11.286	1391	1394	1396	rBV4	2102	2211	0.20%	0.027%
49	11.516	1429	1433	1434	rBV4	1652	1899	0.17%	0.024%
50	11.533	1434	1436	1440	rVB4	2251	1875	0.17%	0.023%

51	11.692	1455	1463	1464	rVV8	2862	6012	0.54%	0.075%
52	11.986	1509	1513	1515	rBV5	2150	2708	0.24%	0.034%
53	12.004	1515	1516	1519	rVV3	2896	1875	0.17%	0.023%
54	12.051	1522	1524	1528	rVV5	1575	2147	0.19%	0.027%
55	12.228	1549	1554	1556	rBV6	2985	5479	0.49%	0.068%

56	12.298	1565	1566	1570	rVB4	1979	1924	0.17%	0.024%
57	12.375	1573	1579	1580	rBV6	5448	8816	0.79%	0.109%
58	12.698	1632	1634	1638	rVV5	2358	2222	0.20%	0.028%
59	12.839	1655	1658	1659	rBV3	1679	1849	0.16%	0.023%
60	12.963	1677	1679	1682	rBV4	2133	2458	0.22%	0.031%

61	13.022	1687	1689	1696	rVV8	1486	2537	0.23%	0.032%
62	13.169	1713	1714	1719	rVB4	2204	2368	0.21%	0.029%
63	13.292	1731	1735	1738	rVB6	1625	2458	0.22%	0.031%
64	13.363	1738	1747	1754	rBV8	9066	21024	1.87%	0.261%
65	13.492	1765	1769	1771	rVB5	2205	2662	0.24%	0.033%

66	13.727	1805	1809	1812	rBV6	2847	2379	0.21%	0.030%
67	13.822	1822	1825	1828	rVB5	1536	1994	0.18%	0.025%
68	13.945	1840	1846	1860	rBV	144002	236431	21.08%	2.936%
69	14.222	1887	1893	1904	rBV2	161317	253790	22.63%	3.151%
70	14.357	1915	1916	1922	rVV6	2464	2319	0.21%	0.029%

71	14.522	1934	1944	1955	rBV	476850	747396	66.63%	9.280%
72	14.598	1955	1957	1960	rVB4	2210	2481	0.22%	0.031%
73	14.686	1970	1972	1975	rVB4	2245	1778	0.16%	0.022%
74	14.898	2006	2008	2012	rVB5	1588	1845	0.16%	0.023%
75	14.939	2012	2015	2017	rBV4	2067	2819	0.25%	0.035%

76	15.133	2045	2048	2052	rVB6	3062	4264	0.38%	0.053%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018106.D
 Acq On : 12 Nov 2023 15:30
 Operator : MA/JU
 Sample : 05158-15
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

77	15.251	2065	2068	2071	rBV5	1795	2549	0.23%	0.032%
78	15.298	2073	2076	2078	rBV4	2007	2452	0.22%	0.030%
79	15.527	2107	2115	2125	rBV	193077	334742	29.84%	4.157%
80	15.616	2128	2130	2133	rVB4	2284	2474	0.22%	0.031%
81	15.710	2140	2146	2151	rBV8	13630	29059	2.59%	0.361%
82	16.380	2257	2260	2261	rVV3	2169	2352	0.21%	0.029%
83	16.398	2261	2263	2266	rVB4	2593	2445	0.22%	0.030%
84	17.080	2375	2379	2381	rBV5	2265	3336	0.30%	0.041%
85	17.304	2410	2417	2429	rBV	538959	873177	77.85%	10.842%
86	17.404	2429	2434	2445	rVB2	208422	347202	30.95%	4.311%
87	17.633	2470	2473	2474	rBV2	2085	2099	0.19%	0.026%
88	17.721	2486	2488	2491	rBV4	1560	1809	0.16%	0.022%
89	17.927	2520	2523	2529	rVB8	4194	6846	0.61%	0.085%
90	18.151	2556	2561	2570	rBV4	22157	41018	3.66%	0.509%
91	18.239	2575	2576	2580	rVV4	2555	2746	0.24%	0.034%
92	18.368	2595	2598	2599	rBV3	2193	2457	0.22%	0.031%
93	18.551	2625	2629	2631	rBV5	4384	5413	0.48%	0.067%
94	18.774	2665	2667	2669	rBV3	2864	2096	0.19%	0.026%
95	19.392	2769	2772	2777	rBV6	12443	18627	1.66%	0.231%
96	19.521	2792	2794	2798	rBV5	7281	7046	0.63%	0.087%
97	19.657	2812	2817	2826	rBV	293708	428761	38.23%	5.324%
98	21.427	3113	3118	3126	rBV	746742	1026195	91.49%	12.742%
99	23.762	3510	3515	3523	rVB	217572	457989	40.83%	5.687%
100	23.927	3537	3543	3556	rVB	522204	1121647	100.00%	13.928%




Sum of corrected areas: 8053432

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018106.D
Acq On : 12 Nov 2023 15:30
Operator : MA/JU
Sample : 05158-15
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH365

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

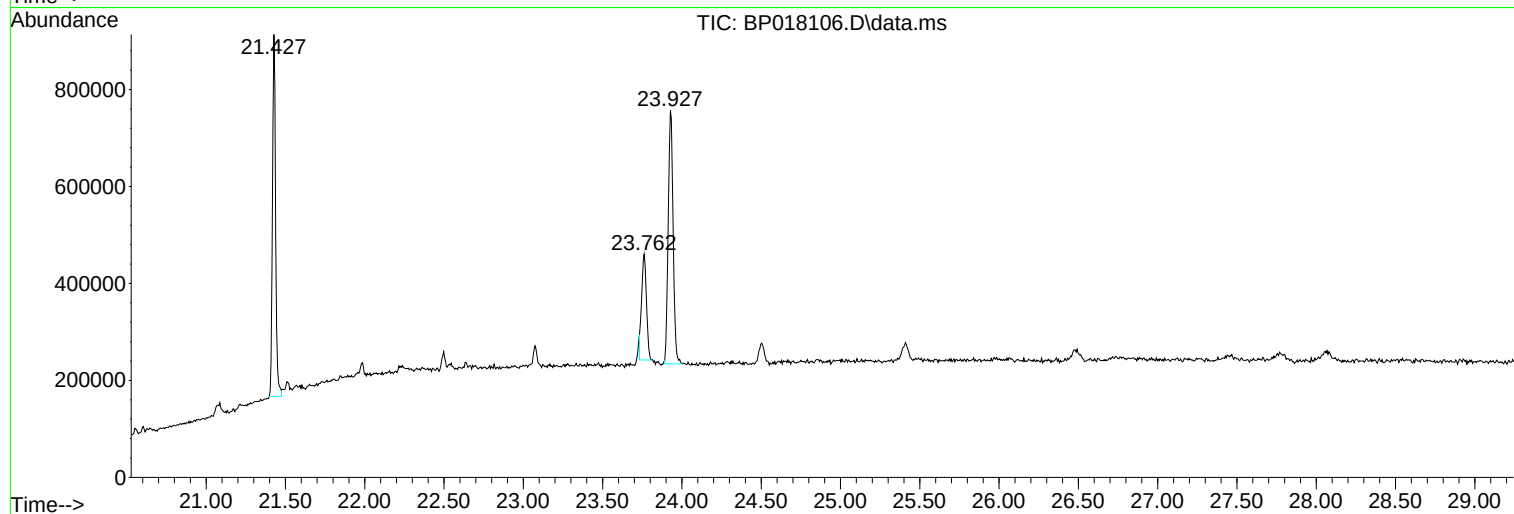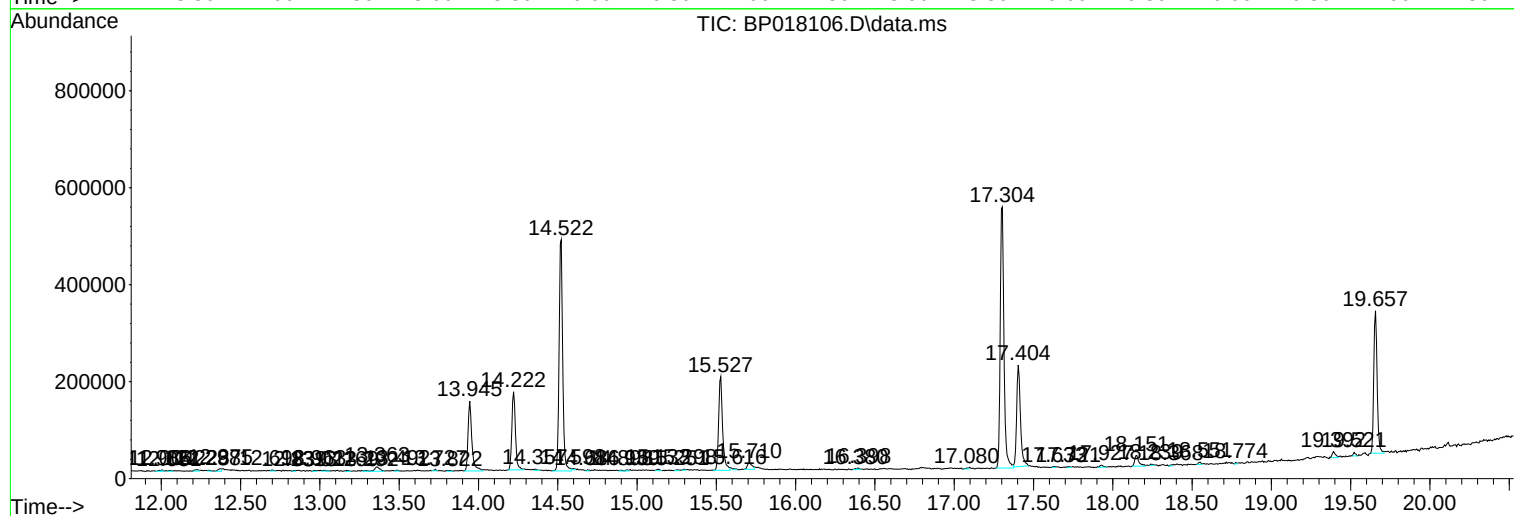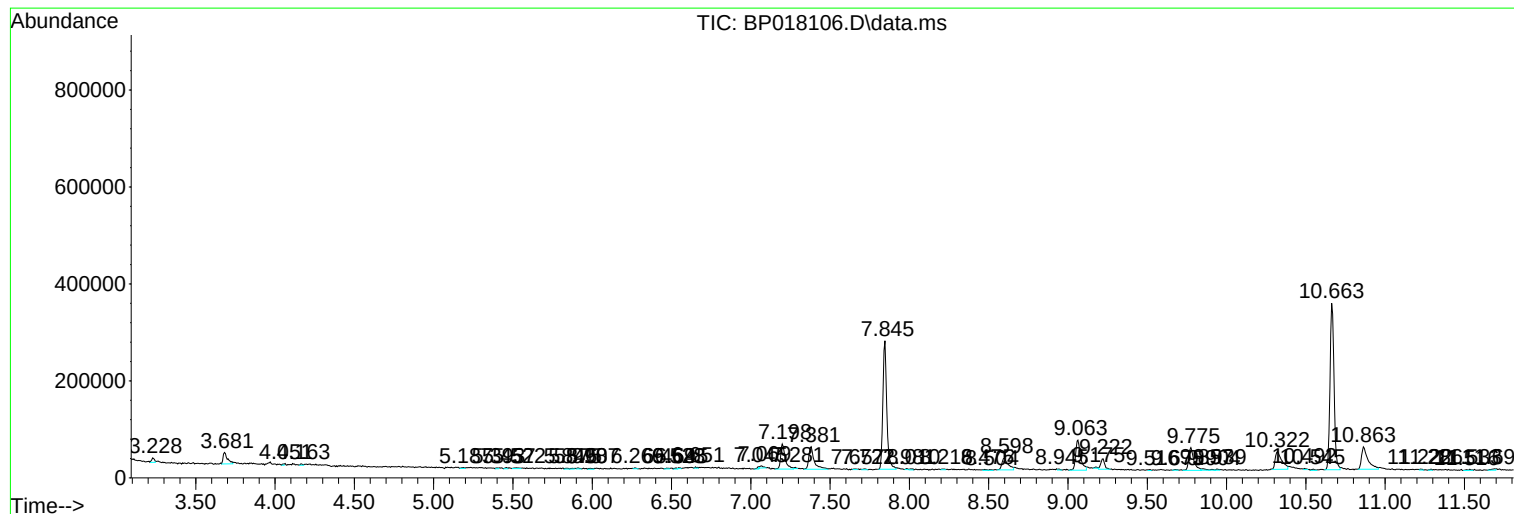

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018106.D
Acq On : 12 Nov 2023 15:30
Operator : MA/JU
Sample : 05158-15
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH365

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018106.D
Acq On : 12 Nov 2023 15:30
Operator : MA/JU
Sample : 05158-15
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH365

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc