

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018109.D
 Acq On : 12 Nov 2023 17:11
 Operator : MA/JU
 Sample : 05082-04
 Misc :
 ALS Vial : 89 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH330

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018109.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	28	rBV	17267	20664	0.67%	0.084%
2	3.264	28	30	35	rVB3	9254	10133	0.33%	0.041%
3	3.340	40	43	49	rVB	18604	24793	0.80%	0.101%
4	3.670	96	99	113	rBV	92806	168794	5.46%	0.686%
5	3.834	123	127	133	rVB6	16254	24653	0.80%	0.100%
6	3.893	133	137	140	rBV5	4162	6071	0.20%	0.025%
7	3.964	146	149	157	rVB4	7188	13086	0.42%	0.053%
8	5.705	441	445	451	rBV8	2858	5788	0.19%	0.024%
9	6.834	634	637	640	rBV5	2397	3238	0.10%	0.013%
10	7.022	661	669	681	rBV3	95809	236574	7.66%	0.962%
11	7.193	692	698	712	rBV	326157	517132	16.74%	2.102%
12	7.369	722	728	743	rBV	354742	614178	19.88%	2.497%
13	7.840	800	808	819	rBV	306178	521856	16.89%	2.122%
14	8.569	926	932	944	rBV	261328	503425	16.30%	2.047%
15	9.052	1006	1014	1023	rBV	414908	723103	23.41%	2.940%
16	9.763	1128	1135	1153	rBV	354863	646018	20.91%	2.626%
17	10.040	1178	1182	1185	rBV5	3545	4977	0.16%	0.020%
18	10.293	1218	1225	1247	rBV	403790	858666	27.80%	3.491%
19	10.663	1281	1288	1299	rBV	420122	694481	22.48%	2.823%
20	10.846	1309	1319	1346	rBV	338677	759693	24.59%	3.089%
21	11.704	1459	1465	1467	rBV7	5806	8768	0.28%	0.036%
22	12.275	1559	1562	1574	rBV7	4671	11204	0.36%	0.046%
23	13.357	1741	1746	1751	rVB5	8363	14199	0.46%	0.058%
24	13.722	1805	1808	1813	rVB6	2297	3780	0.12%	0.015%
25	13.940	1839	1845	1863	rBV	947156	1380932	44.71%	5.614%
26	14.216	1885	1892	1905	rBV2	965663	1468870	47.55%	5.972%
27	14.516	1937	1943	1954	rBV	574577	853118	27.62%	3.468%
28	14.828	1990	1996	2008	rBV3	28640	95871	3.10%	0.390%
29	15.251	2065	2068	2071	rBV5	2064	3548	0.11%	0.014%
30	15.522	2107	2114	2124	rBV	1309639	1875456	60.72%	7.625%
31	15.681	2135	2141	2152	rBV	460656	750717	24.30%	3.052%
32	17.298	2410	2416	2425	rBV	744077	1039558	33.66%	4.226%
33	17.398	2427	2433	2450	rVB	1506614	2234680	72.35%	9.085%
34	17.928	2519	2523	2525	rBV5	3892	5676	0.18%	0.023%
35	18.145	2556	2560	2568	rBV3	37296	59097	1.91%	0.240%
36	18.239	2574	2576	2581	rBV6	3833	3882	0.13%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018109.D
Acq On : 12 Nov 2023 17:11
Operator : MA/JU
Sample : 05082-04
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH330

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

37	18.710	2652	2656	2662	rBV9	5408	9630	0.31%	0.039%
38	19.222	2740	2743	2747	rVB2	18251	21909	0.71%	0.089%
39	19.298	2752	2756	2759	rVB	19883	25439	0.82%	0.103%
40	19.392	2768	2772	2777	rBV6	25507	35642	1.15%	0.145%
41	19.657	2811	2817	2825	rBV	2064632	2751791	89.09%	11.188%
42	21.427	3113	3118	3127	rBV	879612	1205332	39.02%	4.900%
43	23.768	3508	3516	3527	rVB	1513633	3088858	100.00%	12.558%
44	23.933	3537	3544	3555	rVB	622916	1291521	41.81%	5.251%




Sum of corrected areas: 24596801

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018109.D
Acq On : 12 Nov 2023 17:11
Operator : MA/JU
Sample : 05082-04
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH330

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

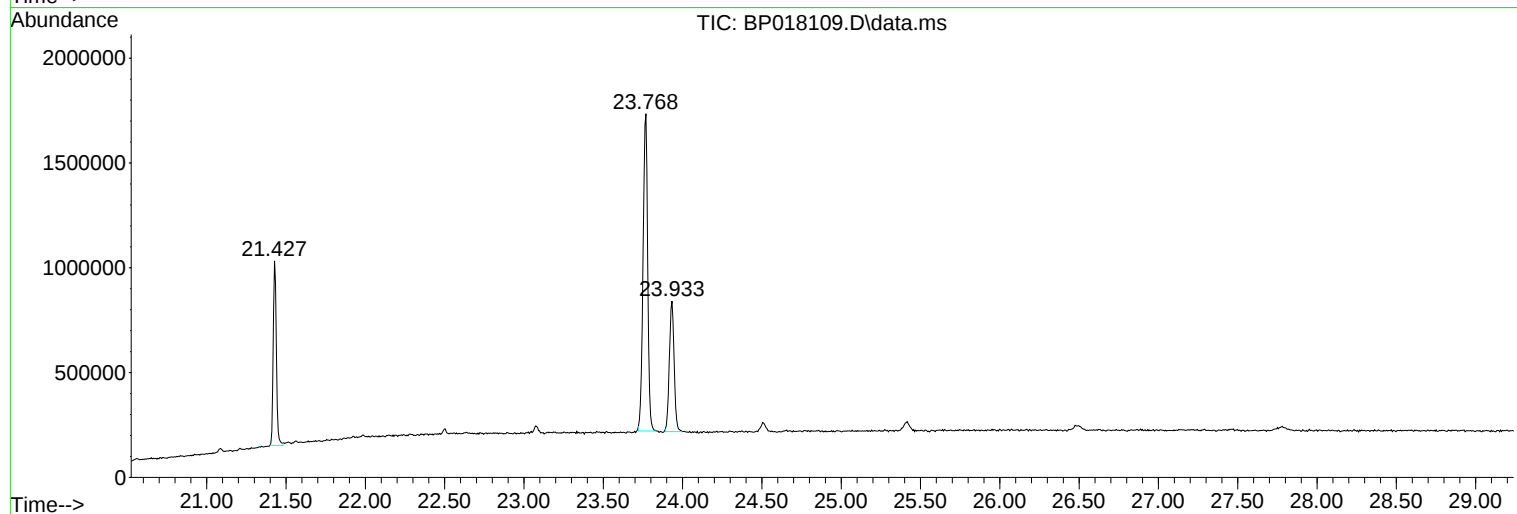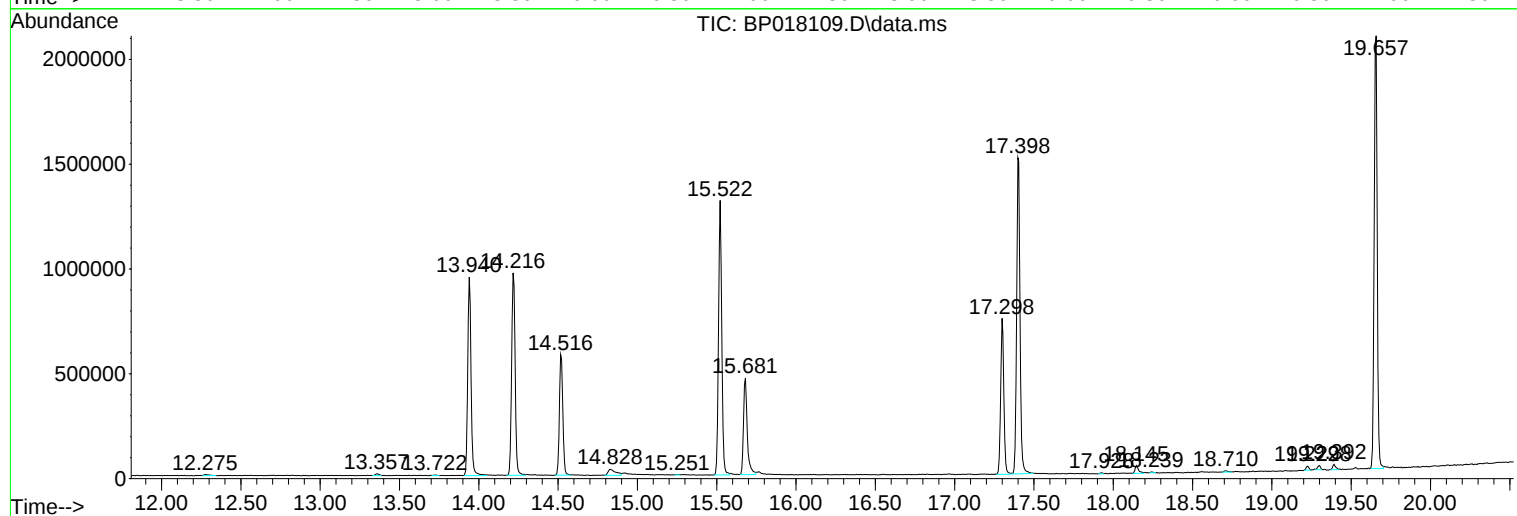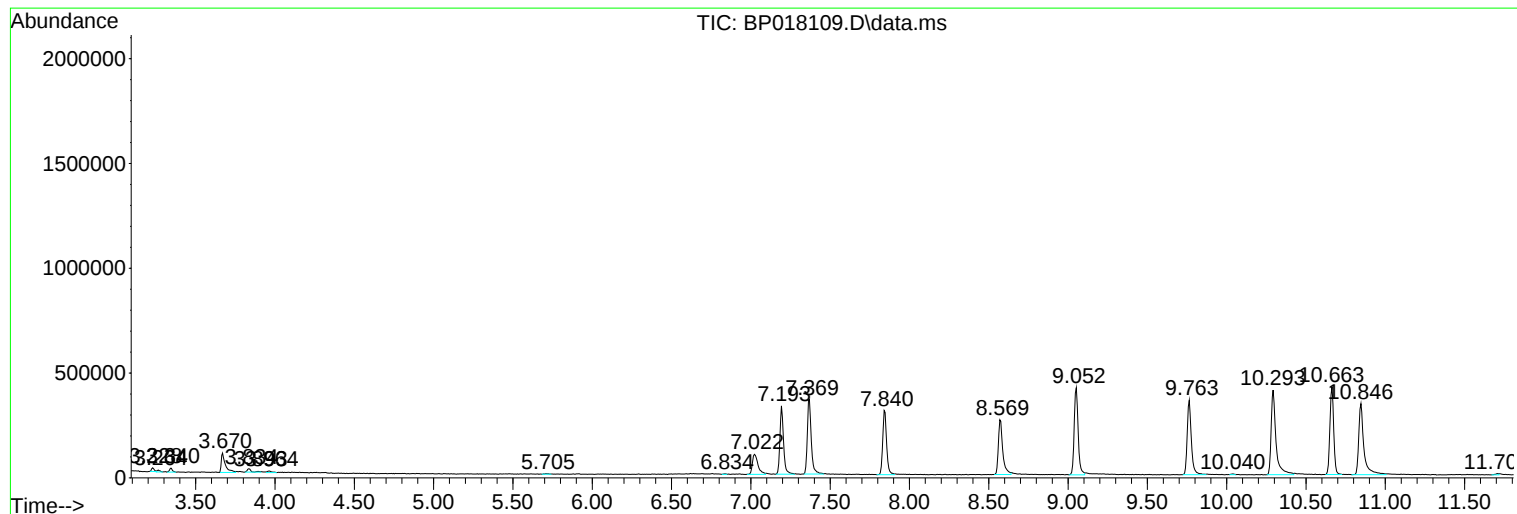

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018109.D
Acq On : 12 Nov 2023 17:11
Operator : MA/JU
Sample : 05082-04
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH330

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018109.D
Acq On : 12 Nov 2023 17:11
Operator : MA/JU
Sample : 05082-04
Misc :
ALS Vial : 89 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH330

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc