

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018110.D
 Acq On : 12 Nov 2023 17:45
 Operator : MA/JU
 Sample : 05082-05
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH331

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	31	rBV	20042	28578	0.88%	0.112%
2	3.669	96	99	110	rBV	77465	132837	4.08%	0.520%
3	3.840	124	128	132	rBV4	8632	12389	0.38%	0.049%
4	3.958	146	148	151	rBV3	4951	5726	0.18%	0.022%
5	7.016	662	668	688	rBV	102439	235992	7.25%	0.925%
6	7.193	691	698	713	rBV	315162	505802	15.55%	1.982%
7	7.369	719	728	744	rBV	347282	613790	18.87%	2.405%
8	7.840	802	808	819	rBV	311431	525703	16.16%	2.060%
9	8.569	925	932	951	rBV	291612	552132	16.97%	2.163%
10	9.051	1007	1014	1022	rBV	403382	710668	21.84%	2.784%
11	9.104	1022	1023	1034	rVB8	17827	29452	0.91%	0.115%
12	9.763	1127	1135	1148	rBV	353194	631353	19.41%	2.474%
13	10.293	1214	1225	1245	rBV	422819	891980	27.42%	3.495%
14	10.663	1279	1288	1298	rBV	411840	703346	21.62%	2.756%
15	10.845	1312	1319	1331	rBV	333856	710849	21.85%	2.785%
16	12.287	1556	1564	1573	rVB8	5602	16855	0.52%	0.066%
17	12.375	1575	1579	1581	rBV5	2597	4209	0.13%	0.016%
18	12.822	1652	1655	1659	rBV6	2431	3643	0.11%	0.014%
19	13.092	1692	1701	1703	rVB9	2493	5031	0.15%	0.020%
20	13.263	1725	1730	1734	rBV7	2144	3827	0.12%	0.015%
21	13.357	1741	1746	1751	rVB7	8437	14146	0.43%	0.055%
22	13.939	1838	1845	1858	rBV	1013565	1429018	43.92%	5.599%
23	14.216	1884	1892	1903	rBV	1011916	1505940	46.29%	5.900%
24	14.516	1935	1943	1955	rBV	586960	865379	26.60%	3.391%
25	14.822	1989	1995	2005	rBV5	38726	130743	4.02%	0.512%
26	15.239	2061	2066	2067	rBV5	4637	5150	0.16%	0.020%
27	15.522	2106	2114	2130	rBV	1400500	1972215	60.62%	7.727%
28	15.675	2134	2140	2152	rBV	512007	807997	24.83%	3.166%
29	15.851	2168	2170	2174	rBV5	2724	4003	0.12%	0.016%
30	16.045	2200	2203	2208	rVB7	2396	3379	0.10%	0.013%
31	16.557	2285	2290	2292	rBV5	3526	5603	0.17%	0.022%
32	17.298	2410	2416	2425	rBV	763342	1063304	32.68%	4.166%
33	17.398	2427	2433	2450	rVB	1563088	2365435	72.71%	9.268%
34	17.927	2519	2523	2525	rBV5	7177	8079	0.25%	0.032%
35	18.145	2556	2560	2567	rBV2	60228	88980	2.73%	0.349%
36	18.233	2573	2575	2580	rVB4	4530	5772	0.18%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018110.D
Acq On : 12 Nov 2023 17:45
Operator : MA/JU
Sample : 05082-05
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH331

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

37	18.704	2652	2655	2660	rBV7	6426	9469	0.29%	0.037%
38	19.069	2713	2717	2722	rVB8	7543	10582	0.33%	0.041%
39	19.221	2740	2743	2747	rVB4	19691	24500	0.75%	0.096%
40	19.298	2752	2756	2761	rVB	19377	29617	0.91%	0.116%
41	19.386	2768	2771	2775	rBV3	33985	44534	1.37%	0.174%
42	19.521	2792	2794	2799	rVB5	7346	8268	0.25%	0.032%
43	19.657	2811	2817	2826	rBV	2206647	2903364	89.24%	11.375%
44	21.427	3113	3118	3126	rBV2	925312	1289233	39.63%	5.051%
45	23.768	3507	3516	3524	rVB2	1595744	3253468	100.00%	12.747%
46	23.927	3537	3543	3554	rVB	632447	1350681	41.52%	5.292%




Sum of corrected areas: 25523021

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018110.D
Acq On : 12 Nov 2023 17:45
Operator : MA/JU
Sample : 05082-05
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH331

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

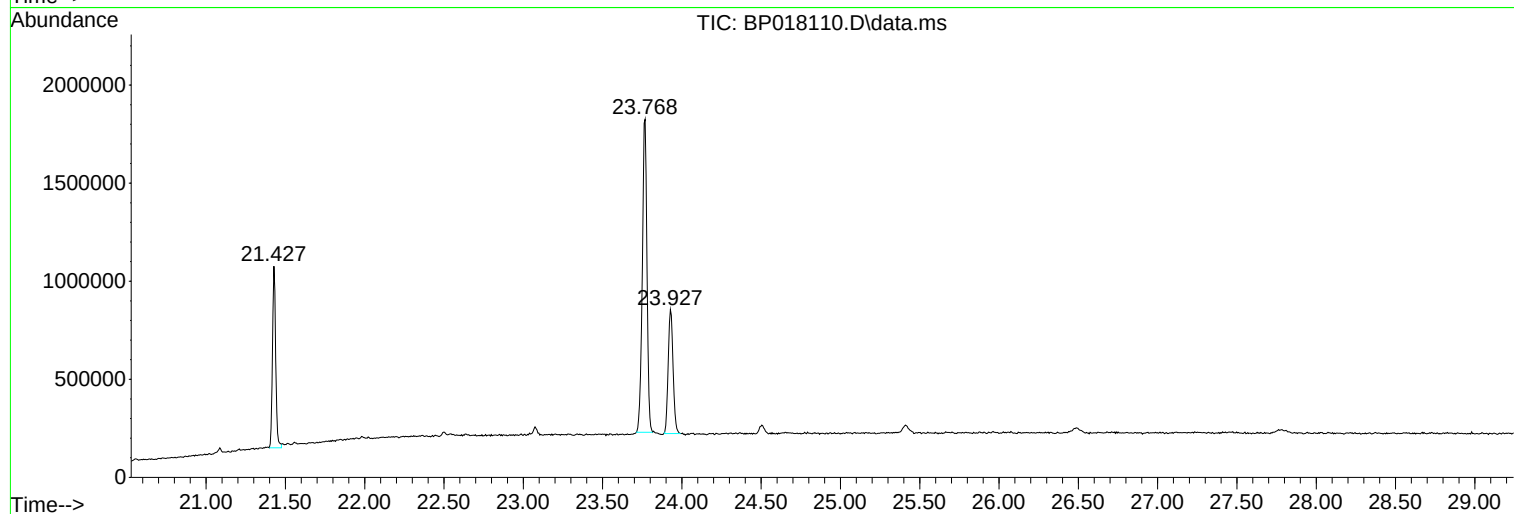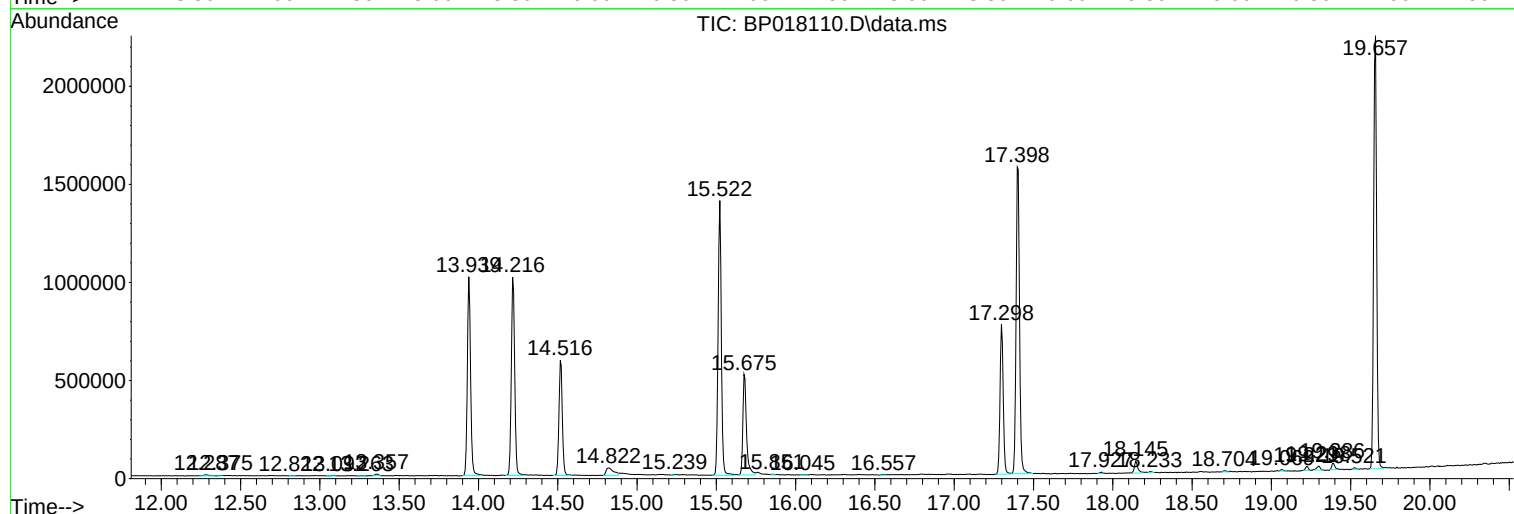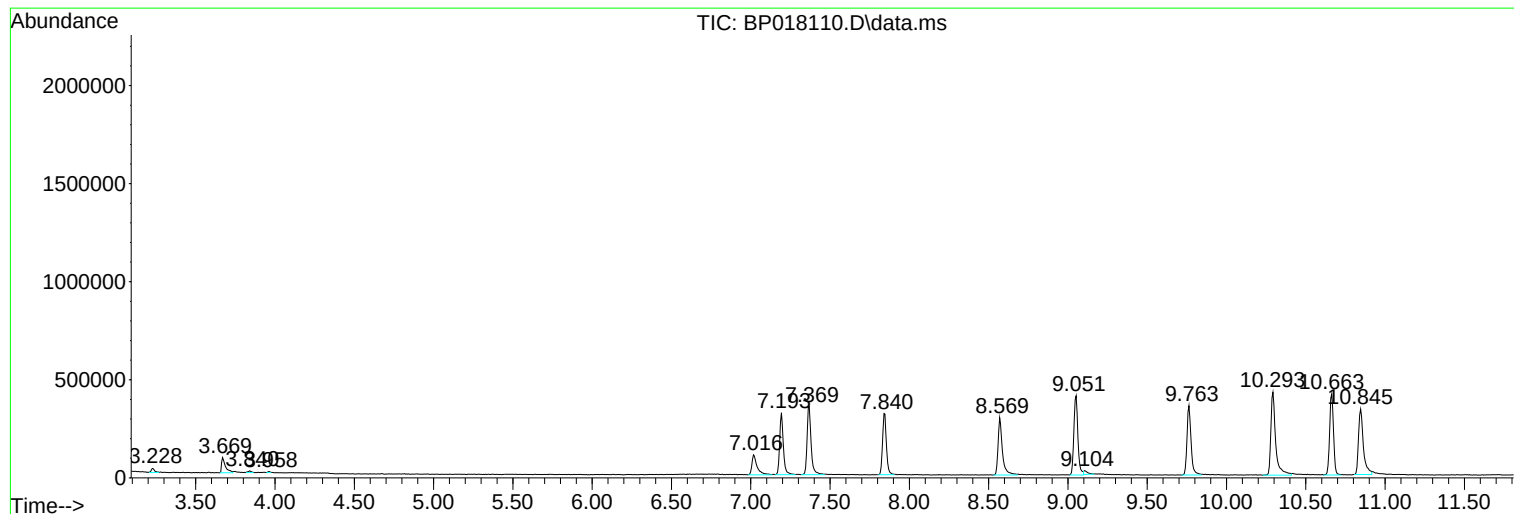

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018110.D
Acq On : 12 Nov 2023 17:45
Operator : MA/JU
Sample : 05082-05
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH331

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018110.D
Acq On : 12 Nov 2023 17:45
Operator : MA/JU
Sample : 05082-05
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH331

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc