

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018115.D
 Acq On : 12 Nov 2023 21:42
 Operator : MA/JU
 Sample : PB156723BL
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK723

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	31	rVB	39014	49894	1.92%	0.170%
2	3.658	94	97	110	rBV	412549	644638	24.81%	2.193%
3	4.952	314	317	321	rBV6	2470	3697	0.14%	0.013%
4	5.193	356	358	361	rBV4	2015	2740	0.11%	0.009%
5	5.511	409	412	415	rBV4	1749	2803	0.11%	0.010%
6	7.011	661	667	688	rVV	543032	971965	37.41%	3.306%
7	7.193	692	698	714	rVB	439435	694357	26.73%	2.362%
8	7.364	719	727	742	rBV	610095	979872	37.72%	3.333%
9	7.840	801	808	822	rBV	299355	504530	19.42%	1.716%
10	8.316	885	889	891	rVB5	3172	3797	0.15%	0.013%
11	8.352	891	895	896	rBV4	2079	2865	0.11%	0.010%
12	8.563	924	931	953	rBV	672179	1235663	47.56%	4.203%
13	9.046	1007	1013	1025	rBV	572360	986311	37.96%	3.355%
14	9.469	1082	1085	1088	rBV5	1633	2818	0.11%	0.010%
15	9.763	1125	1135	1149	rBV	509176	923499	35.55%	3.141%
16	9.869	1151	1153	1157	rVB5	2595	3100	0.12%	0.011%
17	10.287	1217	1224	1243	rBV	635534	1277719	49.18%	4.346%
18	10.663	1280	1288	1300	rBV	425433	734649	28.28%	2.499%
19	10.840	1311	1318	1341	rVV	584810	1201224	46.24%	4.086%
20	11.663	1453	1458	1462	rBV7	1428	2667	0.10%	0.009%
21	12.287	1559	1564	1573	rVV5	7334	17652	0.68%	0.060%
22	13.269	1729	1731	1738	rBV8	1614	3394	0.13%	0.012%
23	13.363	1741	1747	1750	rVB7	5087	8908	0.34%	0.030%
24	13.940	1838	1845	1856	rBV	1351417	1917269	73.80%	6.522%
25	14.216	1885	1892	1911	rBV	1454294	2134753	82.17%	7.261%
26	14.516	1936	1943	1952	rBV	676339	984428	37.89%	3.349%
27	14.793	1982	1990	2019	rBV2	170851	609098	23.44%	2.072%
28	15.228	2061	2064	2069	rVB7	2923	5199	0.20%	0.018%
29	15.522	2107	2114	2129	rBV	1740562	2583703	99.45%	8.789%
30	15.681	2134	2141	2152	rVV	345185	603911	23.25%	2.054%
31	15.757	2152	2154	2171	rVV7	15847	40078	1.54%	0.136%
32	16.304	2244	2247	2250	rBV5	2504	3171	0.12%	0.011%
33	16.563	2285	2291	2293	rVB7	2531	4203	0.16%	0.014%
34	16.957	2352	2358	2361	rBV8	3431	5851	0.23%	0.020%
35	17.092	2379	2381	2386	rVB6	2680	3957	0.15%	0.013%
36	17.298	2409	2416	2427	rBV	751051	1074022	41.34%	3.653%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018115.D
 Acq On : 12 Nov 2023 21:42
 Operator : MA/JU
 Sample : PB156723BL
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK723

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	17.398	2427	2433	2447	rVV2	1759008	2578728	99.26%	8.772%
38	17.628	2468	2472	2477	rBV8	2512	2929	0.11%	0.010%
39	18.175	2561	2565	2567	rBV5	2312	3808	0.15%	0.013%
40	18.422	2605	2607	2609	rBV3	2239	2822	0.11%	0.010%
41	18.992	2702	2704	2705	rBV2	2950	2697	0.10%	0.009%
42	19.222	2739	2743	2748	rBV2	20761	31185	1.20%	0.106%
43	19.298	2752	2756	2760	rVV	17494	24012	0.92%	0.082%
44	19.651	2811	2816	2831	rBV	1923303	2598022	100.00%	8.837%
45	21.427	3113	3118	3128	rBV2	590660	856257	32.96%	2.913%
46	23.763	3508	3515	3528	rVB2	1067324	2218366	85.39%	7.546%
47	23.927	3537	3543	3557	rVB2	363927	851075	32.76%	2.895%




Sum of corrected areas: 29398306

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018115.D
Acq On : 12 Nov 2023 21:42
Operator : MA/JU
Sample : PB156723BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK723

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

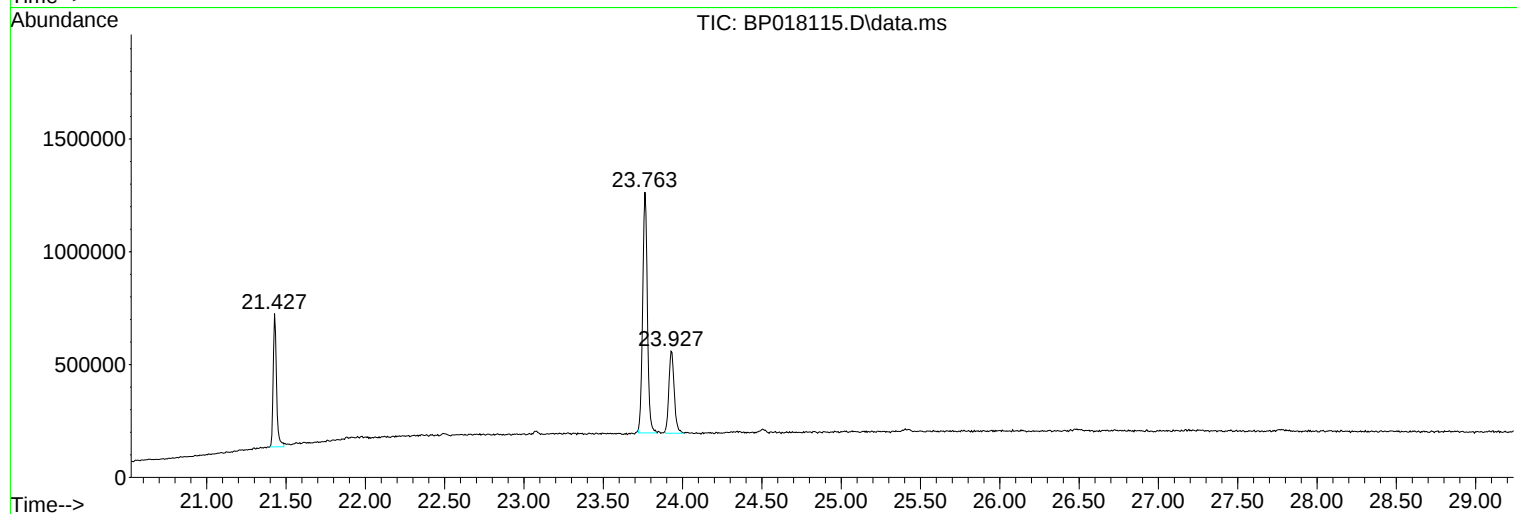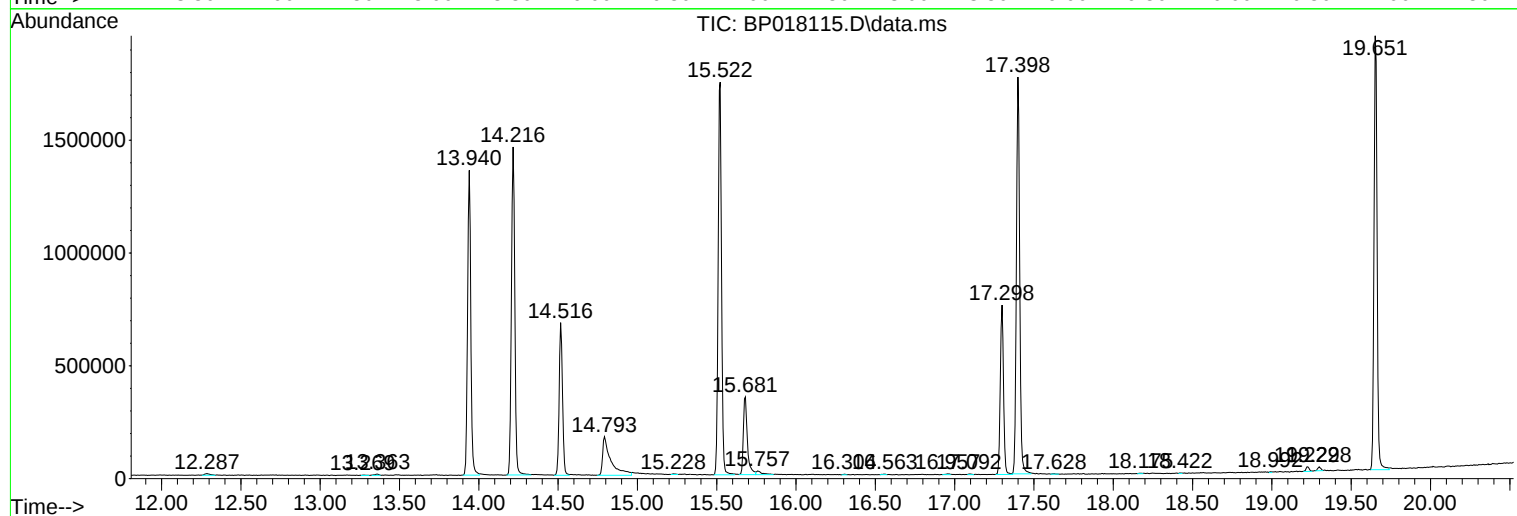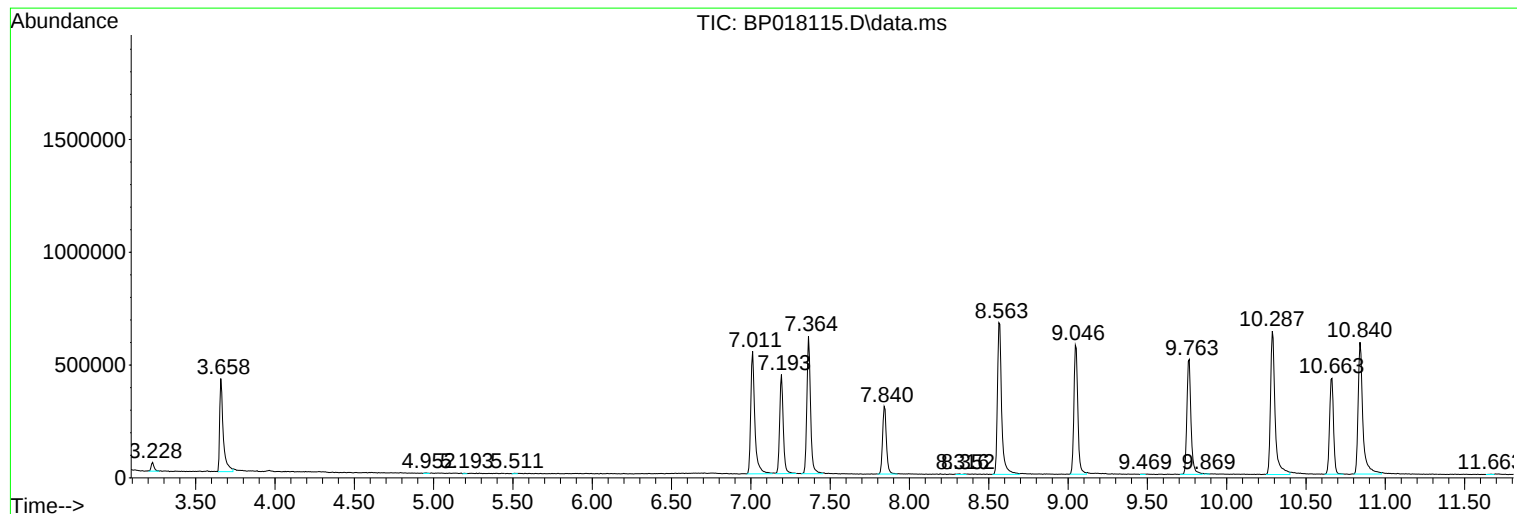

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018115.D
Acq On : 12 Nov 2023 21:42
Operator : MA/JU
Sample : PB156723BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK723

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018115.D
Acq On : 12 Nov 2023 21:42
Operator : MA/JU
Sample : PB156723BL
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK723

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------