

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018116.D
 Acq On : 12 Nov 2023 22:16
 Operator : MA/JU
 Sample : PB156806BL
 Misc :
 ALS Vial : 97 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK806

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	29	rVB	22379	24049	1.36%	0.137%
2	3.664	94	98	117	rBV	239793	410973	23.32%	2.337%
3	4.211	189	191	194	rVB3	3178	2651	0.15%	0.015%
4	4.428	226	228	232	rVB5	2034	2249	0.13%	0.013%
5	4.634	261	263	269	rVB7	2591	3491	0.20%	0.020%
6	4.716	274	277	280	rBV5	2091	2489	0.14%	0.014%
7	5.340	380	383	385	rBV4	1774	2001	0.11%	0.011%
8	5.658	435	437	438	rBV2	2315	1894	0.11%	0.011%
9	6.228	532	534	539	rVB5	2182	2593	0.15%	0.015%
10	6.716	613	617	619	rBV4	1564	2048	0.12%	0.012%
11	6.899	643	648	651	rVV7	1820	3216	0.18%	0.018%
12	6.922	651	652	656	rVB4	2146	2278	0.13%	0.013%
13	7.010	661	667	686	rBV	286512	541043	30.70%	3.076%
14	7.193	692	698	711	rBV	234739	379583	21.54%	2.158%
15	7.363	720	727	747	rBV	328411	568315	32.25%	3.231%
16	7.734	787	790	793	rVB5	2159	2698	0.15%	0.015%
17	7.769	793	796	799	rBV4	1427	2272	0.13%	0.013%
18	7.840	801	808	822	rBV	188619	330637	18.76%	1.880%
19	8.081	845	849	851	rBV6	1753	2176	0.12%	0.012%
20	8.422	902	907	911	rBV7	1237	1817	0.10%	0.010%
21	8.569	925	932	952	rVV	340105	663996	37.68%	3.776%
22	8.699	952	954	956	rVB3	2365	2167	0.12%	0.012%
23	8.822	972	975	977	rBV4	2196	2567	0.15%	0.015%
24	9.052	1006	1014	1027	rBV	293742	542582	30.79%	3.085%
25	9.352	1064	1065	1070	rVB4	2008	2637	0.15%	0.015%
26	9.404	1070	1074	1079	rBV8	1688	3213	0.18%	0.018%
27	9.763	1127	1135	1151	rBV	270488	500459	28.40%	2.846%
28	9.993	1170	1174	1177	rVB6	1228	2039	0.12%	0.012%
29	10.040	1178	1182	1185	rBV5	1376	1920	0.11%	0.011%
30	10.293	1218	1225	1252	rBV	303616	693729	39.36%	3.945%
31	10.557	1268	1270	1272	rVB3	2571	2083	0.12%	0.012%
32	10.663	1281	1288	1298	rBV	257554	446840	25.36%	2.541%
33	10.846	1311	1319	1343	rBV	277925	645941	36.65%	3.673%
34	11.063	1354	1356	1361	rVB6	1225	1903	0.11%	0.011%
35	11.440	1415	1420	1422	rBV5	1770	2822	0.16%	0.016%
36	11.475	1424	1426	1429	rBV4	2138	2974	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018116.D
 Acq On : 12 Nov 2023 22:16
 Operator : MA/JU
 Sample : PB156806BL
 Misc :
 ALS Vial : 97 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK806

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	11.504	1429	1431	1436	rVV6	1608	2602	0.15%	0.015%
38	11.569	1436	1442	1445	rVB7	2183	3665	0.21%	0.021%
39	11.769	1473	1476	1481	rVB7	1633	2631	0.15%	0.015%
40	12.181	1543	1546	1548	rBV4	1407	1828	0.10%	0.010%
41	12.298	1558	1566	1571	rBV10	4153	9682	0.55%	0.055%
42	12.704	1634	1635	1640	rVB5	1549	2002	0.11%	0.011%
43	13.081	1696	1699	1702	rVB5	2076	2601	0.15%	0.015%
44	13.116	1702	1705	1706	rBV3	2173	2131	0.12%	0.012%
45	13.357	1741	1746	1753	rBV8	6671	11339	0.64%	0.064%
46	13.657	1794	1797	1799	rBV4	1422	1775	0.10%	0.010%
47	13.728	1804	1809	1812	rBV7	1614	2656	0.15%	0.015%
48	13.804	1820	1822	1825	rVB4	1526	1792	0.10%	0.010%
49	13.940	1839	1845	1859	rBV	625734	951475	53.99%	5.410%
50	14.040	1861	1862	1867	rVB5	1671	2179	0.12%	0.012%
51	14.140	1876	1879	1881	rBV4	1663	2006	0.11%	0.011%
52	14.216	1885	1892	1904	rBV	727182	1070149	60.72%	6.085%
53	14.516	1935	1943	1954	rBV	377030	562787	31.93%	3.200%
54	14.804	1984	1992	2017	rBV2	88798	359803	20.42%	2.046%
55	15.151	2049	2051	2054	rVB4	2479	2113	0.12%	0.012%
56	15.392	2089	2092	2093	rBV3	1823	2093	0.12%	0.012%
57	15.522	2107	2114	2127	rBV	850268	1308635	74.26%	7.441%
58	15.681	2135	2141	2153	rBV	209986	366189	20.78%	2.082%
59	15.881	2173	2175	2179	rVB5	2129	2191	0.12%	0.012%
60	16.310	2244	2248	2251	rBV6	1838	3347	0.19%	0.019%
61	16.416	2263	2266	2268	rBV4	2136	2488	0.14%	0.014%
62	16.516	2280	2283	2285	rBV4	2008	2253	0.13%	0.013%
63	16.551	2285	2289	2293	rVV7	2913	3709	0.21%	0.021%
64	16.634	2300	2303	2305	rBV4	1776	1818	0.10%	0.010%
65	16.710	2315	2316	2321	rVB5	2326	3084	0.17%	0.018%
66	17.216	2399	2402	2405	rBV5	1307	1874	0.11%	0.011%
67	17.298	2410	2416	2427	rBV	466803	671346	38.09%	3.817%
68	17.398	2427	2433	2449	rVV	952531	1423312	80.76%	8.093%
69	17.628	2470	2472	2476	rBV4	2454	2949	0.17%	0.017%
70	17.681	2480	2481	2486	rVB5	1601	1996	0.11%	0.011%
71	18.004	2534	2536	2539	rVB4	1996	1892	0.11%	0.011%
72	18.551	2627	2629	2632	rBV4	2665	2634	0.15%	0.015%
73	19.222	2740	2743	2749	rBV4	12359	18565	1.05%	0.106%
74	19.298	2752	2756	2760	rBV3	10322	17074	0.97%	0.097%
75	19.651	2810	2816	2826	rBV	1257175	1670988	94.82%	9.501%
76	21.427	3113	3118	3129	rBV	513670	748055	42.45%	4.254%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018116.D
Acq On : 12 Nov 2023 22:16
Operator : MA/JU
Sample : PB156806BL
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK806

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

77	23.763	3507	3515	3531	rVB2	827831	1762334	100.00%	10.021%
78	23.927	3537	3543	3553	rVB	358405	766419	43.49%	4.358%




Sum of corrected areas: 17586806

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018116.D
Acq On : 12 Nov 2023 22:16
Operator : MA/JU
Sample : PB156806BL
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK806

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

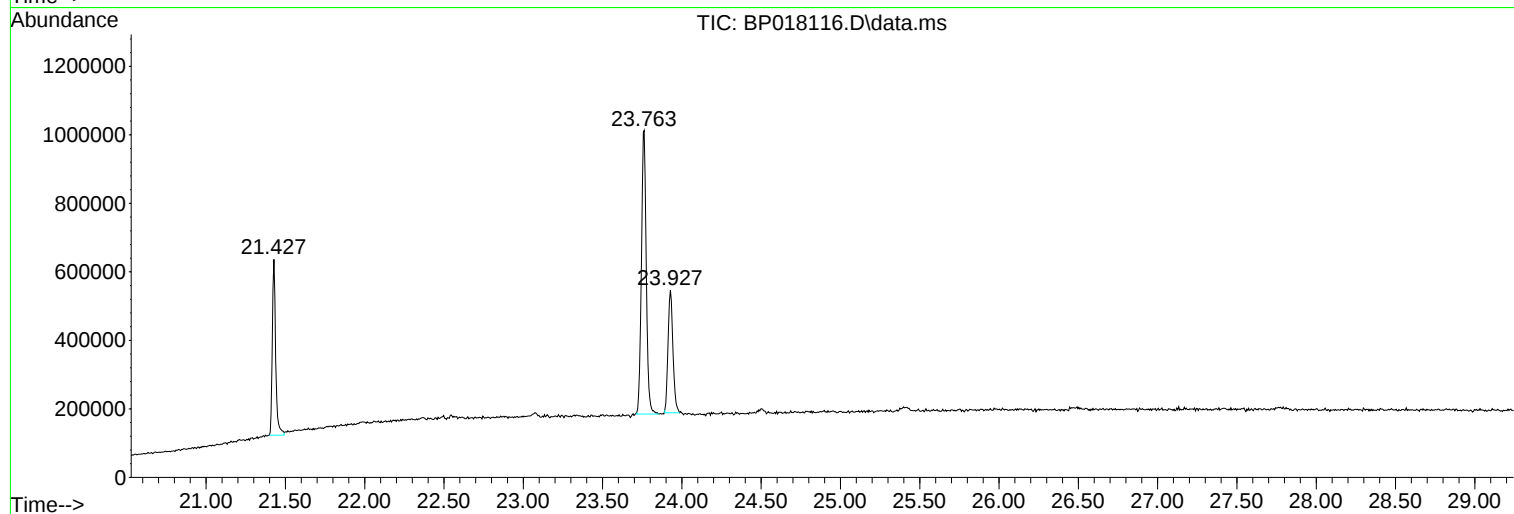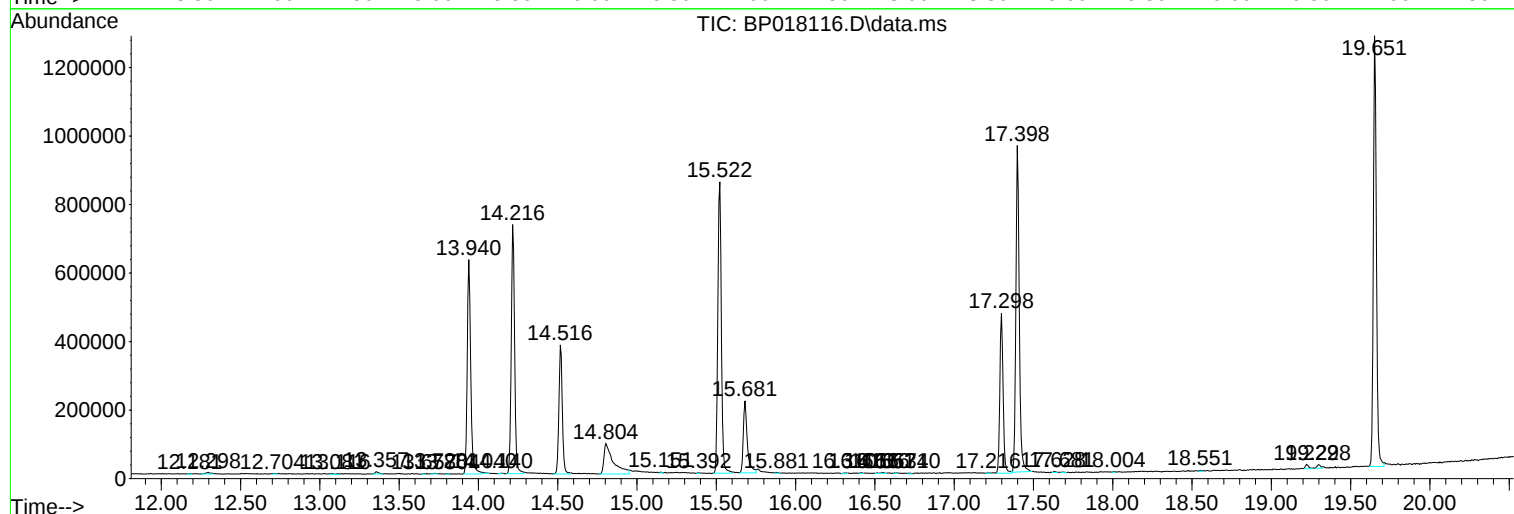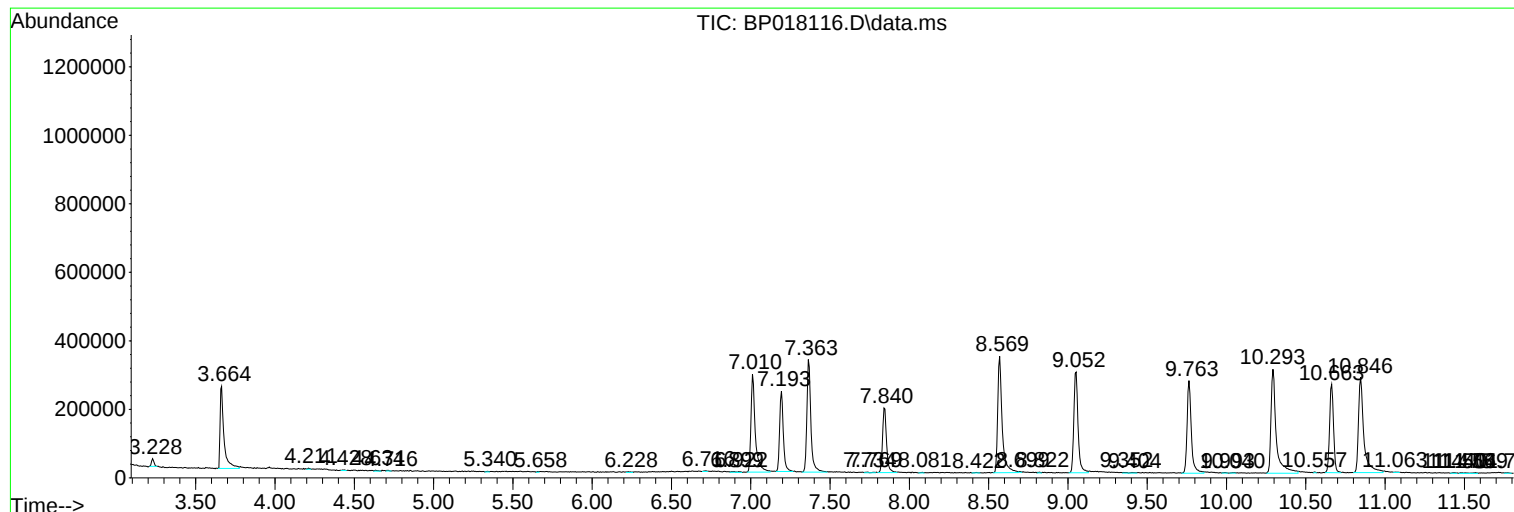

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018116.D
Acq On : 12 Nov 2023 22:16
Operator : MA/JU
Sample : PB156806BL
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK806

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018116.D
Acq On : 12 Nov 2023 22:16
Operator : MA/JU
Sample : PB156806BL
Misc :
ALS Vial : 97 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK806

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------