

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018119.D
 Acq On : 12 Nov 2023 23:58
 Operator : MA/JU
 Sample : PB156922BL
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK922

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	20	23	35	rVB	62791	85024	1.73%	0.177%
2	3.658	93	97	112	rBV	740292	1172900	23.83%	2.447%
3	3.963	145	149	155	rVB6	8867	16110	0.33%	0.034%
4	7.010	660	667	690	rBV	985889	1644799	33.42%	3.432%
5	7.193	692	698	708	rVV	775261	1162138	23.61%	2.425%
6	7.363	720	727	748	rBV	1070268	1694812	34.43%	3.536%
7	7.840	799	808	819	rBV	429403	695385	14.13%	1.451%
8	8.563	925	931	953	rBV	1189040	2030512	41.25%	4.237%
9	9.045	1006	1013	1032	rBV	980305	1683664	34.21%	3.513%
10	9.757	1127	1134	1152	rBV	908100	1569990	31.90%	3.276%
11	10.287	1217	1224	1246	rBV	1093264	2102216	42.71%	4.386%
12	10.663	1279	1288	1298	rBV	551570	927912	18.85%	1.936%
13	10.839	1308	1318	1336	rBV	1065734	2001804	40.67%	4.177%
14	11.686	1454	1462	1464	rBV8	2862	5337	0.11%	0.011%
15	12.275	1556	1562	1571	rBV4	12655	32925	0.67%	0.069%
16	13.351	1741	1745	1752	rBV4	8766	14508	0.29%	0.030%
17	13.939	1838	1845	1858	rBV	2037403	2837797	57.66%	5.921%
18	14.216	1885	1892	1908	rBV	2325471	3288947	66.82%	6.863%
19	14.516	1935	1943	1954	rBV	771358	1117347	22.70%	2.331%
20	14.775	1981	1987	2003	rBV	516692	1187058	24.12%	2.477%
21	15.522	2105	2114	2129	rBV	2740285	3863067	78.49%	8.060%
22	15.675	2134	2140	2151	rVV	913165	1351186	27.45%	2.819%
23	15.757	2152	2154	2164	rVB3	19466	36226	0.74%	0.076%
24	16.098	2209	2212	2218	rVB6	4503	5872	0.12%	0.012%
25	16.957	2353	2358	2363	rBV9	5537	9123	0.19%	0.019%
26	17.298	2410	2416	2423	rBV	898362	1224150	24.87%	2.554%
27	17.398	2426	2433	2449	rVV	2872916	4012123	81.52%	8.371%
28	18.157	2559	2562	2565	rBV5	3155	5336	0.11%	0.011%
29	18.674	2644	2650	2651	rBV6	2938	5069	0.10%	0.011%
30	18.716	2653	2657	2659	rBV5	4218	6301	0.13%	0.013%
31	19.221	2739	2743	2748	rBV2	33663	45738	0.93%	0.095%
32	19.298	2750	2756	2760	rVV	26700	39936	0.81%	0.083%
33	19.651	2810	2816	2826	rBV	3469627	4445620	90.32%	9.276%
34	21.427	3113	3118	3128	rBV	940501	1292199	26.25%	2.696%
35	23.762	3507	3515	3531	rVB2	2440123	4921936	100.00%	10.270%
36	23.927	3536	3543	3557	rVB	626905	1391295	28.27%	2.903%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018119.D
Acq On : 12 Nov 2023 23:58
Operator : MA/JU
Sample : PB156922BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK922

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 47926362

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018119.D
Acq On : 12 Nov 2023 23:58
Operator : MA/JU
Sample : PB156922BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

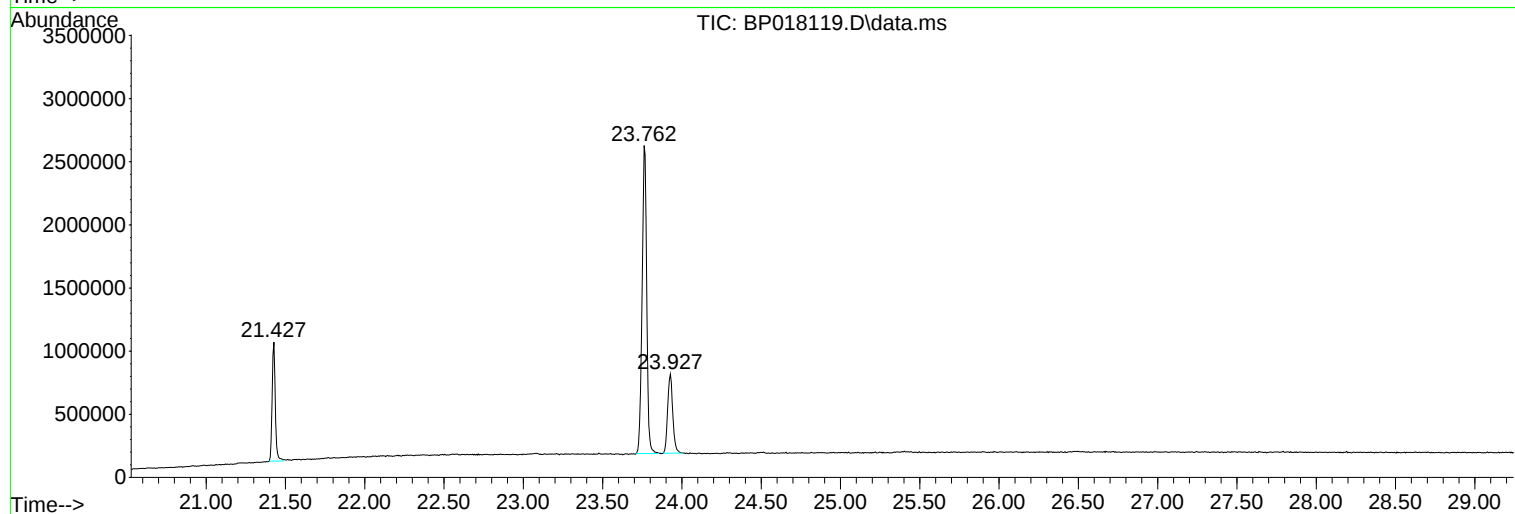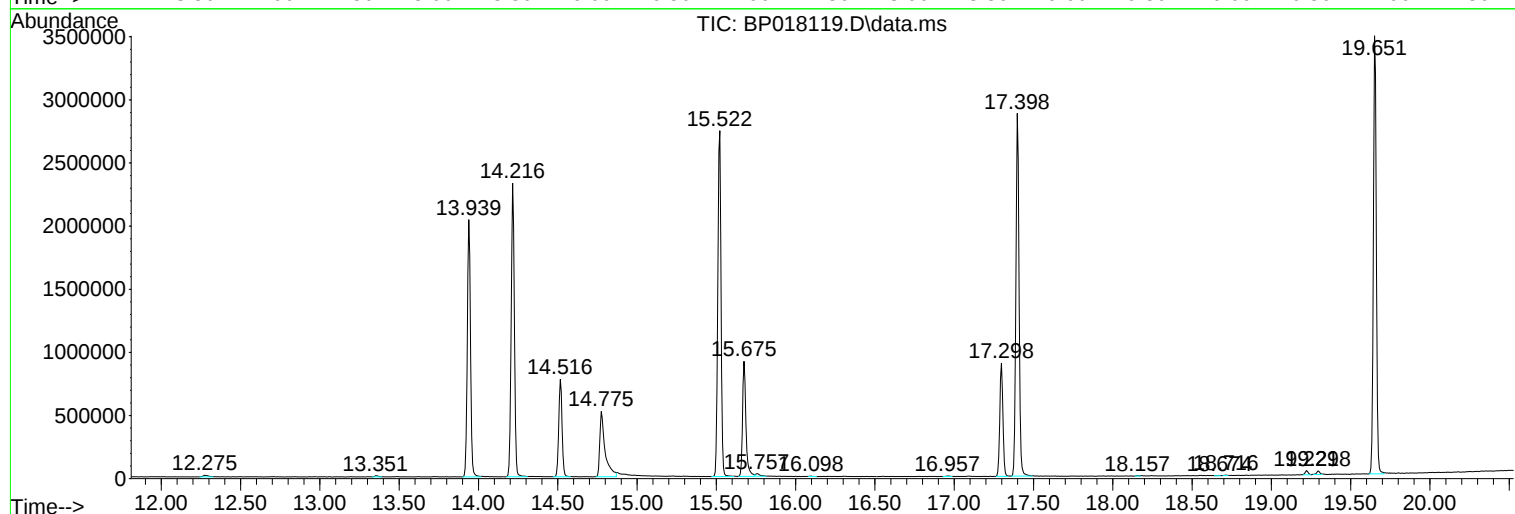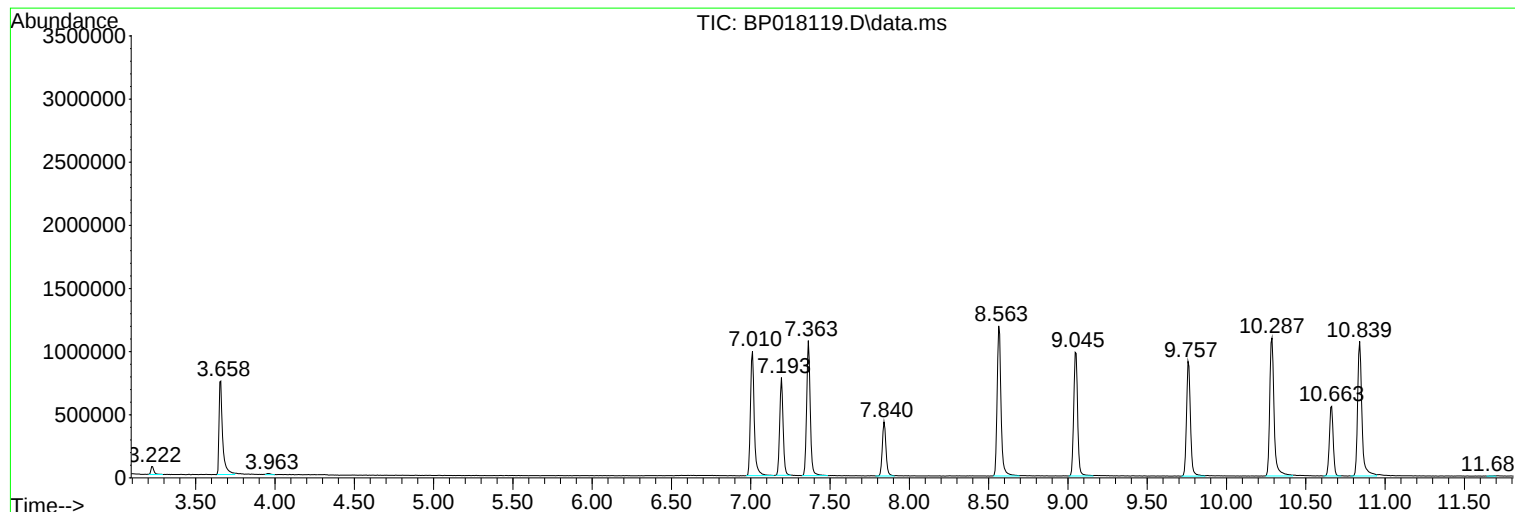

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018119.D
Acq On : 12 Nov 2023 23:58
Operator : MA/JU
Sample : PB156922BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018119.D
Acq On : 12 Nov 2023 23:58
Operator : MA/JU
Sample : PB156922BL
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK922

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------