

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018126.D
 Acq On : 13 Nov 2023 03:55
 Operator : MA/JU
 Sample : 05158-04
 Misc :
 ALS Vial : 107 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH371

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018126.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	21	24	28	rVB2	15737	16759	0.64%	0.081%
2	3.670	95	99	110	rBV	70651	124153	4.74%	0.600%
3	3.840	125	128	134	rVB4	5716	9833	0.38%	0.048%
4	3.964	145	149	155	rVB5	5974	8808	0.34%	0.043%
5	5.293	373	375	379	rVB4	2152	2660	0.10%	0.013%
6	6.187	524	527	530	rVB5	2203	2798	0.11%	0.014%
7	6.328	548	551	553	rBV4	2002	2878	0.11%	0.014%
8	6.587	590	595	596	rBV5	2577	3654	0.14%	0.018%
9	7.022	661	669	686	rBV	47538	121949	4.65%	0.590%
10	7.193	692	698	711	rBV	231394	378647	14.44%	1.830%
11	7.364	721	727	744	rVV	244454	440428	16.80%	2.129%
12	7.469	744	745	751	rVB6	3432	4519	0.17%	0.022%
13	7.840	801	808	820	rBV	256488	439285	16.75%	2.124%
14	8.569	925	932	947	rBV	158681	338891	12.93%	1.638%
15	9.046	1007	1013	1026	rBV	302786	546220	20.83%	2.641%
16	9.216	1038	1042	1048	rVB	11584	18370	0.70%	0.089%
17	9.763	1128	1135	1148	rBV	252119	483719	18.45%	2.338%
18	9.946	1159	1166	1169	rVB8	2411	4953	0.19%	0.024%
19	10.122	1191	1196	1197	rVB5	2049	2636	0.10%	0.013%
20	10.293	1217	1225	1246	rBV	293032	650522	24.81%	3.145%
21	10.658	1279	1287	1299	rBV	339489	583809	22.27%	2.822%
22	10.846	1311	1319	1337	rBV	235901	551426	21.03%	2.666%
23	11.405	1409	1414	1416	rBV6	1901	2957	0.11%	0.014%
24	12.275	1556	1562	1571	rBV6	3927	10579	0.40%	0.051%
25	12.352	1571	1575	1582	rBV5	6683	18190	0.69%	0.088%
26	13.351	1740	1745	1752	rVB7	8411	16304	0.62%	0.079%
27	13.728	1801	1809	1813	rBV7	2967	6594	0.25%	0.032%
28	13.940	1839	1845	1858	rBV	765062	1124889	42.90%	5.438%
29	14.216	1885	1892	1905	rBV	789573	1168869	44.58%	5.650%
30	14.516	1935	1943	1953	rBV	500757	754145	28.76%	3.646%
31	14.598	1956	1957	1964	rVB7	3586	5138	0.20%	0.025%
32	14.840	1993	1998	2005	rBV6	14466	41715	1.59%	0.202%
33	15.251	2063	2068	2069	rBV5	3002	4057	0.15%	0.020%
34	15.298	2073	2076	2079	rVB4	2223	3124	0.12%	0.015%
35	15.516	2106	2113	2121	rBV	1062330	1543046	58.85%	7.459%
36	15.675	2135	2140	2151	rBV	350122	606134	23.12%	2.930%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
 Data File : BP018126.D
 Acq On : 13 Nov 2023 03:55
 Operator : MA/JU
 Sample : 05158-04
 Misc :
 ALS Vial : 107 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH371

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	16.010	2194	2197	2200	rVB5	2794	4012	0.15%	0.019%
38	16.251	2234	2238	2241	rBV6	1899	2906	0.11%	0.014%
39	16.792	2324	2330	2337	rBV2	10312	22286	0.85%	0.108%
40	16.963	2353	2359	2360	rBV6	2578	4055	0.15%	0.020%
41	17.181	2394	2396	2401	rVB6	2790	3544	0.14%	0.017%
42	17.298	2409	2416	2426	rBV	674848	984553	37.55%	4.759%
43	17.398	2427	2433	2450	rVB2	1308451	1933425	73.74%	9.346%
44	17.622	2469	2471	2476	rVB6	2536	3703	0.14%	0.018%
45	17.922	2519	2522	2527	rVB7	4497	7475	0.29%	0.036%
46	18.139	2555	2559	2566	rBV2	47922	72195	2.75%	0.349%
47	18.234	2573	2575	2580	rVB4	4442	5920	0.23%	0.029%
48	18.551	2626	2629	2632	rBV5	3157	4608	0.18%	0.022%
49	19.222	2739	2743	2747	rBV2	17313	23988	0.91%	0.116%
50	19.292	2752	2755	2759	rVB2	14957	19705	0.75%	0.095%
51	19.386	2767	2771	2777	rBV5	27672	40139	1.53%	0.194%
52	19.651	2810	2816	2824	rBV	1875771	2412340	92.01%	11.662%
53	21.086	3057	3060	3065	rVB6	29869	40902	1.56%	0.198%
54	21.422	3113	3117	3127	rBV	829328	1159614	44.23%	5.606%
55	23.757	3506	3514	3524	rBV2	1270032	2621908	100.00%	12.675%
56	23.927	3536	3543	3558	rVB	577104	1276297	48.68%	6.170%




Sum of corrected areas: 20686233

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018126.D
Acq On : 13 Nov 2023 03:55
Operator : MA/JU
Sample : 05158-04
Misc :
ALS Vial : 107 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

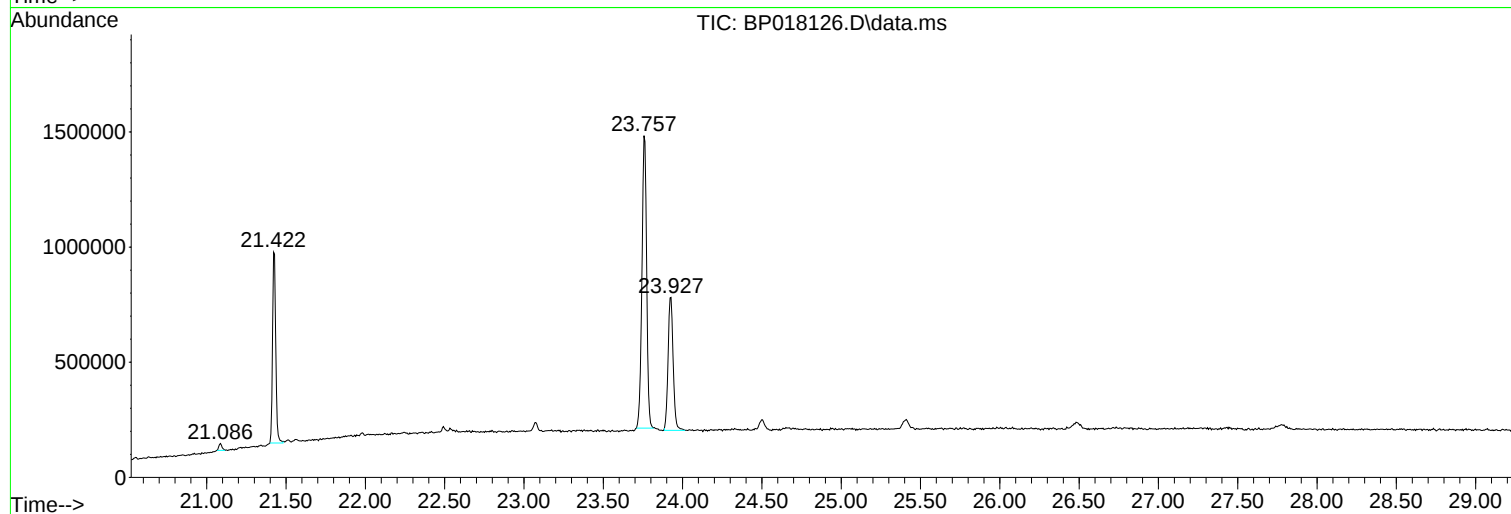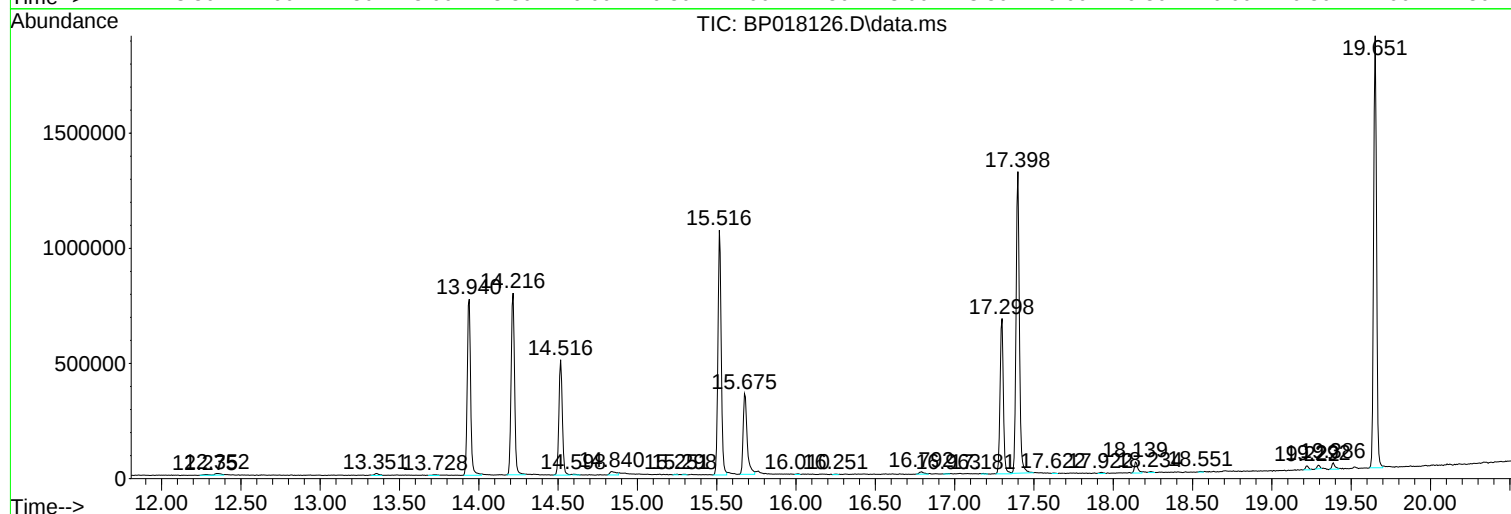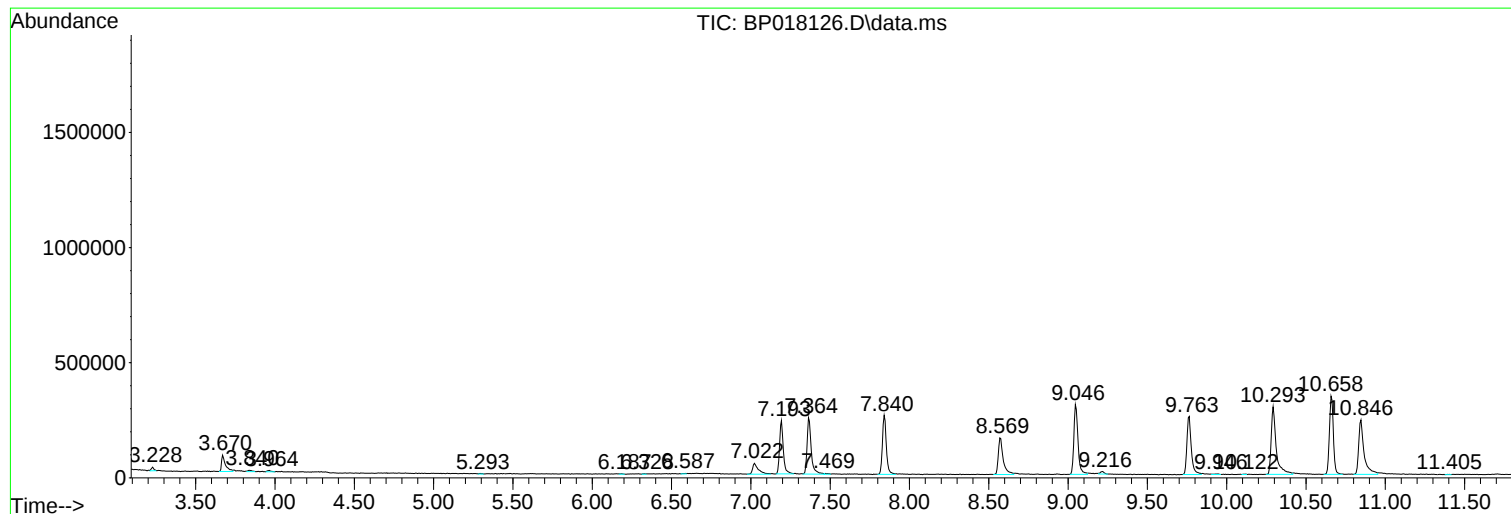

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018126.D
Acq On : 13 Nov 2023 03:55
Operator : MA/JU
Sample : 05158-04
Misc :
ALS Vial : 107 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH371










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.675	16.07 ng/ul	606134	Acenaphthene-d10	14.516

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pteridine, 4-(trifluoromethyl)-	200	C7H3F3N4	023658-17-5	38
2			N-[2-Methyl-4-pyridyl]-4-aminoph...	200	C12H12N2O	1000252-23-9	23
3			4,6-Dinitrobenzene-1,3-diol	200	C6H4N2O6	000616-74-0	16
4			Benzene, 1-methoxy-2-phenoxy-	200	C13H12O2	001695-04-1	9
5			Benzenemethanol, 3-phenoxy-	200	C13H12O2	013826-35-2	9

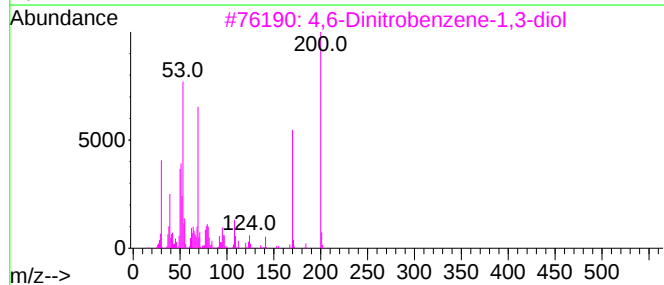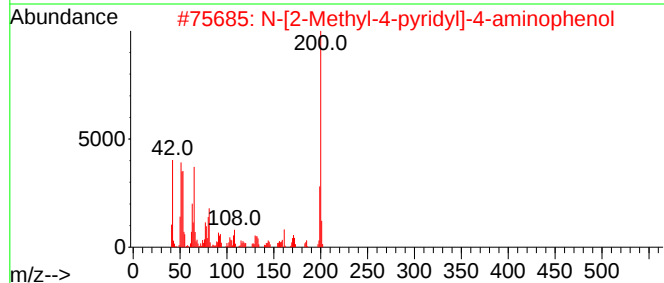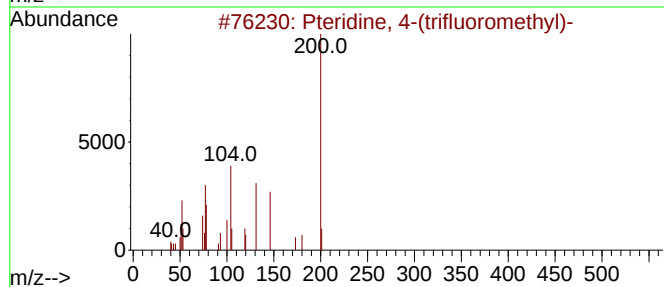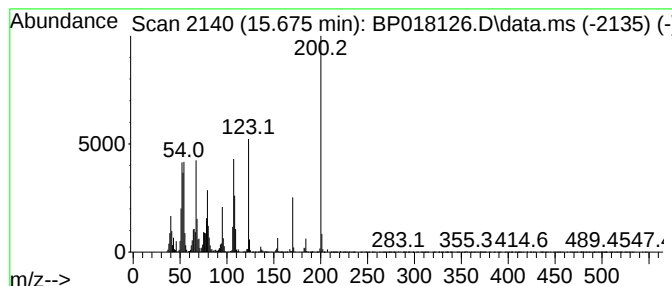

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111023\
Data File : BP018126.D
Acq On : 13 Nov 2023 03:55
Operator : MA/JU
Sample : 05158-04
Misc :
ALS Vial : 107 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	15.675	16.1	ng/ul	606134	3	14.516	754145	20.0